

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW071118\
 Data File : VW003879.D
 Acq On : 11 Jul 2018 22:17
 Operator : SY/AP
 Sample : J3881-08RE
 Misc : 4.84G/5ML/MSVOA W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SURCHARGE-SP-24RE

Quant Time: Jul 12 02:46:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070718S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 07 05:07:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	166295	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	287186	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	229667	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	75208	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	121720	55.97	ug/l	0.00
Spiked Amount 50.000			Recovery	=	111.94%	
35) Dibromofluoromethane	7.88	113	98685	49.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.20%	
50) Toluene-d8	10.33	98	337503	43.90	ug/l	0.00
Spiked Amount 50.000			Recovery	=	87.80%	
62) 4-Bromofluorobenzene	12.62	95	89019	32.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	64.00%	
Target Compounds						
20) Methylene Chloride	4.91	84	36478	16.940	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW071118\
Data File : VW003879.D
Acq On : 11 Jul 2018 22:17
Operator : SY/AP
Sample : J3881-08RE
Misc : 4.84G/5ML/MSVOA W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SURCHARGE-SP-24RE

Quant Time: Jul 12 02:46:13 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W070718S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 07 05:07:25 2018
Response via : Initial Calibration

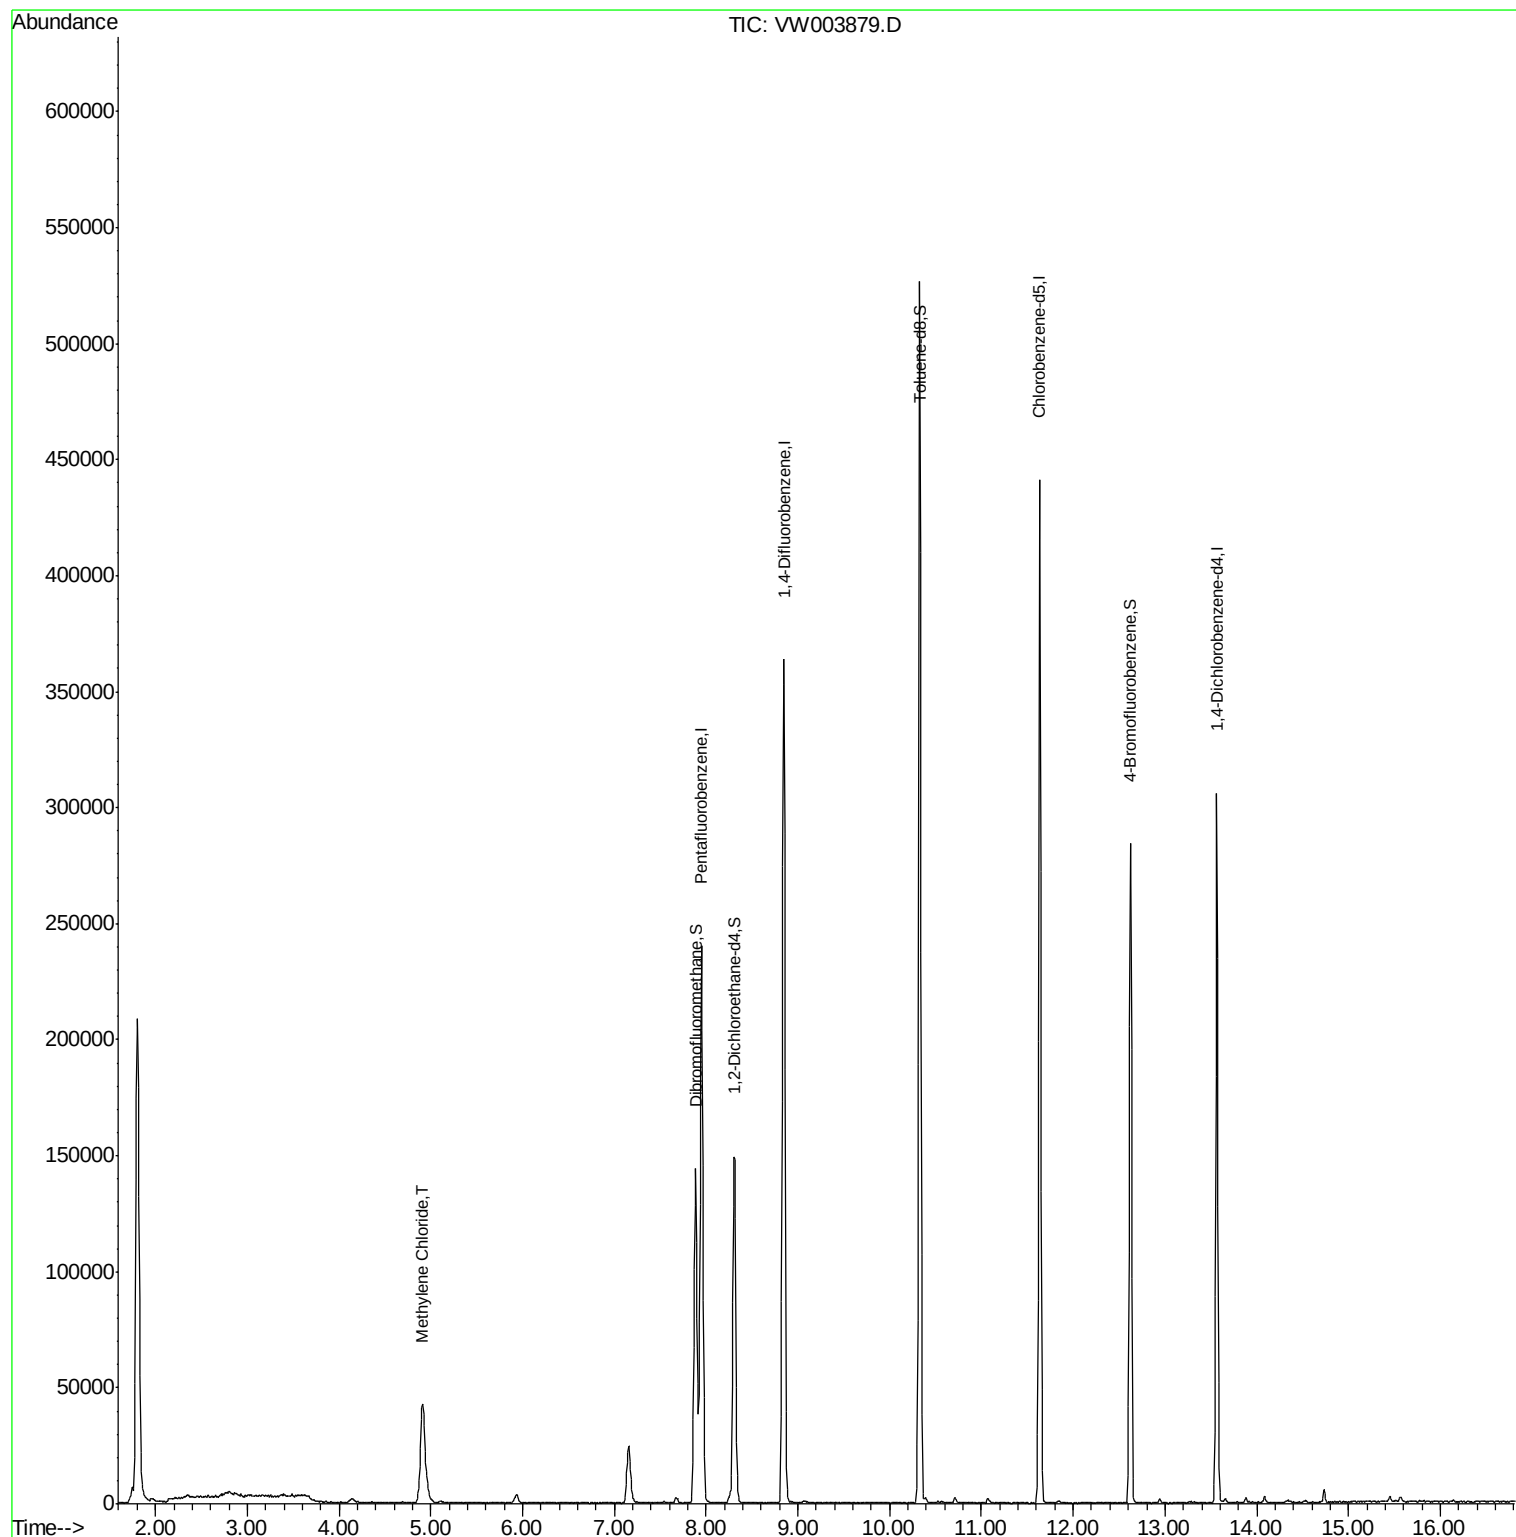

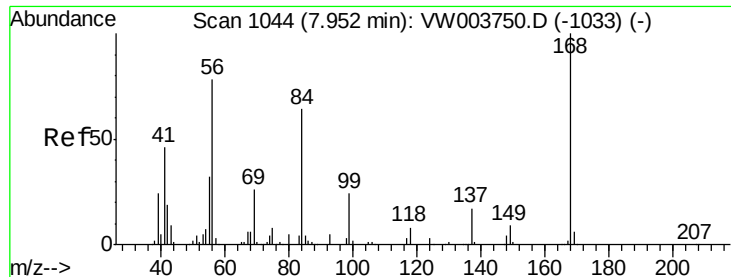

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 1044

Delta R.T. -0.00 min

Lab File: VW003879.D

Acq: 11 Jul 2018 22:17

Instrument :

MSVOA_W

ClientSampleId :


SURCHARGE-SP-24RE

Tot Ion:168 Resp: 166295

Ion Ratio Lower Upper




168 100

99 60.3 45.0 67.6

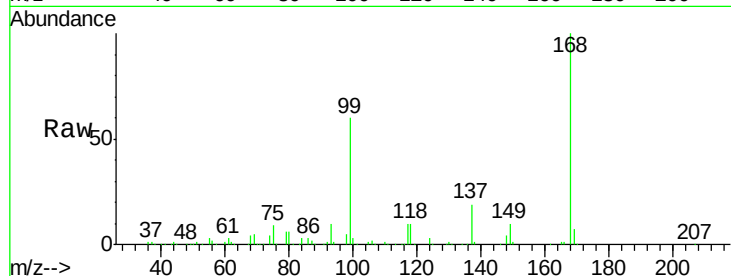

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

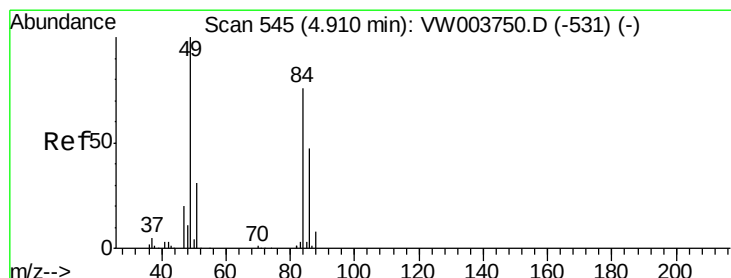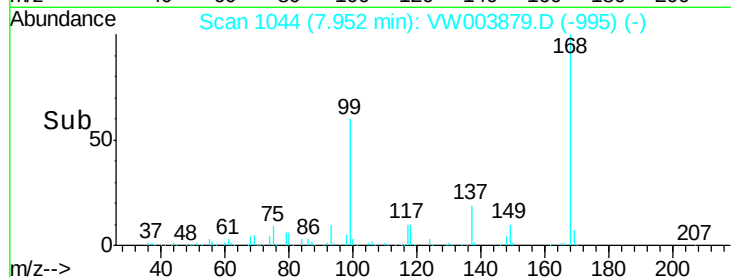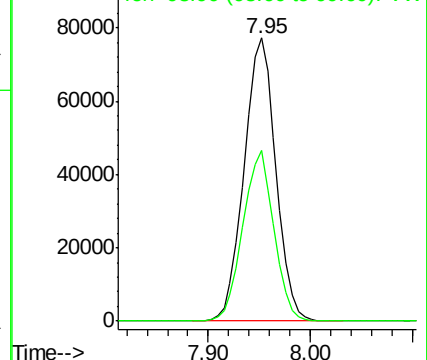

#20

Methylene Chloride

Concen: 16.940 ug/l

RT: 4.91 min Scan# 545

Delta R.T. 0.00 min

Lab File: VW003879.D

Acq: 11 Jul 2018 22:17

Tgt Ion: 84 Resp: 36478


Ion Ratio Lower Upper

84 100

49 137.5 105.1 157.7

51 41.8 32.5 48.7

86 64.9 49.8 74.6


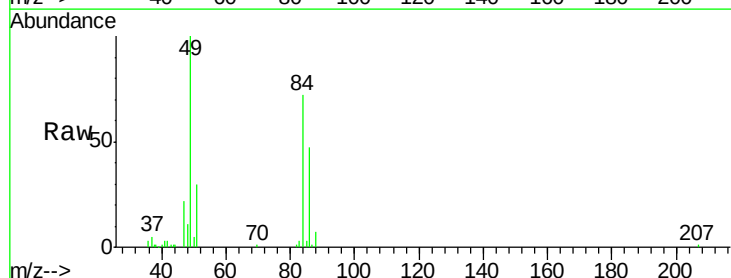



Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW



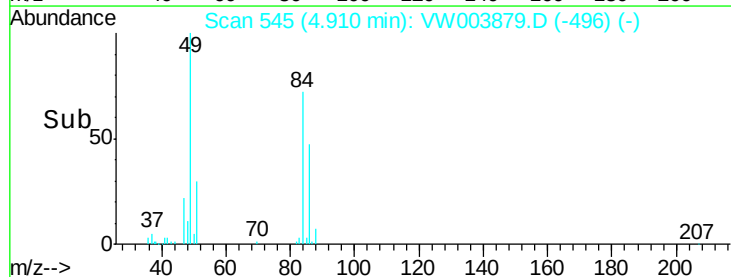
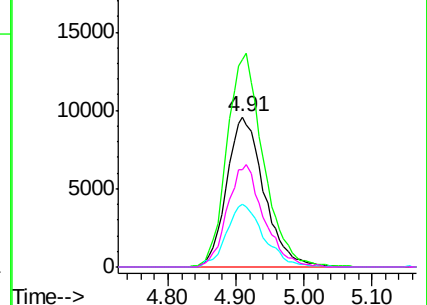


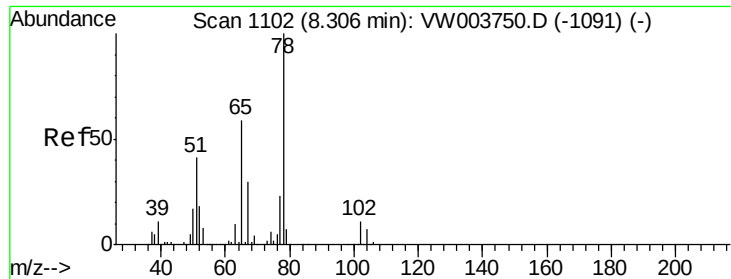

#33
 1,2-Dichloroethane-d4
 Concen: 55.971 ug/l
 RT: 8.31 min Scan# 1102
 Delta R.T. -0.00 min
 Lab File: VW003879.D
 Acq: 11 Jul 2018 22:17




Instrument :
 MSVOA_W
 ClientSampleId :
 SURCHARGE-SP-24RE


Tot Ion: 65 Resp: 121720
 Ion Ratio Lower Upper
 65 100
 67 51.2 0.0 103.8

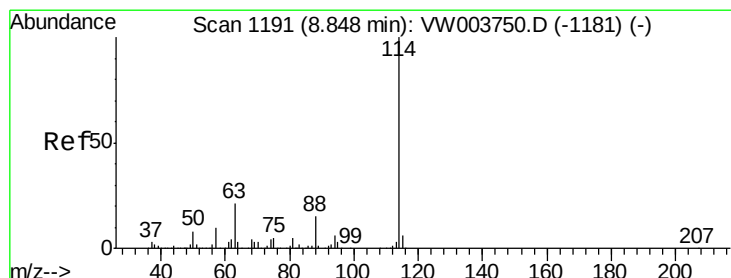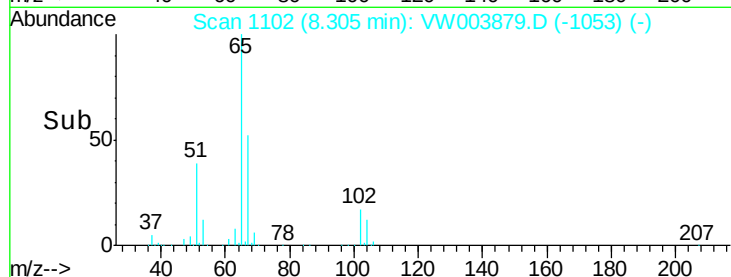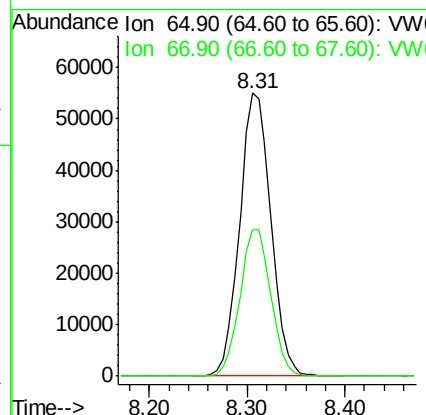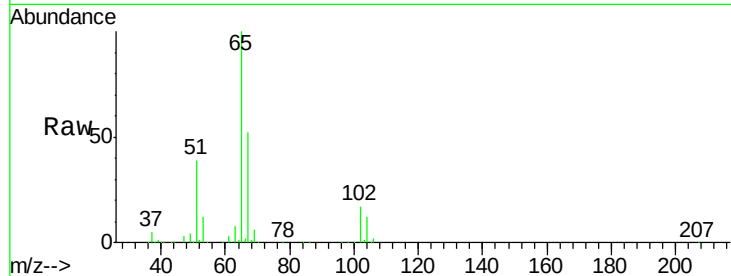

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1191
 Delta R.T. -0.00 min
 Lab File: VW003879.D
 Acq: 11 Jul 2018 22:17

Tgt Ion: 114 Resp: 287186
 Ion Ratio Lower Upper
 114 100
 63 21.6 0.0 41.8
 88 15.2 0.0 30.2

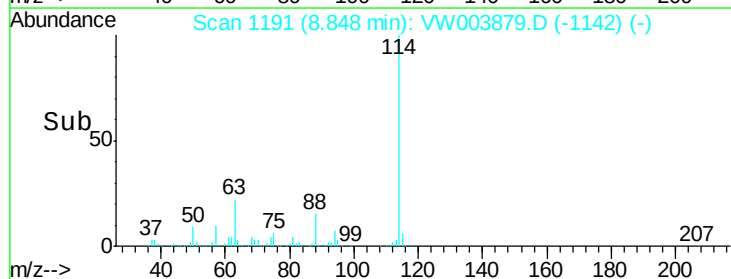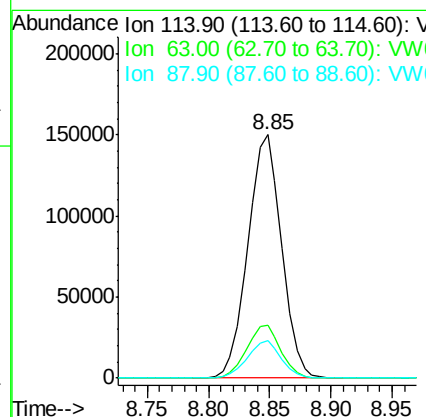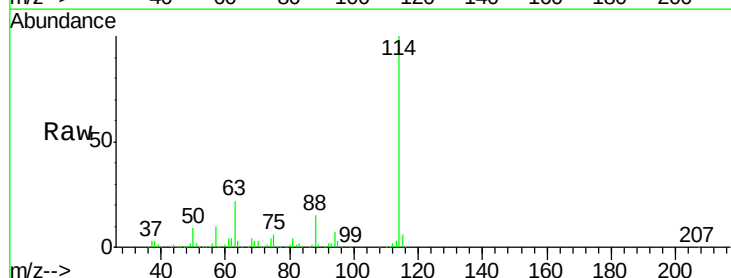


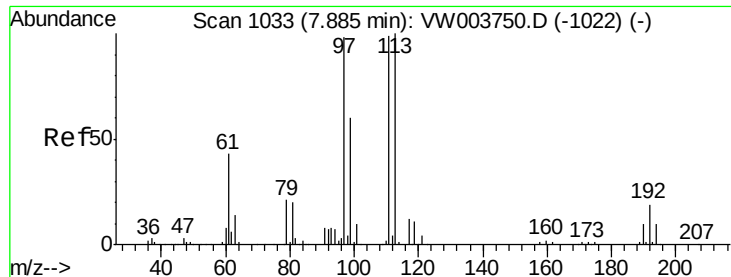




#35
Dibromofluoromethane
Concen: 49.098 ug/l
RT: 7.88 min Scan# 1033
Delta R.T. -0.00 min
Lab File: VW003879.D
Acq: 11 Jul 2018 22:17

Instrument :
MSVOA_W
ClientSampleId :
SURCHARGE-SP-24RE

Tot Ion:113 Resp: 98685
Ion Ratio Lower Upper
113 100
111 103.3 81.7 122.5
192 20.0 15.8 23.8

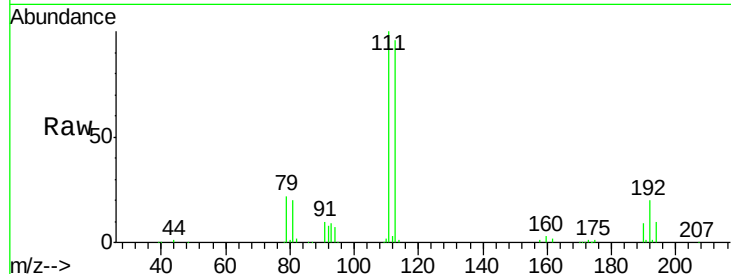


Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

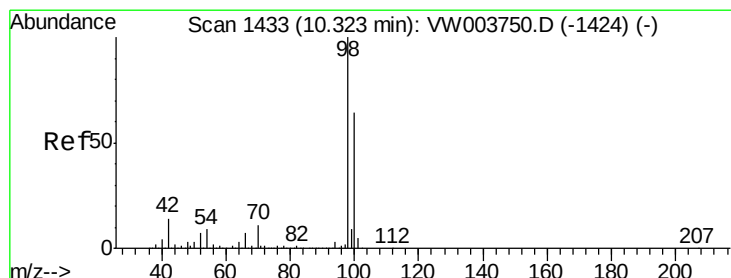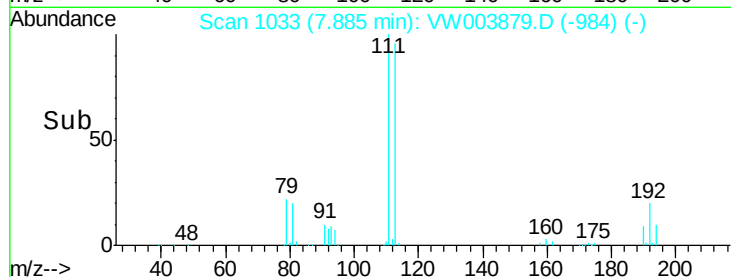
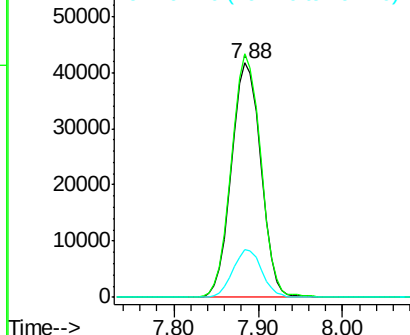



#50
Toluene-d8
Concen: 43.897 ug/l
RT: 10.33 min Scan# 1434
Delta R.T. 0.01 min
Lab File: VW003879.D
Acq: 11 Jul 2018 22:17

Tgt Ion: 98 Resp: 337503
Ion Ratio Lower Upper
98 100
100 62.3 50.8 76.2

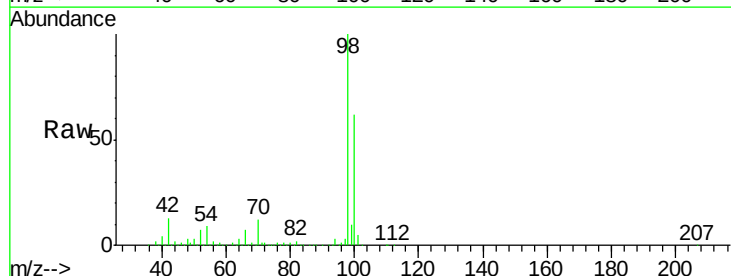

Abundance Ion 98.00 (97.70 to 98.70): VW
Ion 100.00 (99.70 to 100.70): VW

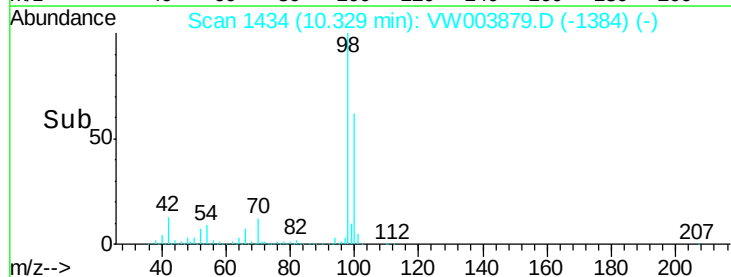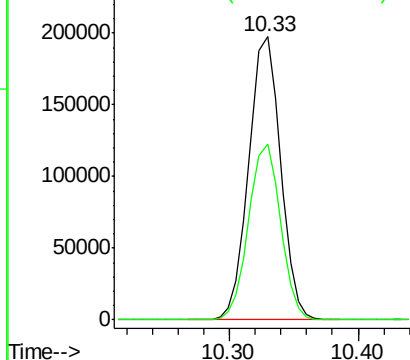

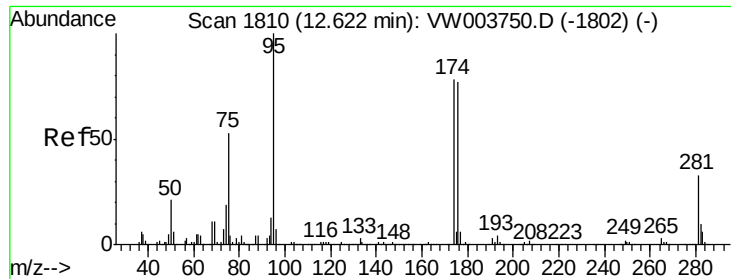

#62

4-Bromofluorobenzene

Concen: 32.000 ug/l

RT: 12.62 min Scan# 1810

Delta R.T. -0.00 min

Lab File: VW003879.D

Acq: 11 Jul 2018 22:17

Instrument :

MSVOA_W

ClientSampleId :

SURCHARGE-SP-24RE


Tot Ion: 95 Resp: 89019

Ion Ratio Lower Upper

95 100

174 80.7 0.0 163.4




176 78.1 0.0 156.8

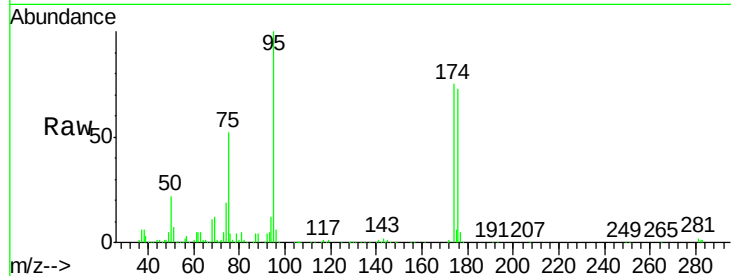

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

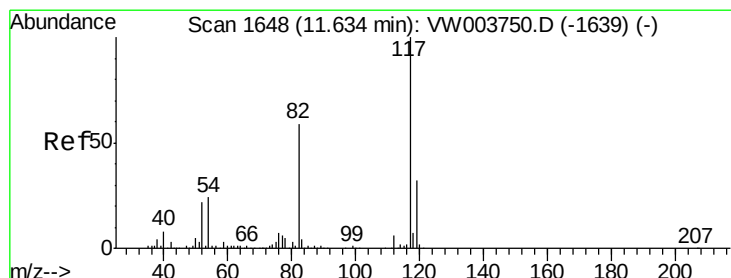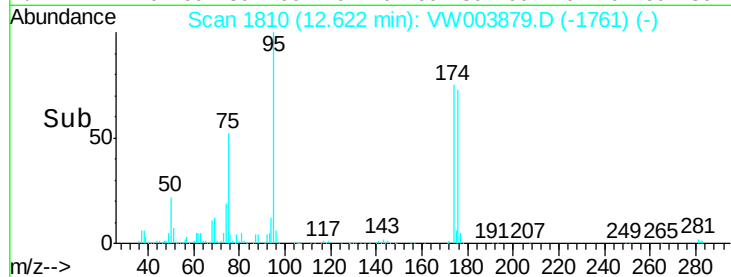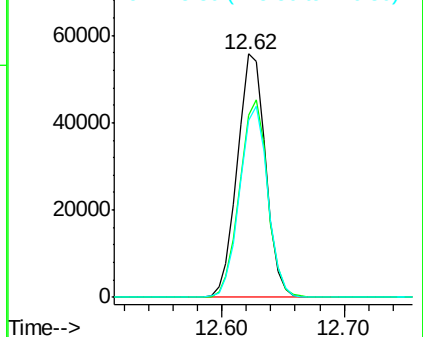

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1648

Delta R.T. -0.00 min

Lab File: VW003879.D

Acq: 11 Jul 2018 22:17


Tgt Ion: 117 Resp: 229667

Ion Ratio Lower Upper

117 100

82 58.4 46.9 70.3



119 32.0 25.5 38.3

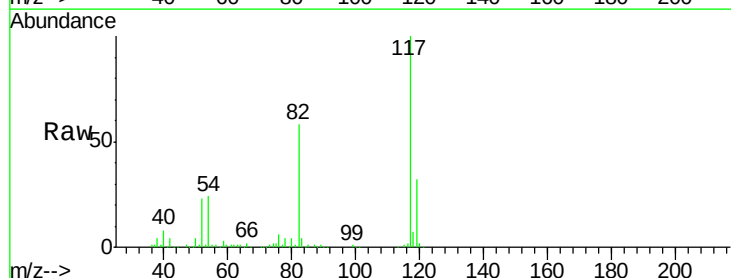


Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW

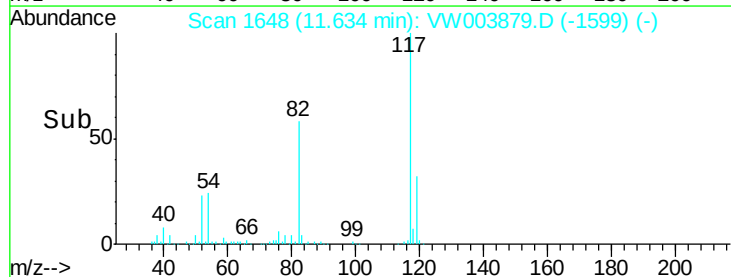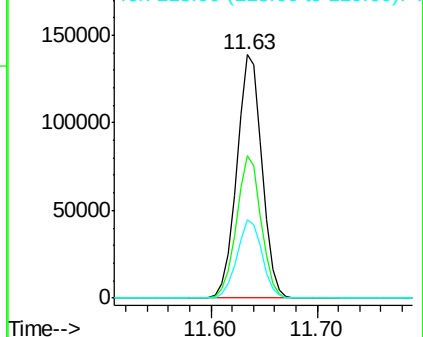

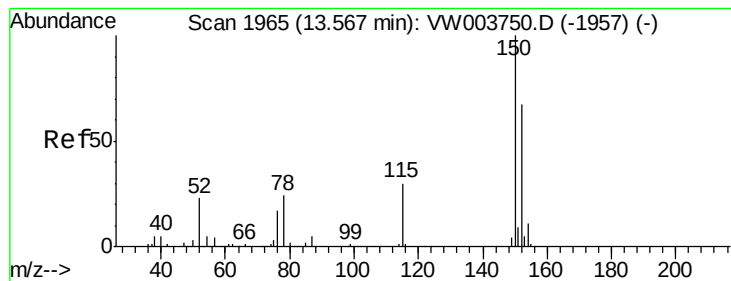

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.57 min Scan# 1965

Delta R.T. -0.00 min

Lab File: VW003879.D

Acq: 11 Jul 2018 22:17

Instrument :

MSVOA_W

ClientSampleId :

SURCHARGE-SP-24RE


Tot Ion:152 Resp: 75208

Ion Ratio Lower Upper

152 100

115 59.8 28.9 86.8

150 157.1 0.0 342.4

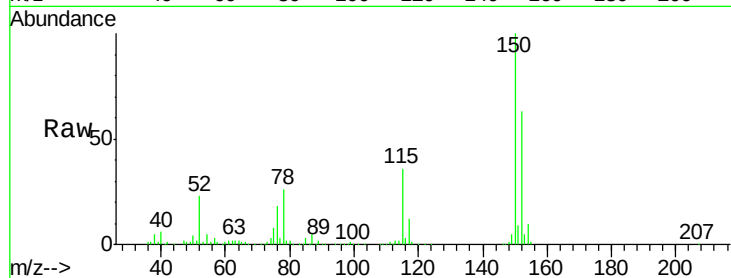

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

