


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071118\  
 Data File : VW003867.D  
 Acq On : 11 Jul 2018 11:49  
 Operator : SY/AP  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W070718S.M  
 Title : SW846 8260  
 Last Update : Sat Jul 07 05:07:25 2018

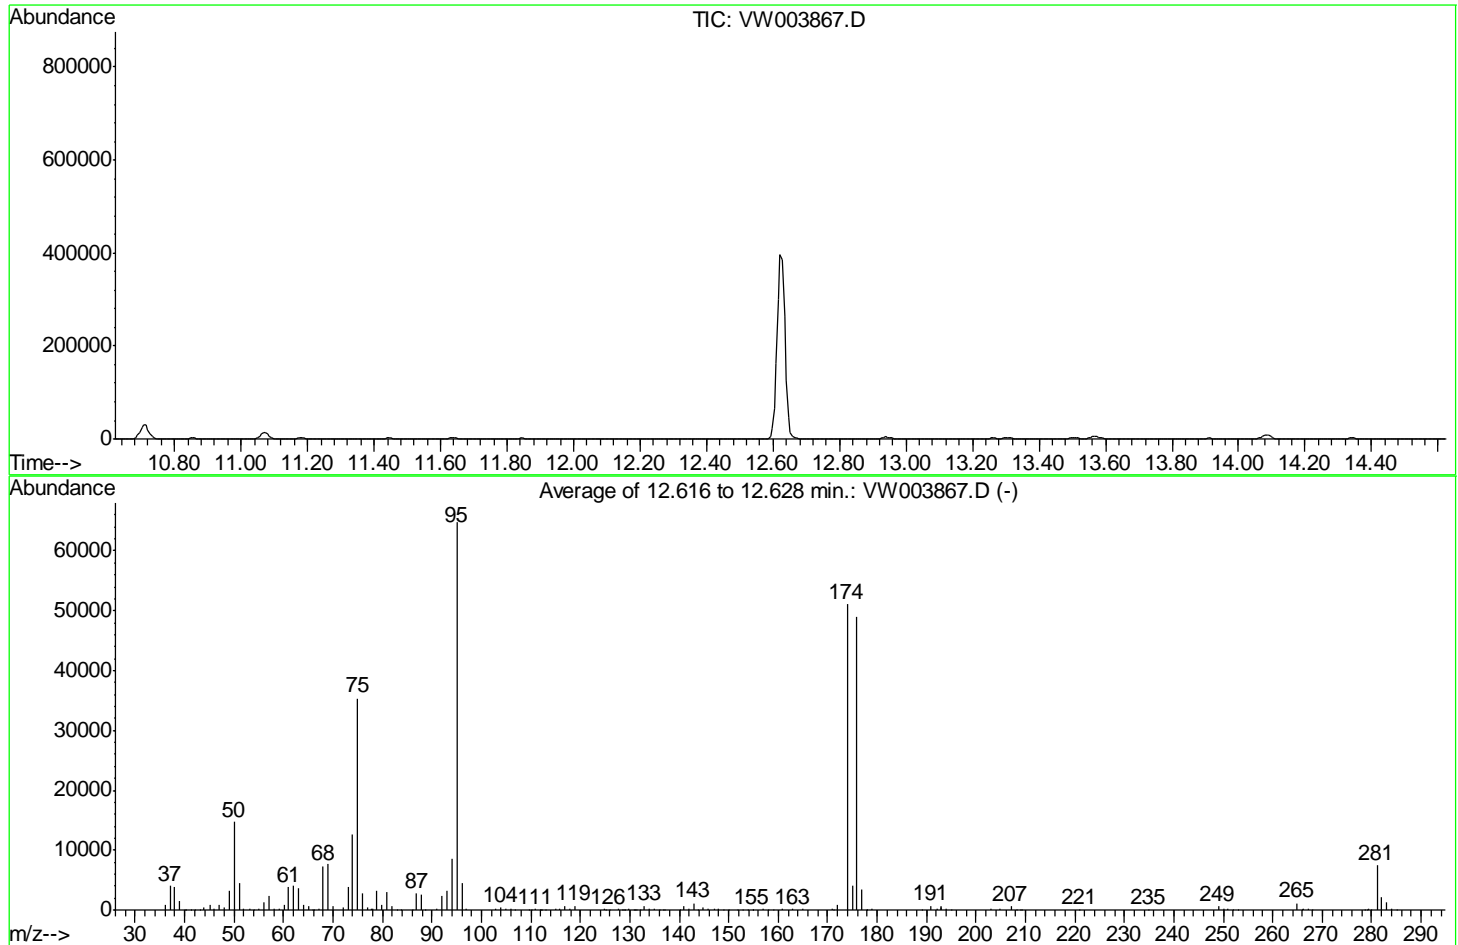

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	14706	PASS
75	95	30	60	54.6	35357	PASS
95	95	100	100	100.0	64765	PASS
96	95	5	9	7.1	4567	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.8	51040	PASS
175	174	5	9	7.9	4051	PASS
176	174	95	101	95.8	48906	PASS
177	176	5	9	6.8	3344	PASS