


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071118\
 Data File : VW003869.D
 Acq On : 11 Jul 2018 16:48
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070718S.M
 Title : SW846 8260
 Last Update : Sat Jul 07 05:07:25 2018

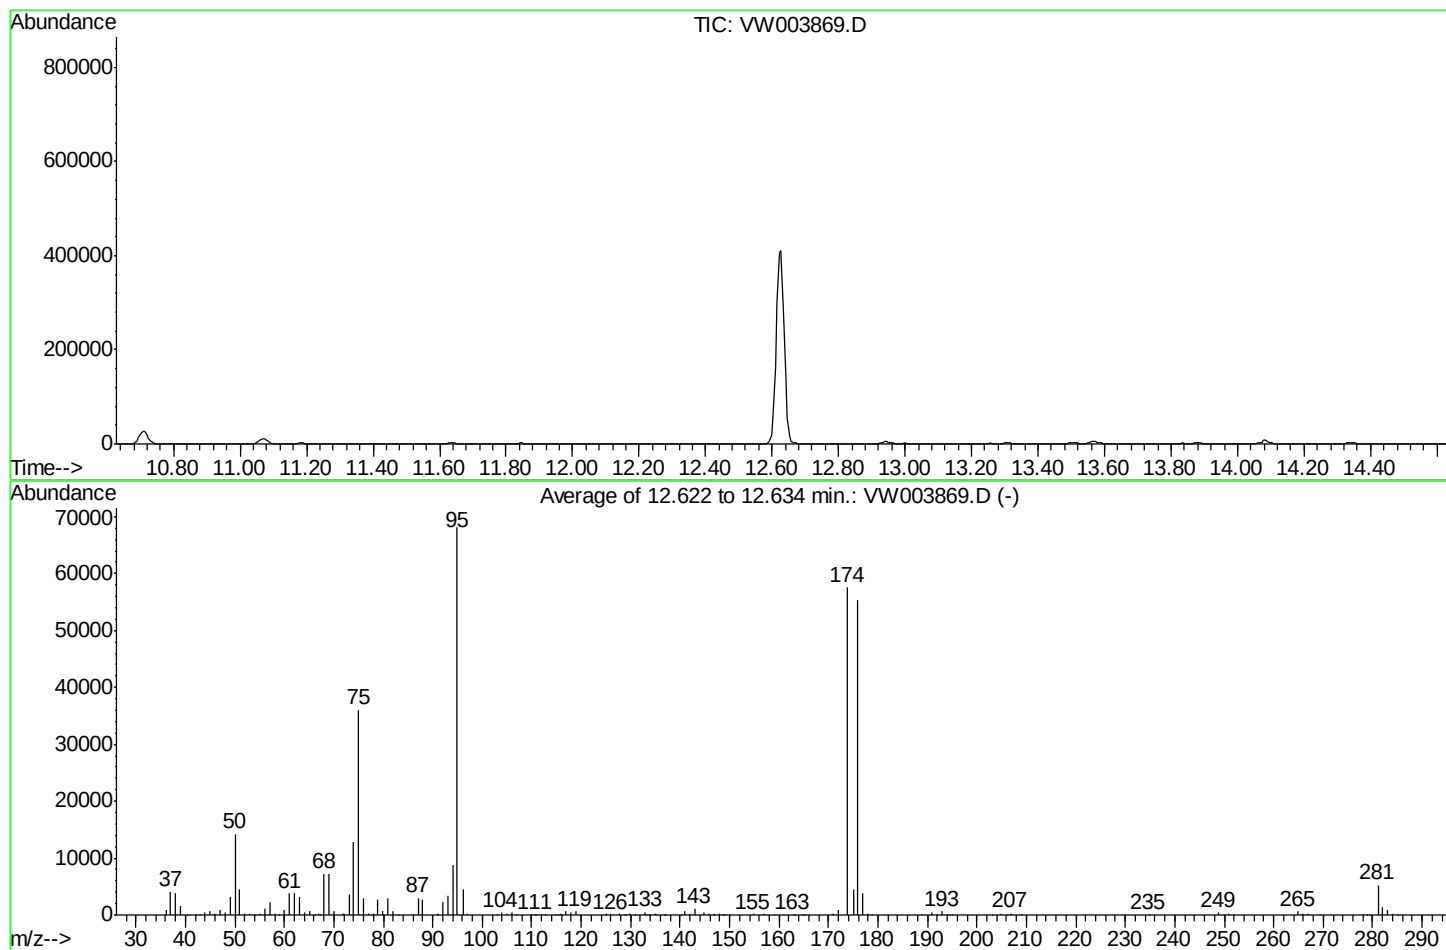

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	14266	PASS
75	95	30	60	52.9	36058	PASS
95	95	100	100	100.0	68144	PASS
96	95	5	9	6.6	4488	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.5	57586	PASS
175	174	5	9	7.9	4541	PASS
176	174	95	101	96.0	55266	PASS
177	176	5	9	6.8	3783	PASS