

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW071119\
 Data File : VW011210.D
 Acq On : 11 Jul 2019 00:57
 Operator : SY/VA
 Sample : K3751-01
 Misc : 5.56G/5ML/MSVOA W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 MANHOLE-TEST-PIT

Quant Time: Jul 11 08:47:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070819S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 11 08:14:17 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	197558	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	341679	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	293543	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	126204	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	135240	54.48	ug/l	0.00
Spiked Amount 50.000			Recovery	=	108.96%	
35) Dibromofluoromethane	7.88	113	103451	50.80	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.60%	
50) Toluene-d8	10.32	98	427480	51.93	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.86%	
62) 4-Bromofluorobenzene	12.62	95	142848	47.34	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.68%	
Target Compounds						
16) Acetone	4.12	43	47049	78.771	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW071119\
Data File : VW011210.D
Acq On : 11 Jul 2019 00:57
Operator : SY/VA
Sample : K3751-01
Misc : 5.56G/5ML/MSVOA W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
MANHOLE-TEST-PIT

Quant Time: Jul 11 08:47:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W070819S.M
Quant Title : SW846 8260
QLast Update : Thu Jul 11 08:14:17 2019
Response via : Initial Calibration

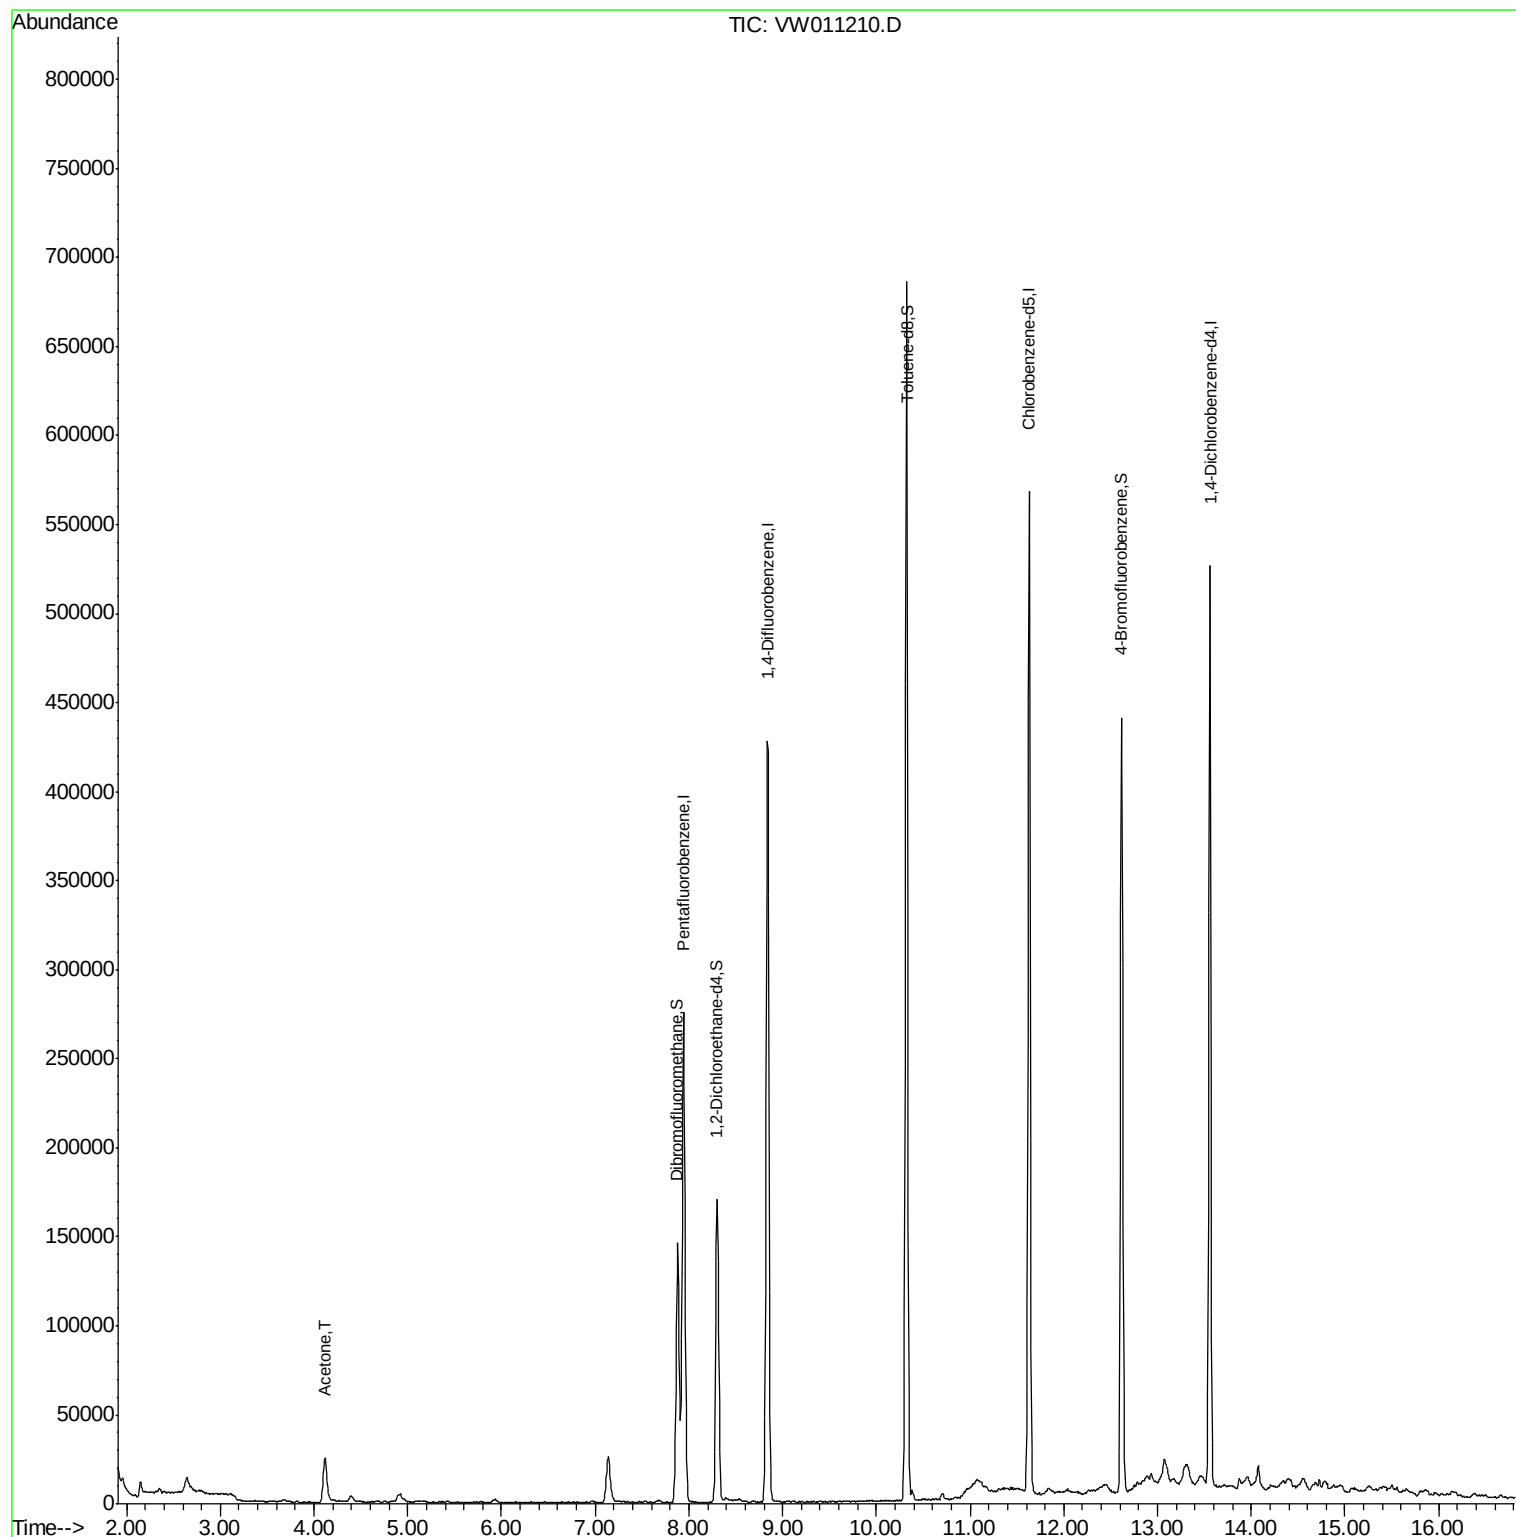

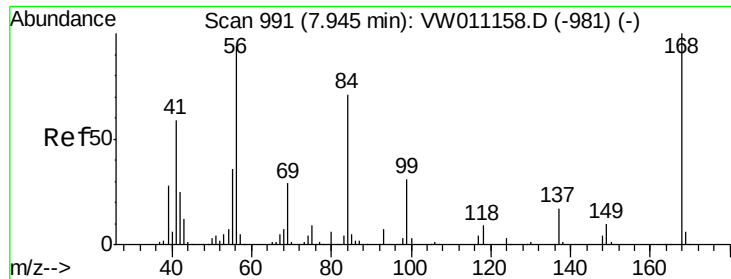

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW011210.D

Acq: 11 Jul 2019 00:57

Instrument :

MSVOA_W

ClientSampleId :


MANHOLE-TEST-PIT

Tot Ion:168 Resp: 197558

Ion Ratio Lower Upper

168 100

99 61.4 50.1 75.1

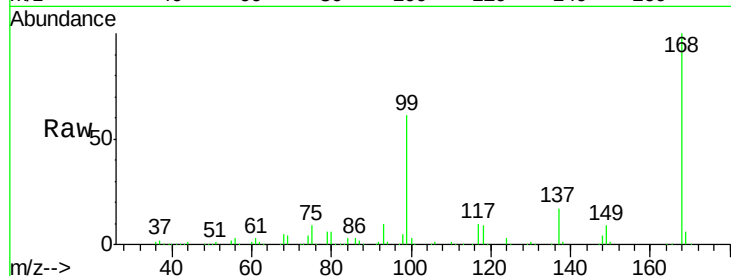

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00

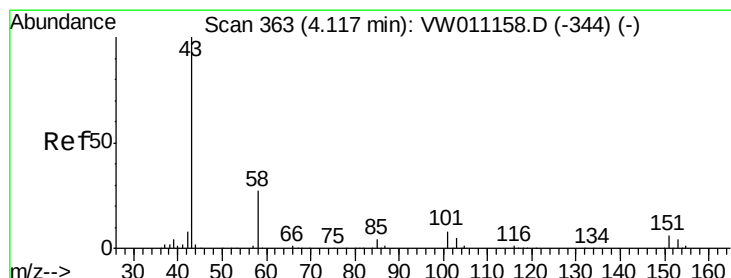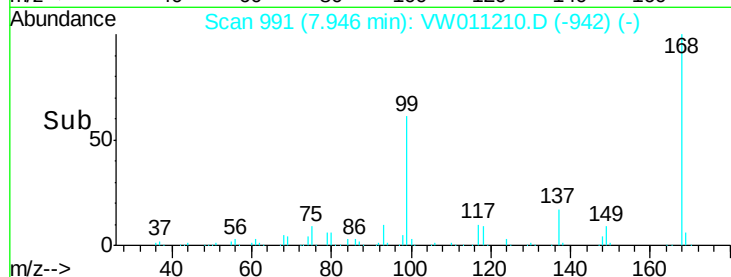

#16

Acetone

Concen: 78.771 ug/l

RT: 4.12 min Scan# 363

Delta R.T. 0.00 min

Lab File: VW011210.D


Acq: 11 Jul 2019 00:57

Tgt Ion: 43 Resp: 47049

Ion Ratio Lower Upper

43 100

58 25.3 21.8 32.6

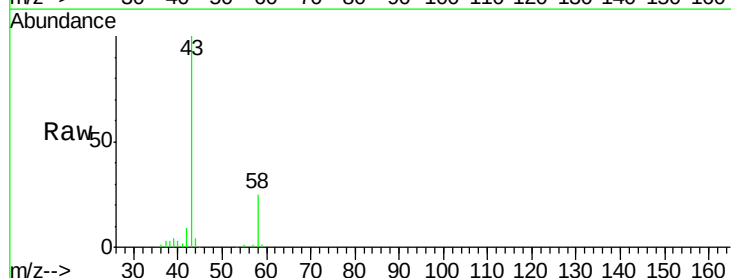

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.12


15000


10000

5000

0

Time--> 4.00 4.10 4.20

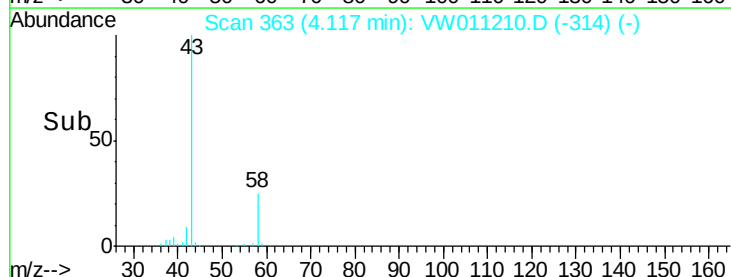

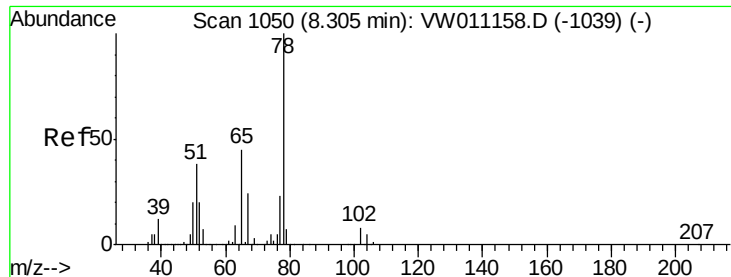

#33

1,2-Dichloroethane-d4

Concen: 54.480 ug/l

RT: 8.30 min Scan# 1049

Delta R.T. -0.01 min

Lab File: VW011210.D

Acq: 11 Jul 2019 00:57

Instrument :

MSVOA_W

ClientSampleId :





MANHOLE-TEST-PIT

Tot Ion: 65 Resp: 135240

Ion Ratio Lower Upper

65 100

67 51.8 0.0 104.4

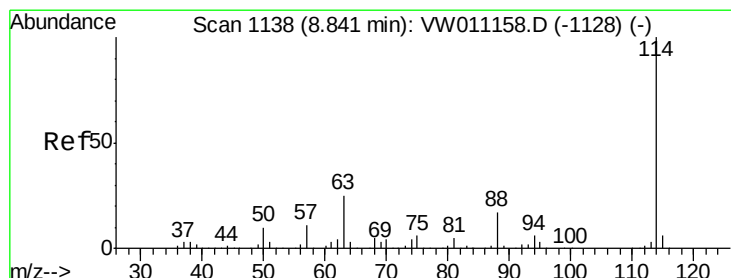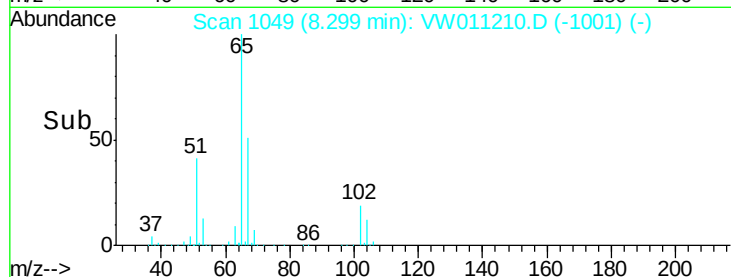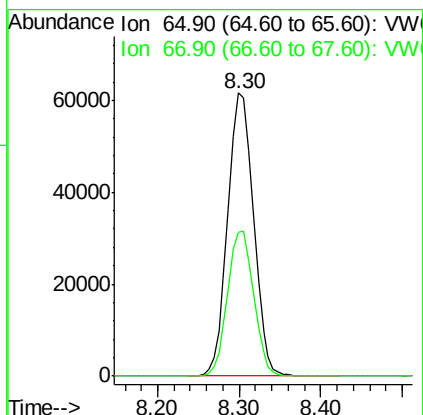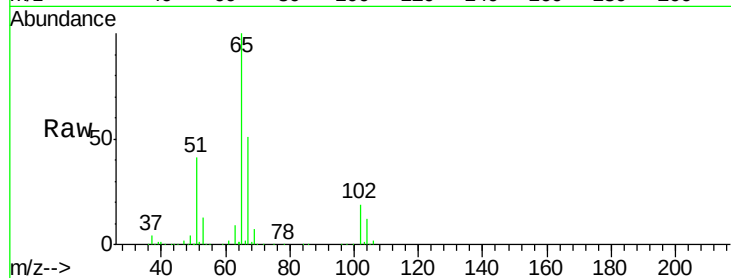

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. 0.00 min

Lab File: VW011210.D

Acq: 11 Jul 2019 00:57




Tgt Ion: 114 Resp: 341679


Ion Ratio Lower Upper

114 100

63 24.7 0.0 50.8

88 16.4 0.0 34.2


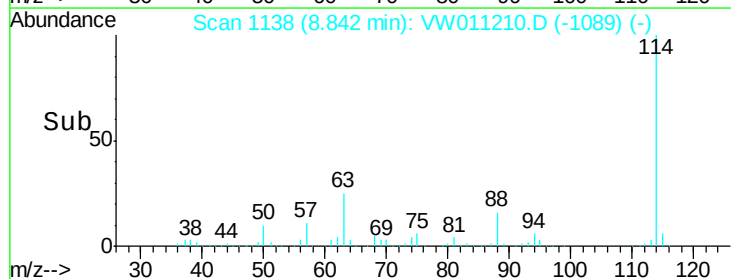
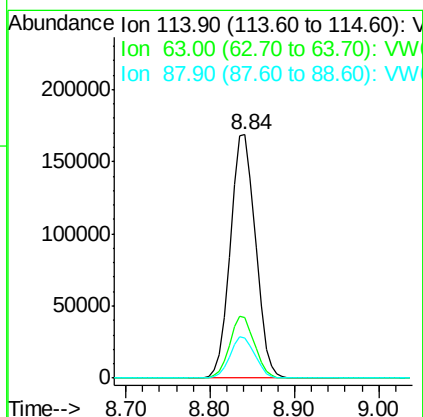
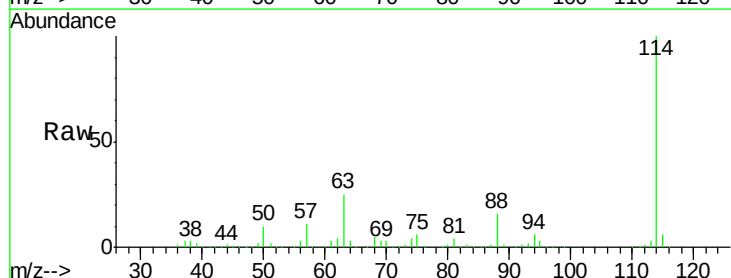


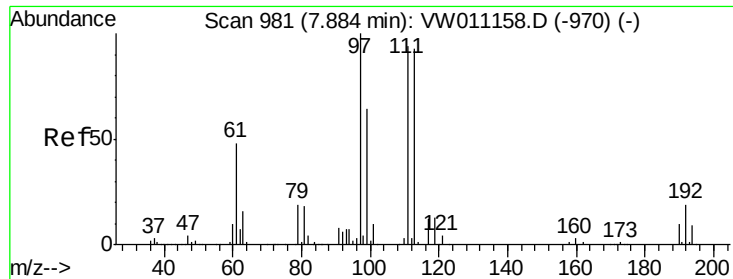

#35
 Dibromofluoromethane
 Concen: 50.797 ug/l
 RT: 7.88 min Scan# 980
 Delta R.T. -0.01 min
 Lab File: VW011210.D
 Acq: 11 Jul 2019 00:57




Instrument :
 MSVOA_W
 ClientSampleId :
 MANHOLE-TEST-PIT


Tot Ion:113 Resp: 103451
 Ion Ratio Lower Upper
 113 100
 111 102.4 82.4 123.6
 192 19.6 15.8 23.8

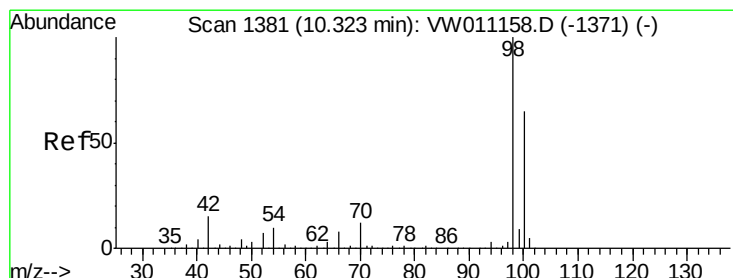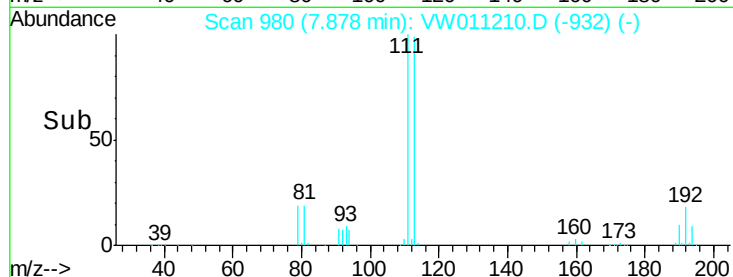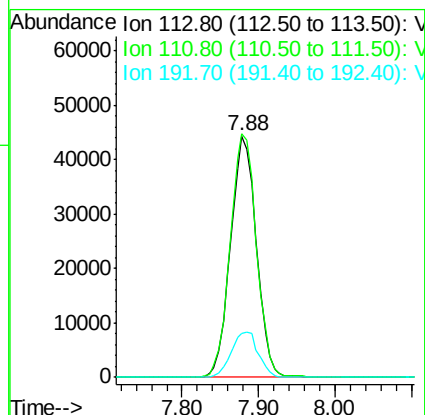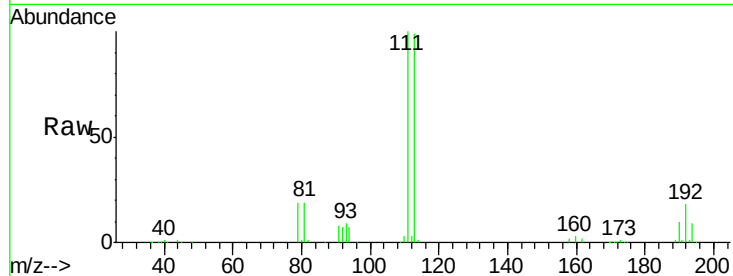

#50
 Toluene-d8
 Concen: 51.929 ug/l
 RT: 10.32 min Scan# 1381
 Delta R.T. 0.00 min
 Lab File: VW011210.D
 Acq: 11 Jul 2019 00:57

Tgt Ion: 98 Resp: 427480
 Ion Ratio Lower Upper
 98 100
 100 65.1 52.4 78.6


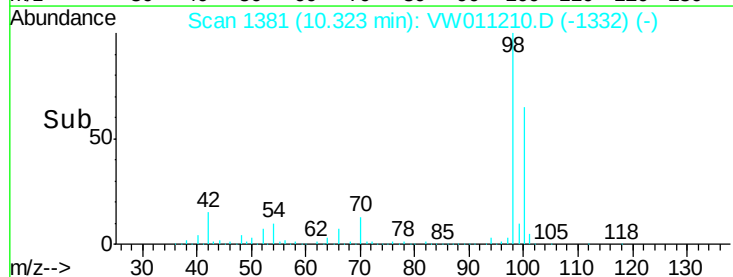
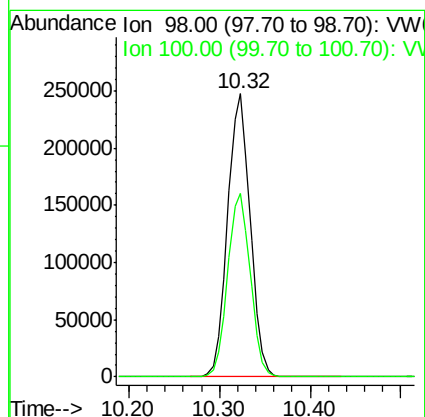
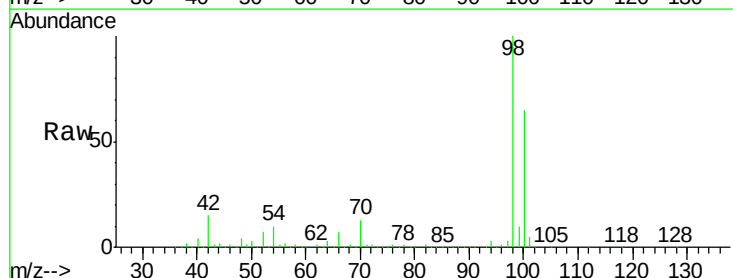


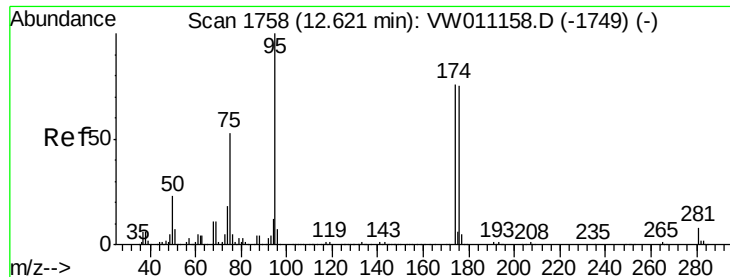

#62
4-Bromofluorobenzene
Concen: 47.342 ug/l
RT: 12.62 min Scan# 1757
Delta R.T. -0.01 min
Lab File: VW011210.D
Acq: 11 Jul 2019 00:57




Instrument :
MSVOA_W
ClientSampleId :
MANHOLE-TEST-PIT


Tot Ion: 95 Resp: 142848
Ion Ratio Lower Upper
95 100
174 76.0 0.0 147.6
176 71.9 0.0 144.6

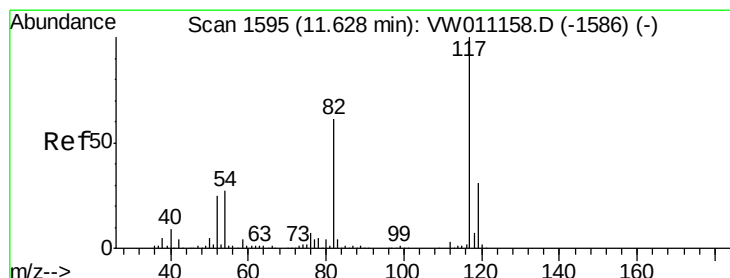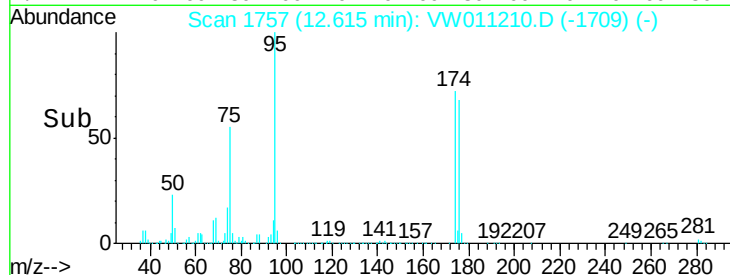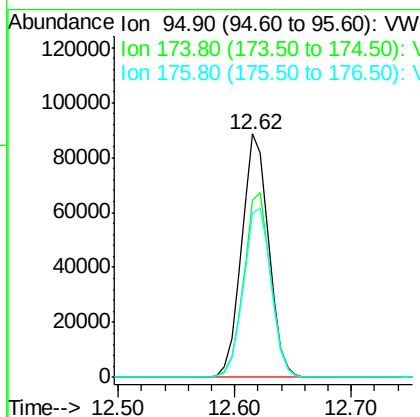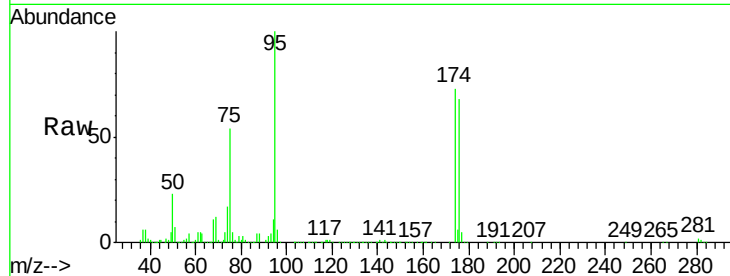

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1595
Delta R.T. 0.00 min
Lab File: VW011210.D
Acq: 11 Jul 2019 00:57

Tgt Ion: 117 Resp: 293543
Ion Ratio Lower Upper
117 100
82 64.0 48.9 73.3
119 32.1 25.0 37.6

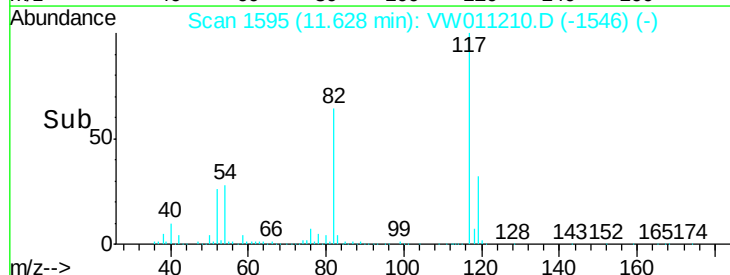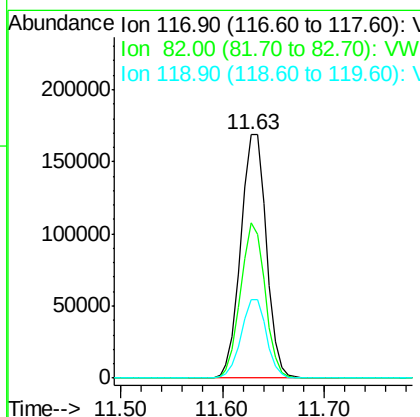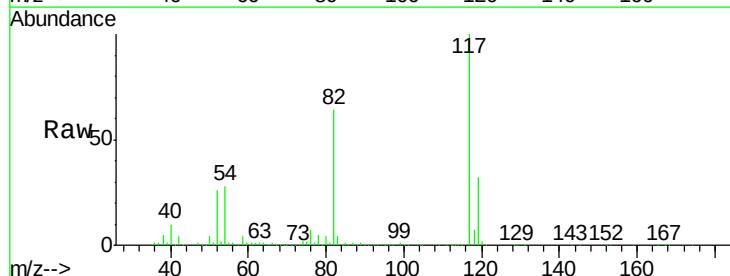

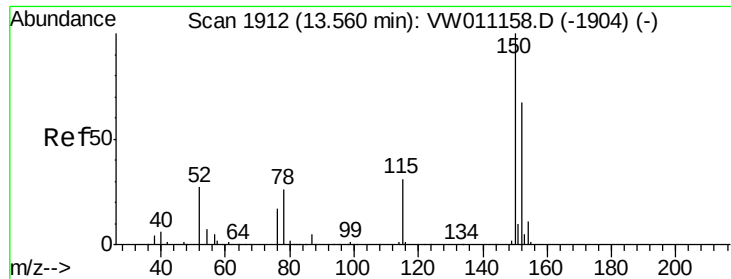

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. 0.00 min

Lab File: VW011210.D

Acq: 11 Jul 2019 00:57

Instrument :

MSVOA_W

ClientSampleId :

MANHOLE-TEST-PIT


Tot Ion:152 Resp: 126204

Ion Ratio Lower Upper

152 100

115 60.7 30.1 90.3

150 156.4 0.0 346.0

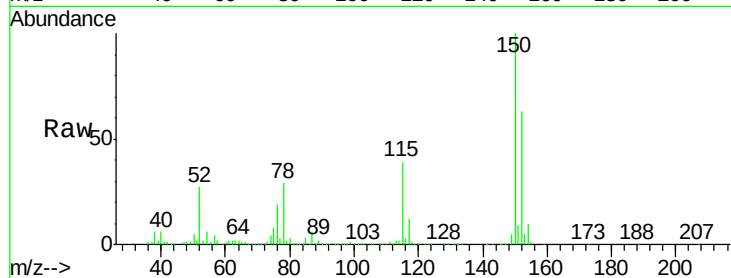

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

