


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071119\
Data File : VW011197.D
Acq On : 10 Jul 2019 17:21
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070819S.M
Title : SW846 8260
Last Update : Thu Jul 11 08:14:17 2019

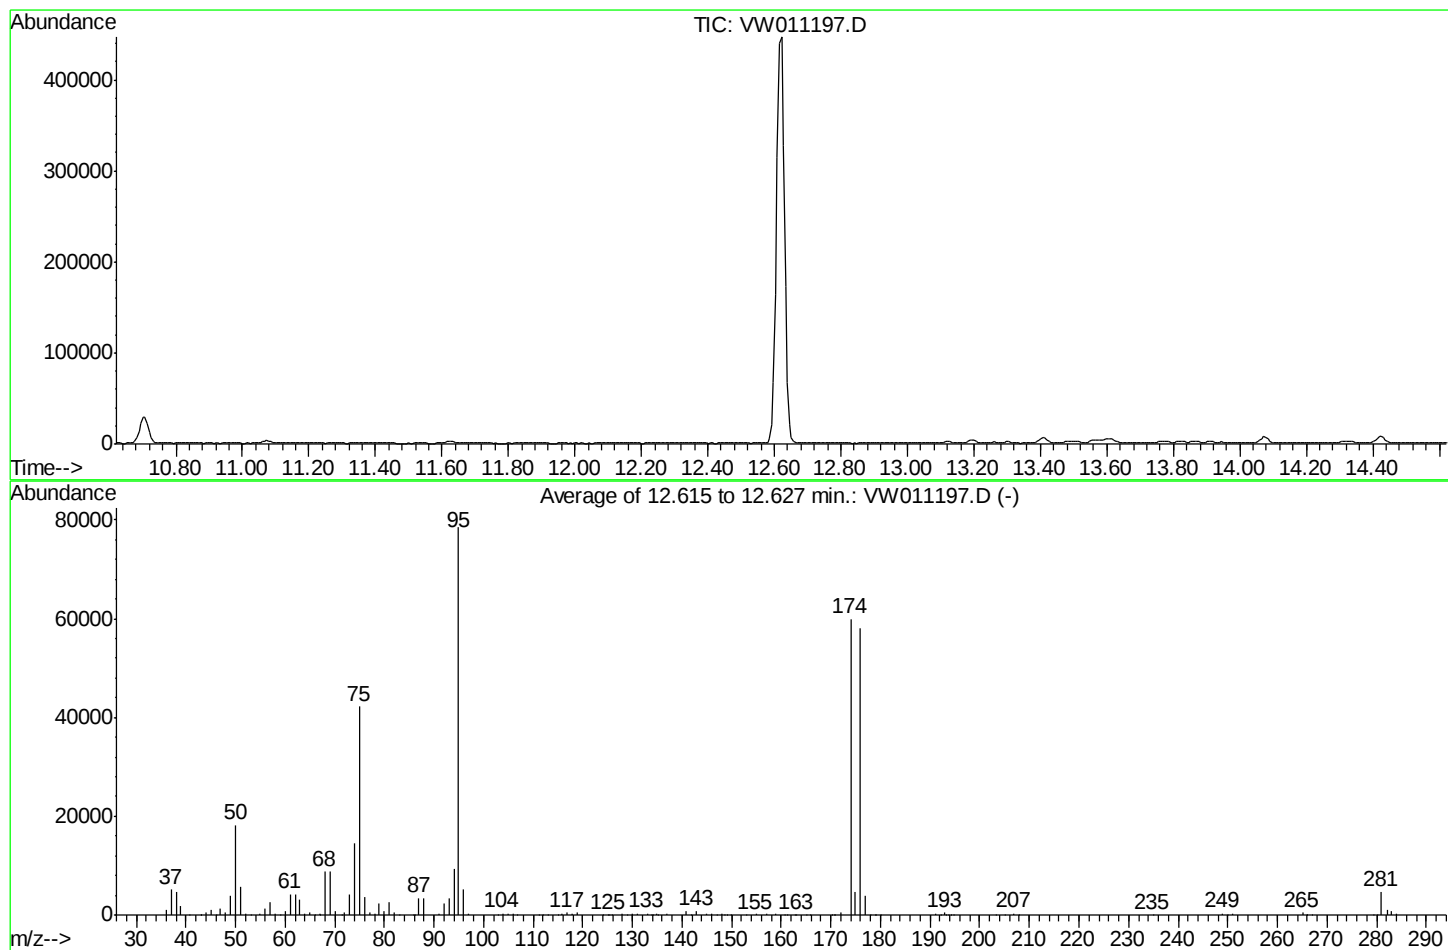

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	18168	PASS
75	95	30	60	53.7	42197	PASS
95	95	100	100	100.0	78525	PASS
96	95	5	9	6.8	5306	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.3	59938	PASS
175	174	5	9	7.7	4622	PASS
176	174	95	101	96.9	58061	PASS
177	176	5	9	6.8	3932	PASS