


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW071218\
 Data File : VW003894.D
 Acq On : 12 Jul 2018 12:50
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070718S.M
 Title : SW846 8260
 Last Update : Sat Jul 07 05:07:25 2018

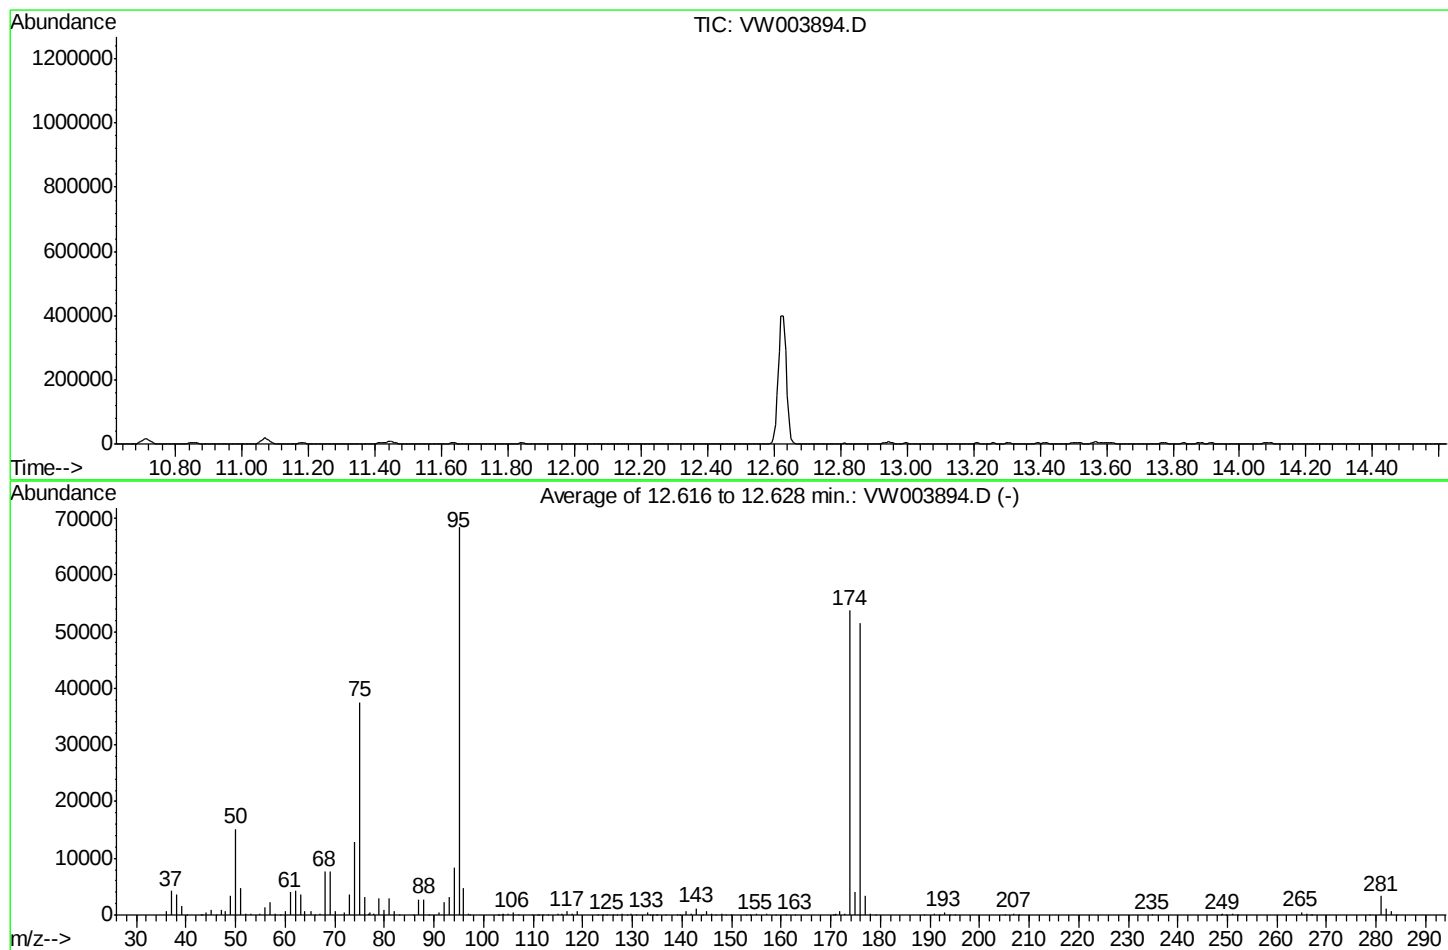

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	15198	PASS
75	95	30	60	54.8	37485	PASS
95	95	100	100	100.0	68373	PASS
96	95	5	9	6.9	4698	PASS
173	174	0.00	2	0.4	208	PASS
174	95	50	100	78.5	53698	PASS
175	174	5	9	7.6	4105	PASS
176	174	95	101	95.7	51413	PASS
177	176	5	9	6.6	3371	PASS