

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071221\
 Data File : VW019428.D
 Acq On : 12 Jul 2021 13:10
 Operator : SY/VA
 Sample : M2970-05
 Misc : 4.27G/10ML/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 13 02:22:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 13 02:19:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	384105	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	331034	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	129256	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	84843	15.590	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.360%
7) Chloroethane-d5	2.898	69	73203	18.862	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.440%
11) 1,1-Dichloroethene-d2	4.026	63	139467	13.281	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.120%
21) 2-Butanone-d5	7.080	46	57347	36.305	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.620%
24) Chloroform-d	7.653	84	212226	19.996	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.000%
26) 1,2-Dichloroethane-d4	8.311	65	114337	19.631	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.520%
32) Benzene-d6	8.281	84	422769	21.455	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.800%
36) 1,2-Dichloropropane-d6	9.275	67	132959	21.648	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.600%
41) Toluene-d8	10.329	98	364745	20.530	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.120%
43) trans-1,3-Dichloroprop...	10.579	79	44440	16.896	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.600%
47) 2-Hexanone-d5	10.927	63	41139	36.104	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.200%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	92300	18.599	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	74.400%
66) 1,2-Dichlorobenzene-d4	13.853	152	99369	21.789	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.160%
Target Compounds					Qvalue	
13) Acetone	4.123	43	78746	67.656	ug/L	90
14) Carbon disulfide	4.385	76	16063	1.000	ug/L	99
16) Methylene chloride	4.934	84	24689	3.224	ug/L	88
22) 2-Butanone	7.177	43	32994	18.320	ug/L	94
34) Trichloroethene	8.848	95	11818	2.235	ug/L #	5
37) 1,2-Dichloropropane	9.281	63	14445	2.751	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071221\
Data File : VW019428.D
Acq On : 12 Jul 2021 13:10
Operator : SY/VA
Sample : M2970-05
Misc : 4.27G/10ML/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jul 13 02:22:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 13 02:19:34 2021
Response via : Initial Calibration




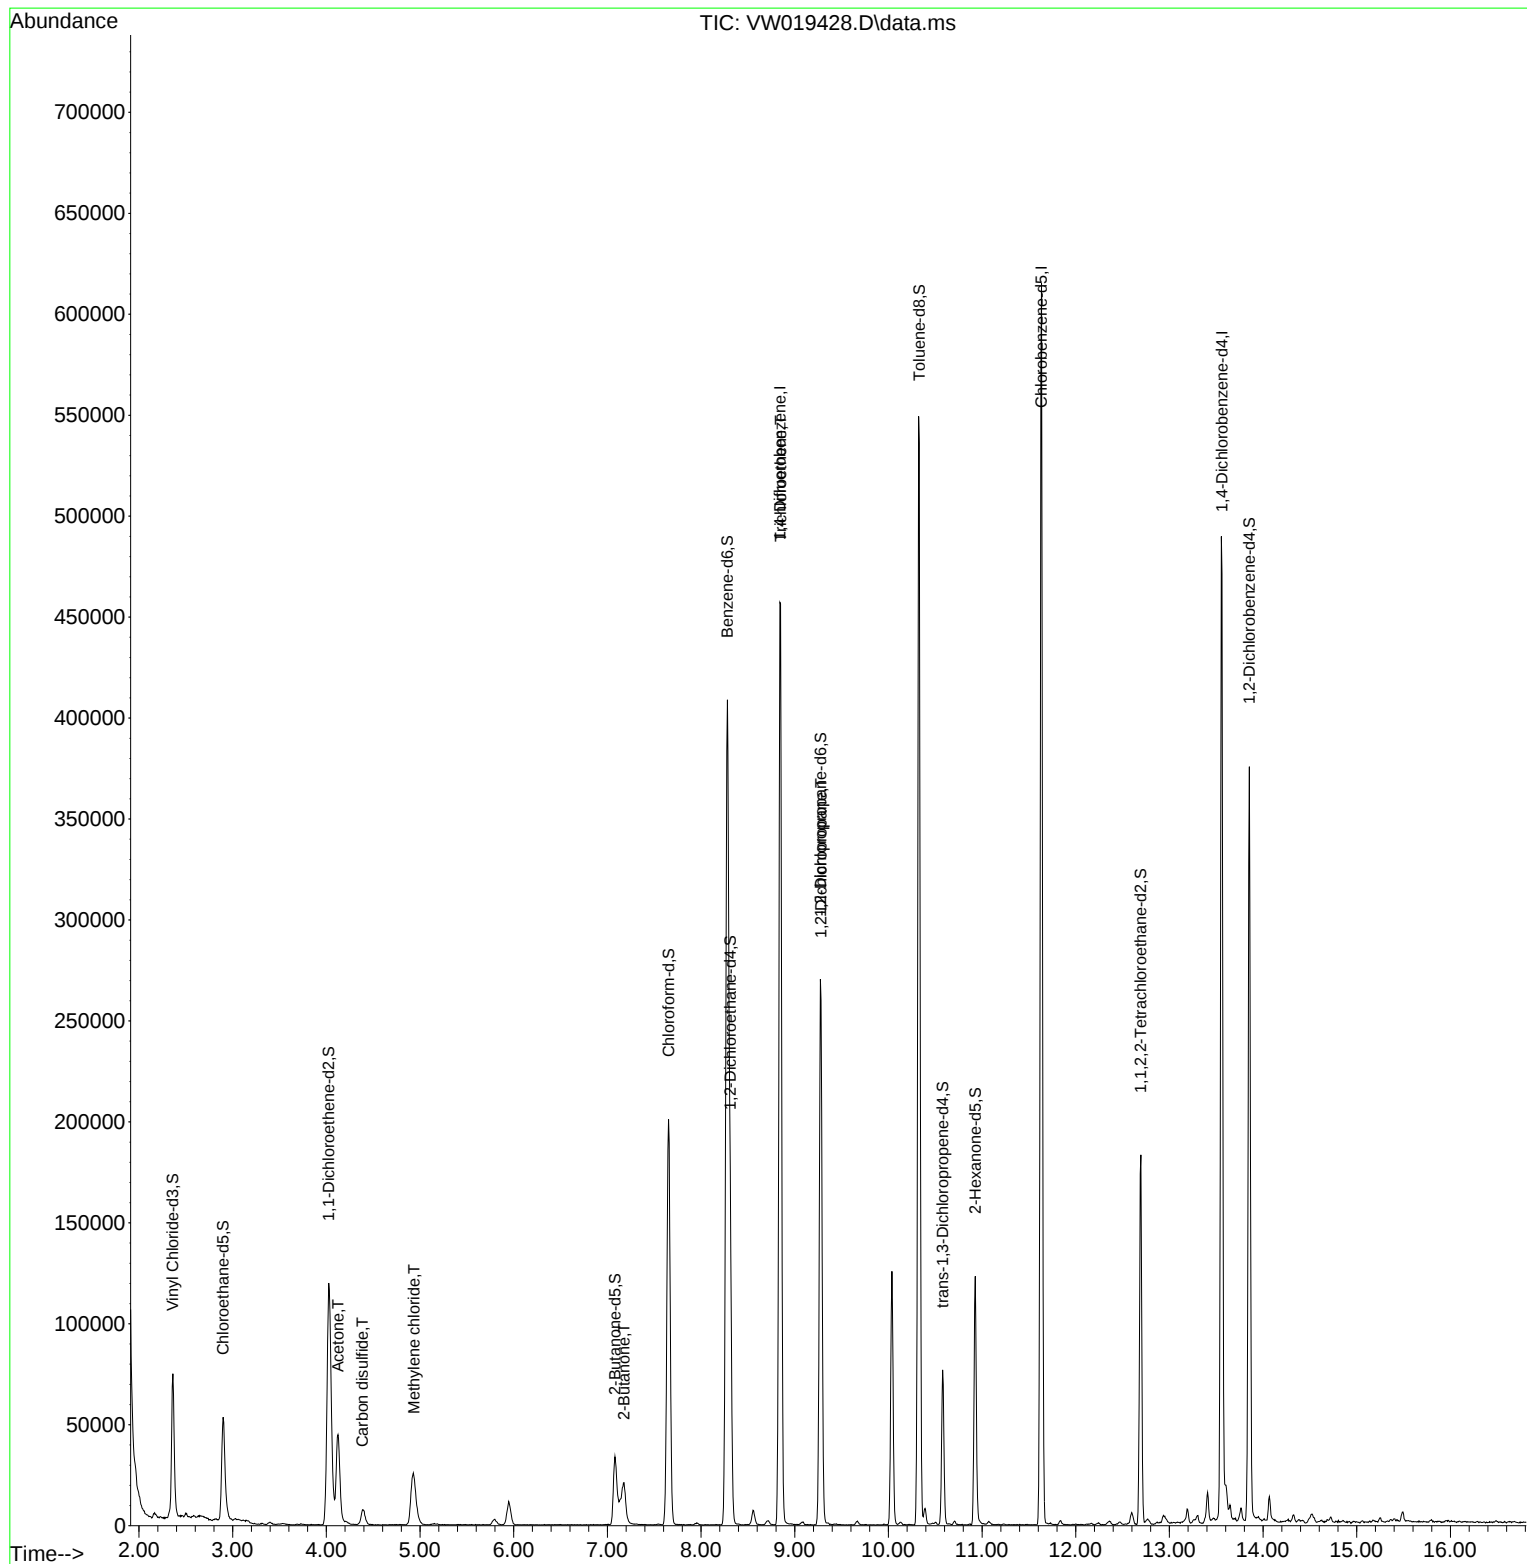


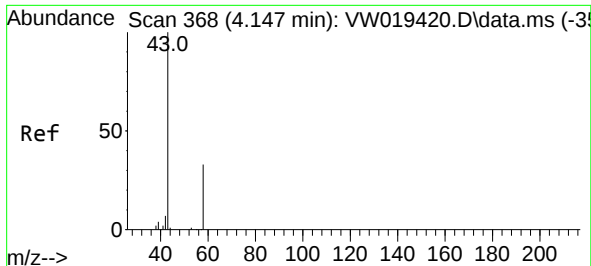

#13
Acetone
Concen: 67.656 ug/L
RT: 4.123 min Scan# 364
Delta R.T. -0.024 min
Lab File: VW019428.D
Acq: 12 Jul 2021 13:10




Instrument :
MSVOA_W
ClientSampled :


Tgt Ion: 43 Resp: 78746
Ion Ratio Lower Upper
43 100
58 32.3 0.0 53.8

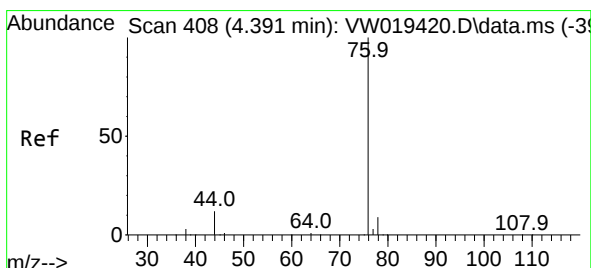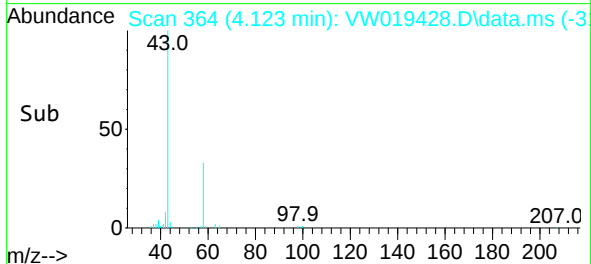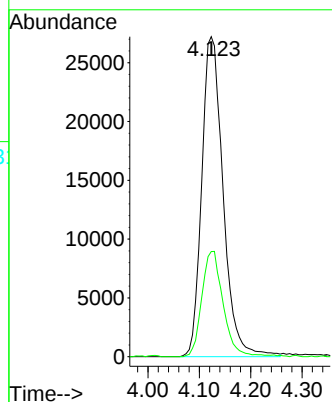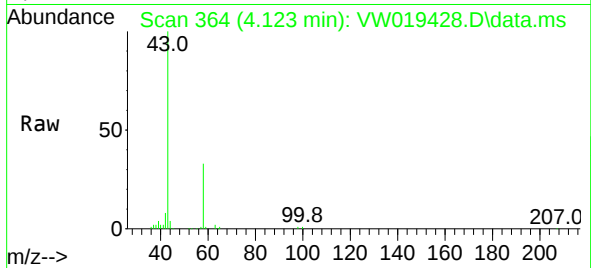

#14
Carbon disulfide
Concen: 1.000 ug/L
RT: 4.385 min Scan# 407
Delta R.T. -0.006 min
Lab File: VW019428.D
Acq: 12 Jul 2021 13:10


Tgt Ion: 76 Resp: 16063
Ion Ratio Lower Upper
76 100
78 9.0 7.4 11.0

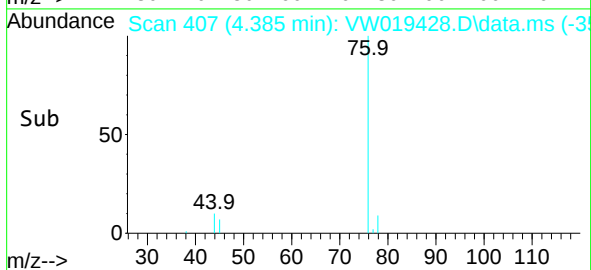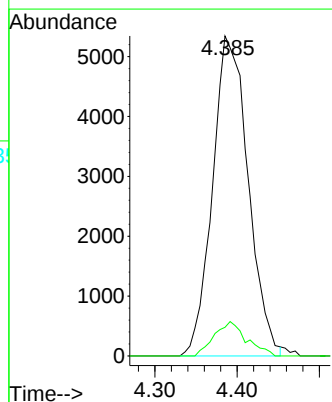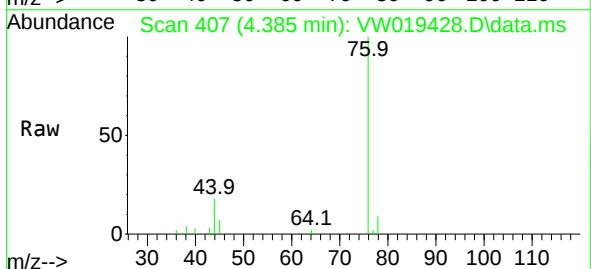

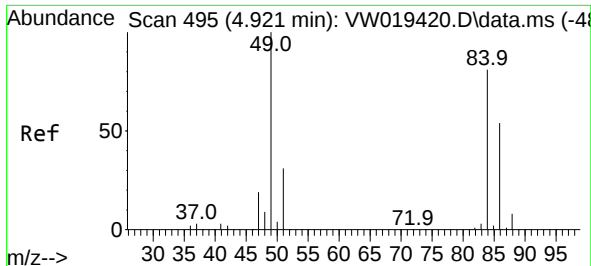




#16
Methylene chloride
Concen: 3.224 ug/L
RT: 4.934 min Scan# 497
Delta R.T. 0.012 min
Lab File: VW019428.D
Acq: 12 Jul 2021 13:10

Instrument :
MSVOA_W
ClientSampleId :

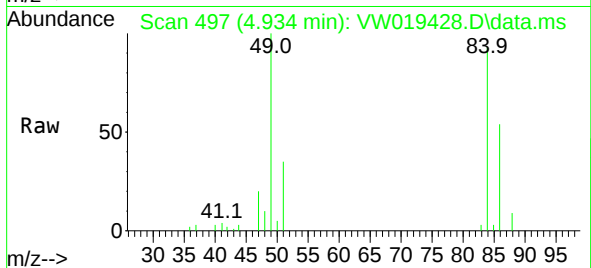

Tgt Ion: 84 Resp: 24689




Ion	Ratio	Lower	Upper
84	100		
86	58.4	45.3	84.1
49	108.1	86.6	160.8

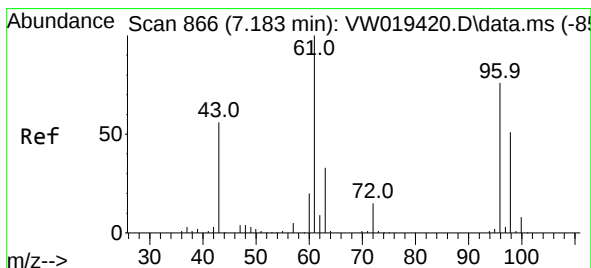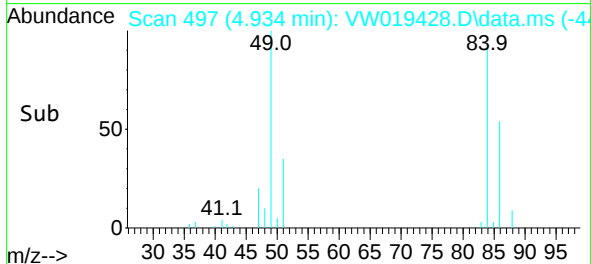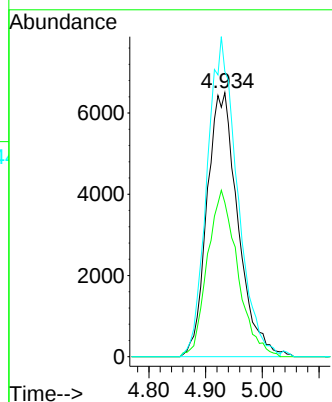


#22
2-Butanone
Concen: 18.320 ug/L
RT: 7.177 min Scan# 865
Delta R.T. -0.006 min
Lab File: VW019428.D
Acq: 12 Jul 2021 13:10

Tgt Ion: 43 Resp: 32994


Ion	Ratio	Lower	Upper
43	100		
72	26.5	14.9	44.7

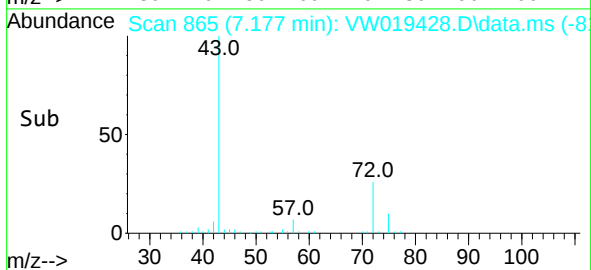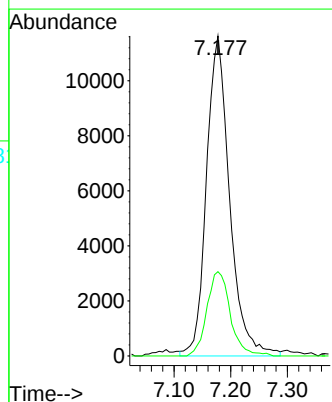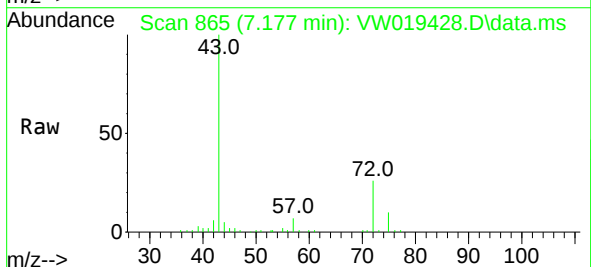



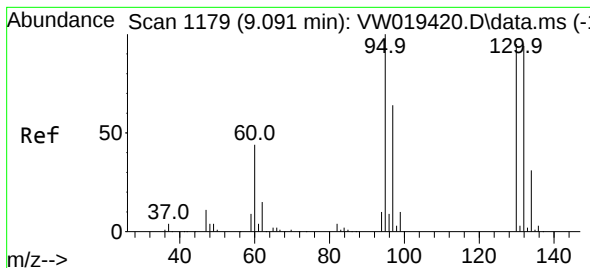


#34
Trichloroethene
Concen: 2.235 ug/L
RT: 8.848 min Scan# 1139
Delta R.T. -0.244 min
Lab File: VW019428.D
Acq: 12 Jul 2021 13:10

Instrument :
MSVOA_W
ClientSampled :

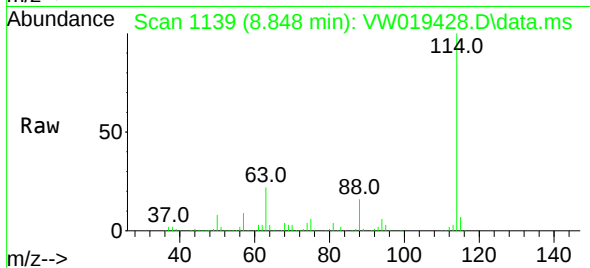

Tgt Ion: 95 Resp: 11818
Ion Ratio Lower Upper
95 100
97 0.0 47.3 87.8#
132 0.0 71.0 131.8#
130 0.0 65.1 120.9#

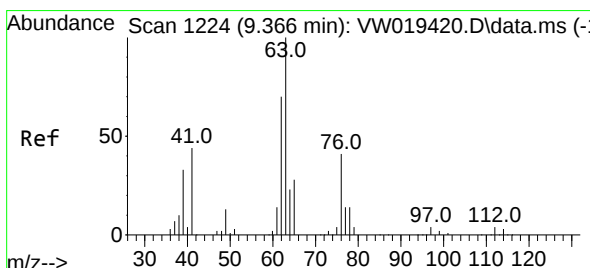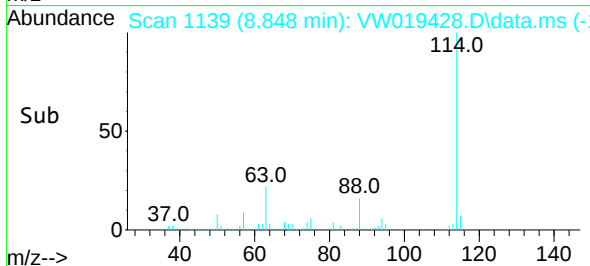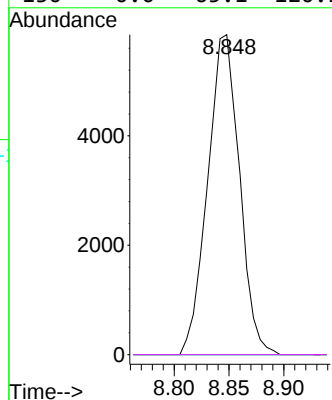

#37
1,2-Dichloropropane
Concen: 2.751 ug/L
RT: 9.281 min Scan# 1210
Delta R.T. -0.085 min
Lab File: VW019428.D
Acq: 12 Jul 2021 13:10

Tgt Ion: 63 Resp: 14445
Ion Ratio Lower Upper
63 100
112 0.3 3.9 5.9#

