
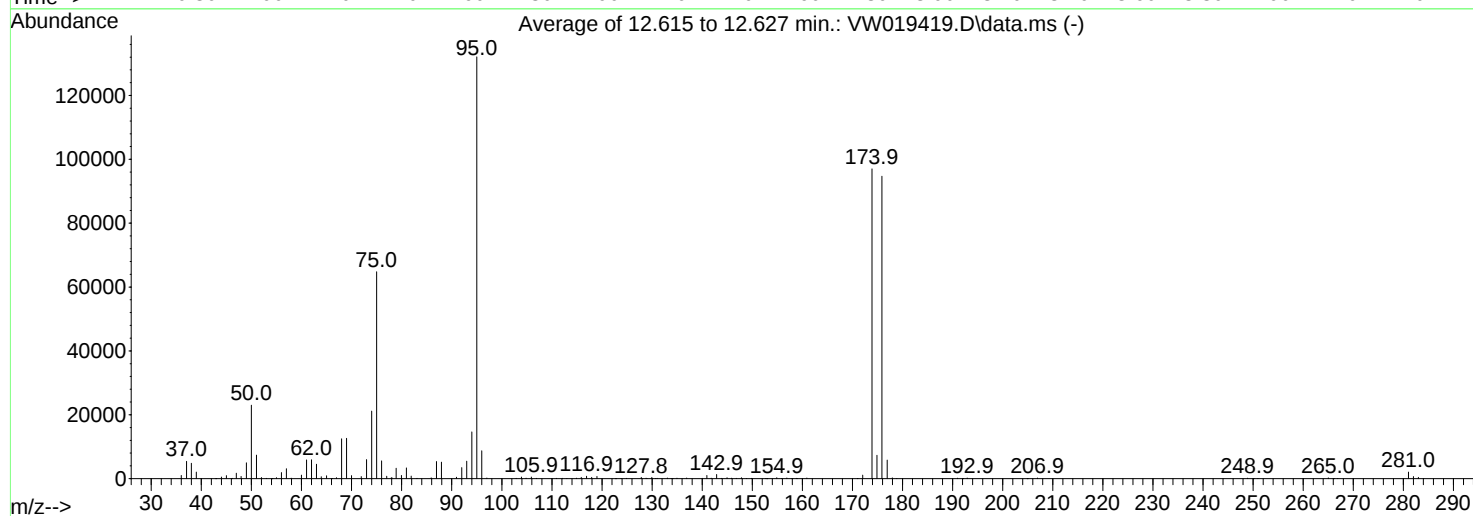


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071221\
 Data File : VW019419.D
 Acq On : 12 Jul 2021 08:56
 Operator : SY/VA
 Sample : BFB404
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB404

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Title : SFAM01.0
 Last Update : Thu Jul 15 01:04:10 2021

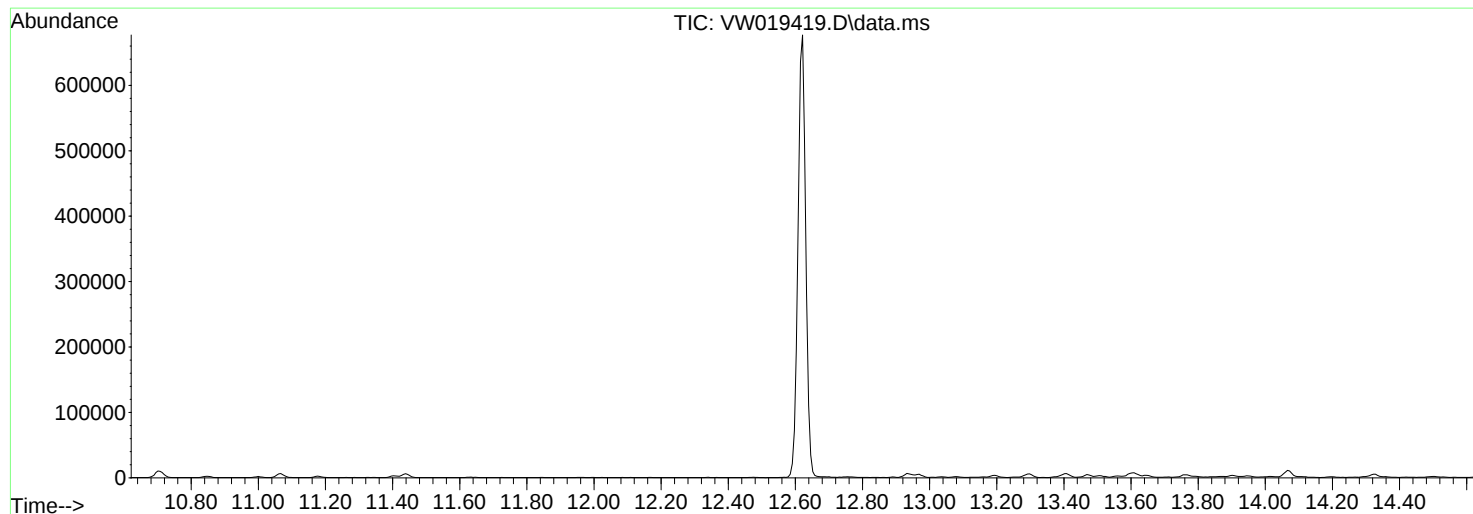

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	22997	PASS
75	95	30	80	49.0	64773	PASS
95	95	100	100	100.0	132096	PASS
96	95	5	9	6.6	8727	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.4	96987	PASS
175	174	5	9	7.6	7339	PASS
176	174	95	105	97.7	94717	PASS
177	176	5	10	6.1	5793	PASS

m/z	Abundance
40.00	211.0
41.10	63.0
42.90	70.0
44.00	327.0
55.00	66.0
56.20	67.0
57.00	91.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

m/z	Abundance
36.00	1070.0
37.10	6200.0
38.00	5084.0
39.00	2311.0
40.10	289.0
41.00	89.0
42.90	108.0
44.00	944.0
45.00	1076.0
46.00	178.0
47.00	1915.0
48.00	745.0
49.00	5510.0
50.00	25264.0
51.00	8270.0
52.00	437.0
53.00	136.0
55.00	349.0
56.00	2032.0
57.00	3592.0
57.90	157.0
60.00	1196.0
61.00	6326.0
62.00	6687.0
63.00	4922.0
64.00	718.0
65.00	1035.0
66.20	104.0
67.00	387.0
68.00	13378.0
69.00	13236.0
70.00	1057.0
71.90	725.0
73.00	6189.0
74.00	23288.0
75.00	68552.0
76.00	5967.0
77.00	860.0
77.90	604.0
78.90	3685.0
80.00	995.0
81.00	3612.0
81.90	966.0
83.00	81.0
85.80	228.0
86.90	5712.0
88.00	5492.0
90.90	465.0
92.00	3474.0
93.00	5787.0
94.00	15633.0
95.00	140672.0
96.00	9452.0
97.00	264.0
102.90	164.0
103.90	560.0
104.90	181.0
105.90	511.0
106.90	130.0
110.00	112.0
110.90	144.0
112.00	50.0
113.00	120.0
114.90	124.0
115.80	337.0
116.90	833.0
118.00	369.0
119.00	863.0
123.70	54.0
124.90	178.0
127.90	355.0
128.80	237.0
130.00	423.0
130.70	162.0
133.10	355.0
133.80	162.0
135.00	188.0
136.90	245.0
140.00	80.0
140.90	1105.0
141.80	183.0
142.90	1331.0
143.90	86.0
145.00	345.0
145.80	169.0
146.80	111.0
147.80	289.0
148.80	72.0
149.90	108.0
152.70	66.0
154.90	300.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

m/z	Abundance
36.00	1172.0
37.00	6218.0
38.00	5464.0
39.00	2274.0
40.00	281.0
41.10	52.0
42.80	57.0
44.00	920.0
45.00	1061.0
46.20	164.0
47.00	1993.0
48.00	842.0
49.00	5523.0
50.00	25768.0
51.00	8340.0
52.00	390.0
53.00	170.0
54.10	53.0
55.00	405.0
56.00	2197.0
57.00	3323.0
58.00	141.0
60.00	1232.0
61.00	6463.0
62.00	6622.0
63.00	5050.0
63.90	677.0
65.00	1078.0
65.90	110.0
67.00	321.0
68.00	13704.0
69.00	14026.0
70.00	1074.0
72.00	789.0
73.00	6896.0
74.00	23680.0
75.00	71120.0
76.00	5987.0
77.00	825.0
78.10	551.0
78.90	3504.0
80.00	1009.0
80.90	3718.0
81.90	787.0
83.10	105.0
85.90	333.0
87.00	6091.0
87.90	5818.0
91.00	476.0
92.00	4210.0
93.00	6297.0
94.00	16370.0
95.00	143680.0
96.00	9848.0
97.00	205.0
102.80	111.0
103.90	596.0
104.90	148.0
105.90	621.0
106.90	125.0
110.00	67.0
110.80	128.0
112.00	95.0
113.00	116.0
114.90	130.0
115.90	533.0
116.90	811.0
117.90	488.0
119.00	771.0
122.70	66.0
123.80	89.0
124.90	74.0
127.80	515.0
129.00	203.0
129.90	458.0
131.00	205.0
132.90	146.0
134.00	55.0
134.90	195.0
136.90	217.0
140.00	90.0
140.90	1031.0
141.80	192.0
142.90	1360.0
143.80	98.0
144.90	389.0
145.90	163.0
146.80	93.0
147.90	335.0
148.80	84.0
149.80	135.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

155.90	70.0
156.80	199.0
158.80	148.0
160.90	159.0
171.00	106.0
171.10	106.0
172.10	1114.0
173.90	93624.0
174.90	7182.0
175.90	91936.0
176.90	5585.0
177.90	236.0
178.90	83.0
191.00	228.0
192.00	67.0
193.00	346.0
204.90	55.0
207.00	253.0
248.90	275.0
250.00	58.0
250.90	112.0
265.00	364.0
266.00	63.0
266.90	117.0
281.00	3232.0
282.00	963.0
283.00	518.0
284.10	136.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

152.70	92.0
154.90	344.0
155.90	104.0
156.90	232.0
157.90	64.0
159.00	111.0
160.90	160.0
172.00	1255.0
173.90	112152.0
174.90	8717.0
175.90	102320.0
177.00	6250.0
177.90	306.0
178.80	73.0
191.00	197.0
192.90	189.0
206.90	196.0
248.90	131.0
251.00	64.0
265.00	276.0
266.90	57.0
281.00	2085.0
282.00	599.0
283.00	470.0
284.00	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

m/z	Abundance
36.00	733.0
37.00	3892.0
38.00	3953.0
39.00	1644.0
40.00	282.0
42.90	58.0
44.00	674.0
45.00	736.0
46.20	118.0
47.00	1265.0
47.90	591.0
49.00	3821.0
50.00	17960.0
51.00	5573.0
52.00	250.0
52.90	66.0
55.00	323.0
56.00	1641.0
57.00	2668.0
57.90	161.0
60.00	977.0
61.00	4760.0
62.00	4380.0
63.00	3620.0
63.90	451.0
65.00	664.0
66.00	71.0
67.10	232.0
68.00	10323.0
69.00	10694.0
70.00	790.0
72.00	522.0
73.00	4816.0
74.00	16520.0
75.00	54648.0
76.00	4731.0
77.00	620.0
78.00	468.0
78.90	2606.0
79.90	975.0
80.90	2719.0
81.90	649.0
83.00	86.0
86.00	166.0
86.90	4279.0
87.90	4232.0
90.90	362.0
92.00	2712.0
93.00	4282.0
94.00	11927.0
95.00	111936.0
96.00	6882.0
97.00	173.0
103.90	402.0
104.80	162.0
105.90	343.0
106.90	107.0
111.00	85.0
112.10	96.0
114.90	140.0
115.80	393.0
116.90	630.0
117.90	324.0
119.00	454.0
123.90	66.0
127.80	345.0
128.80	201.0
129.90	320.0
131.00	149.0
132.90	78.0
135.00	165.0
136.90	173.0
140.10	84.0
141.00	887.0
141.90	124.0
142.90	1272.0
143.80	73.0
144.90	203.0
145.80	154.0
146.80	125.0
147.80	231.0
148.90	71.0
149.80	116.0
152.90	53.0
154.90	238.0
155.80	50.0
157.00	176.0
158.80	97.0
160.90	240.0
172.00	1008.0
173.90	85184.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

174.90	6119.0
175.90	89896.0
177.00	5544.0
178.00	231.0
191.00	65.0
192.80	135.0
207.00	162.0
248.90	65.0
265.00	107.0
281.00	935.0
282.00	335.0
283.10	214.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404