

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW071318\
 Data File : VW003934.D
 Acq On : 13 Jul 2018 23:38
 Operator : VA/AP
 Sample : J3820-03
 Misc : 6.49G/5ML/MSVOA W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BU-02-071218

Quant Time: Jul 14 01:19:31 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070718S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jul 07 05:07:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	195668	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	346347	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	301839	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	126107	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	129509	50.61	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.22%	
35) Dibromofluoromethane	7.88	113	109827	45.31	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.62%	
50) Toluene-d8	10.33	98	409729	44.19	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.38%	
62) 4-Bromofluorobenzene	12.62	95	141085	42.05	ug/l	0.00
Spiked Amount 50.000			Recovery	=	84.10%	
Target Compounds						
16) Acetone	4.14	43	15296	34.45	ug/l	97
20) Methylene Chloride	4.90	84	18002	4.31	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW071318\
Data File : VW003934.D
Acq On : 13 Jul 2018 23:38
Operator : VA/AP
Sample : J3820-03
Misc : 6.49G/5ML/MSVOA W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BU-02-071218

Quant Time: Jul 14 01:19:31 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W070718S.M
Quant Title : SW846 8260
QLast Update : Sat Jul 07 05:07:25 2018
Response via : Initial Calibration

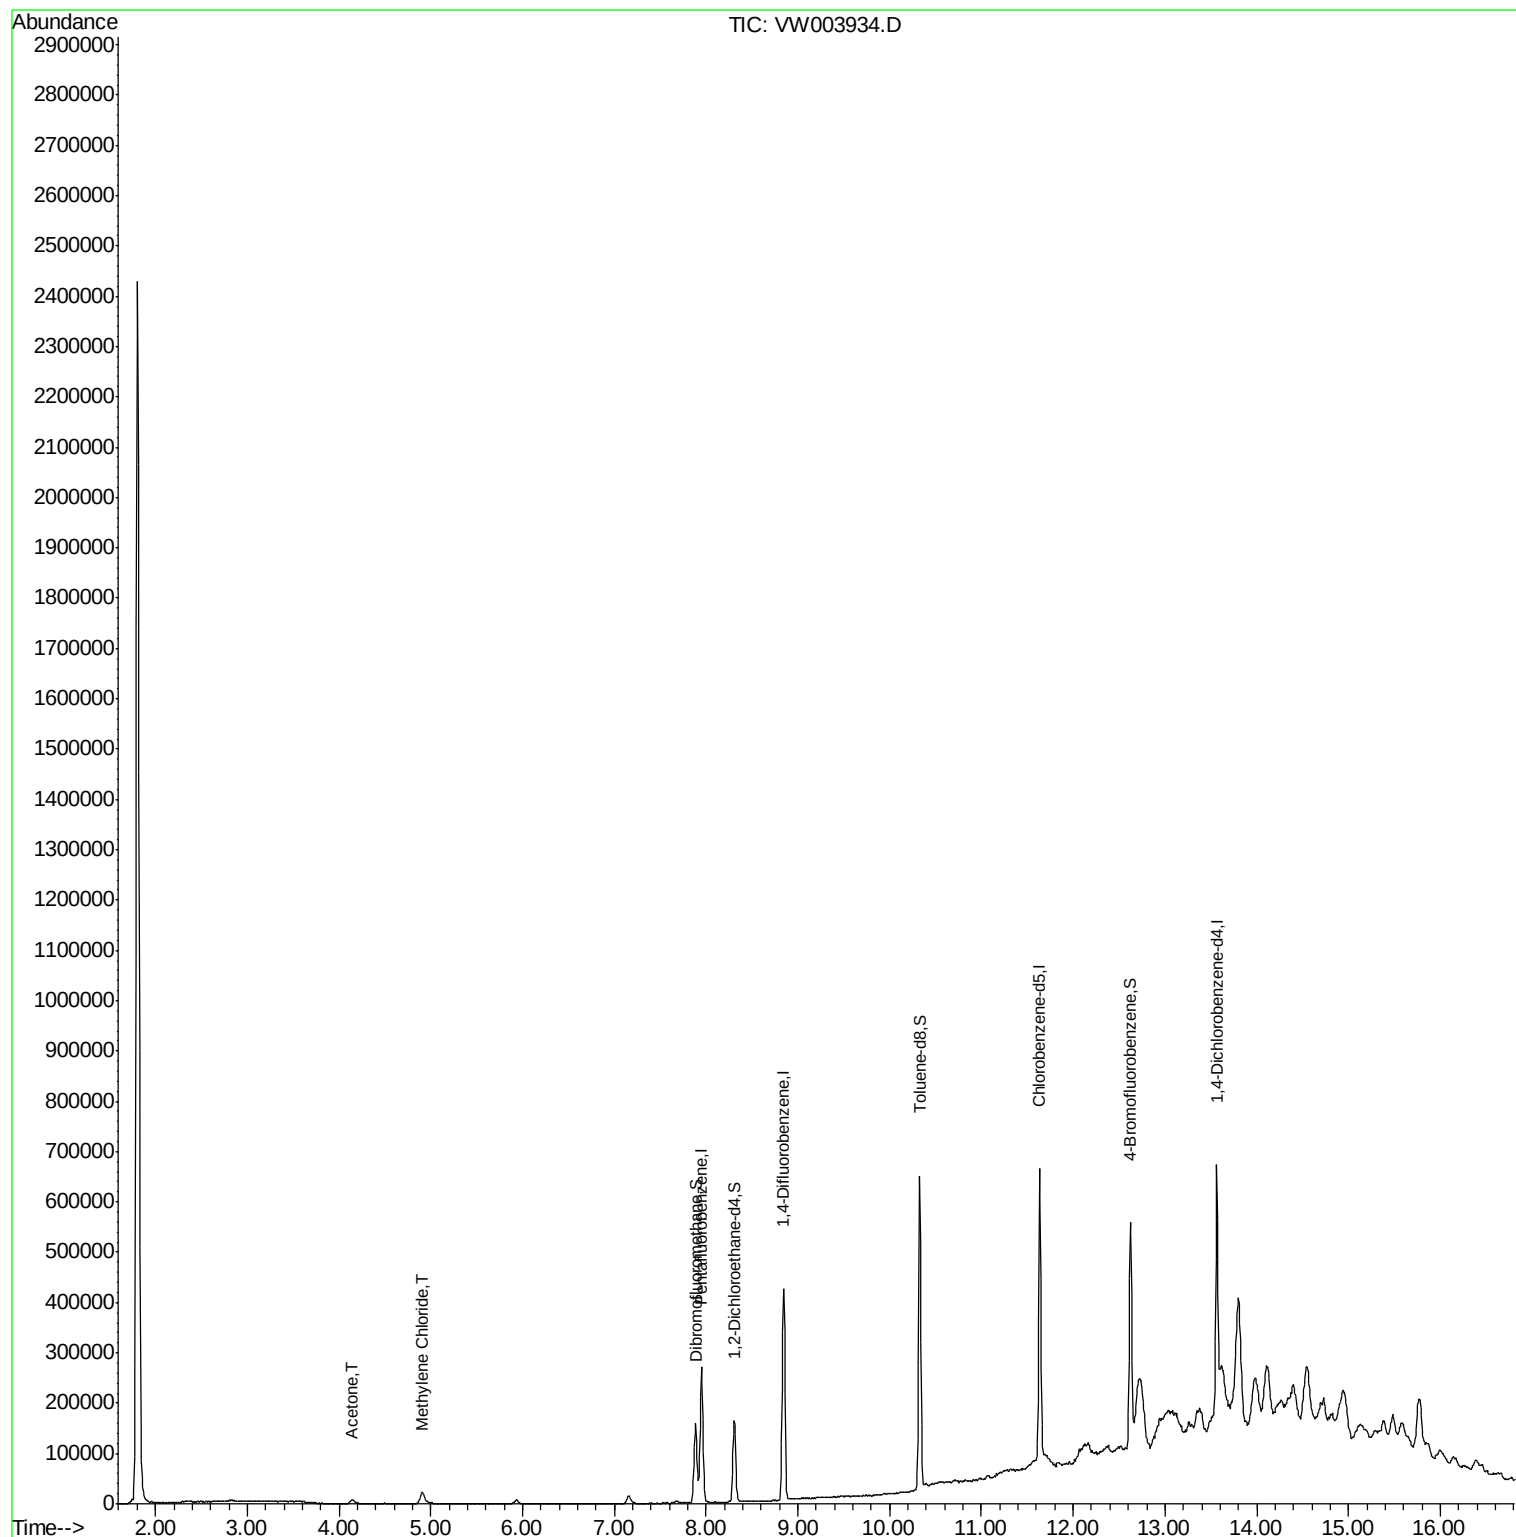

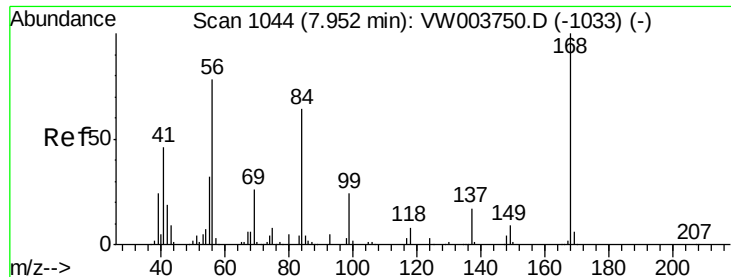

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.95 min Scan# 1044

Delta R.T. -0.00 min

Lab File: VW003934.D

Acq: 13 Jul 2018 23:38

Instrument :

MSVOA_W

ClientSampleId :


BU-02-071218

Tot Ion:168 Resp: 195668

Ion Ratio Lower Upper

168 100

99 55.2 45.0 67.6

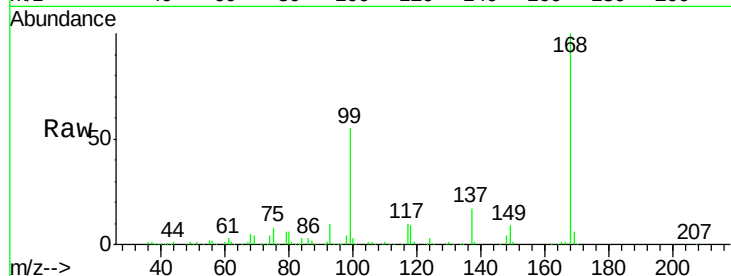

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time-->

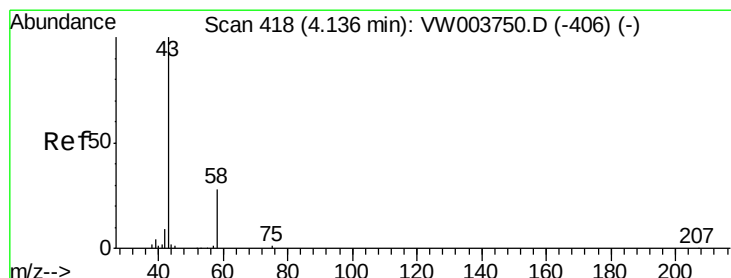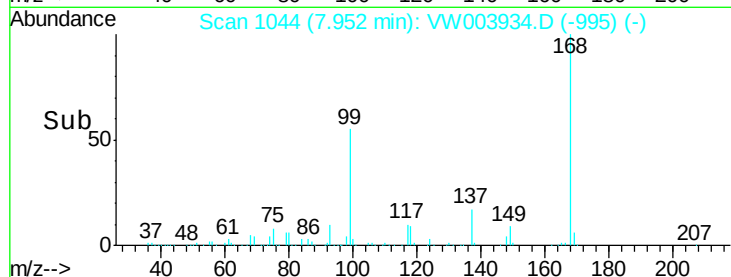

#16

Acetone

Concen: 34.45 ug/l

RT: 4.14 min Scan# 419

Delta R.T. 0.01 min

Lab File: VW003934.D


Acq: 13 Jul 2018 23:38

Tgt Ion: 43 Resp: 15296

Ion Ratio Lower Upper

43 100

58 29.9 22.6 34.0

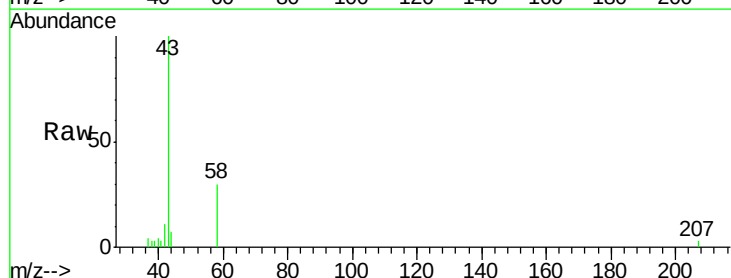

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.14

5000

4000


3000


2000

1000

0

Time-->

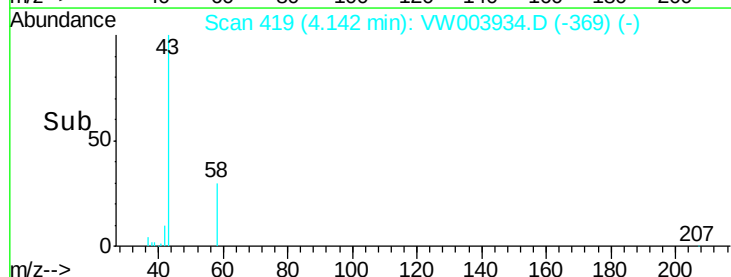

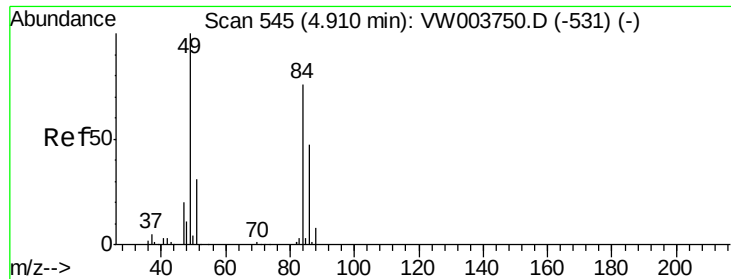

#20

Methylene Chloride

Concen: 4.31 ug/l

RT: 4.90 min Scan# 544

Delta R.T. -0.01 min

Lab File: VW003934.D

Acq: 13 Jul 2018 23:38

Instrument :

MSVOA_W

ClientSampleId :

BU-02-071218

Tot Ion: 84 Resp: 18002


Ion Ratio Lower Upper

84 100

49 127.8 105.1 157.7

51 34.0 32.5 48.7

86 58.3 49.8 74.6



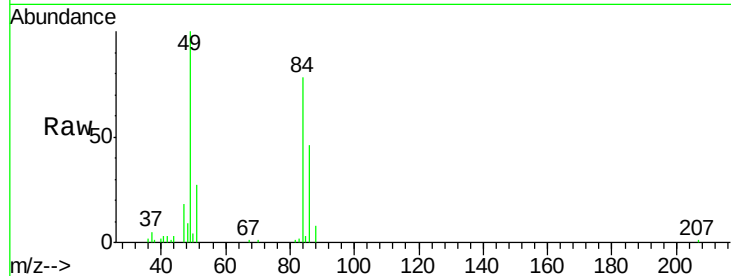


Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW

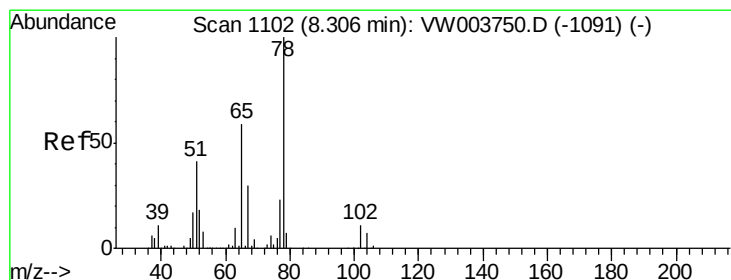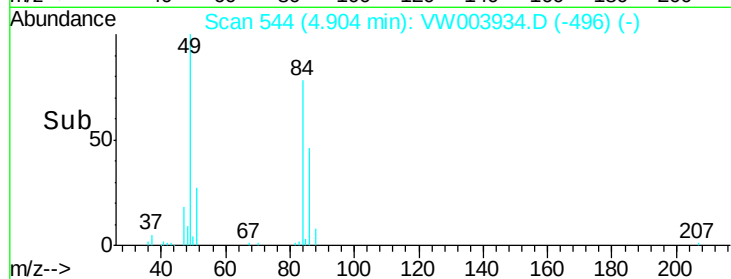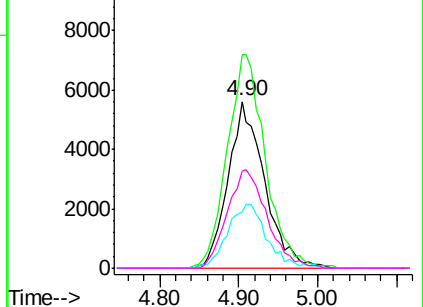

#33

1,2-Dichloroethane-d4

Concen: 50.61 ug/l

RT: 8.31 min Scan# 1102

Delta R.T. -0.00 min

Lab File: VW003934.D


Acq: 13 Jul 2018 23:38

Tgt Ion: 65 Resp: 129509

Ion Ratio Lower Upper



65 100


67 51.6 0.0 103.8

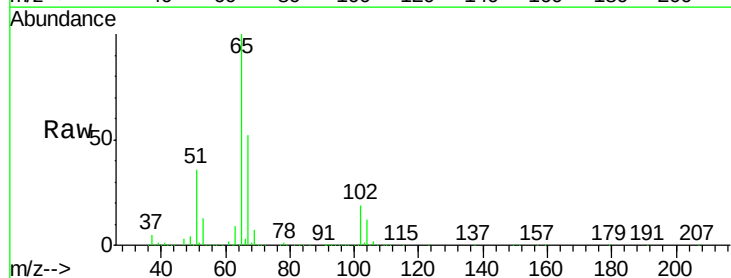

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

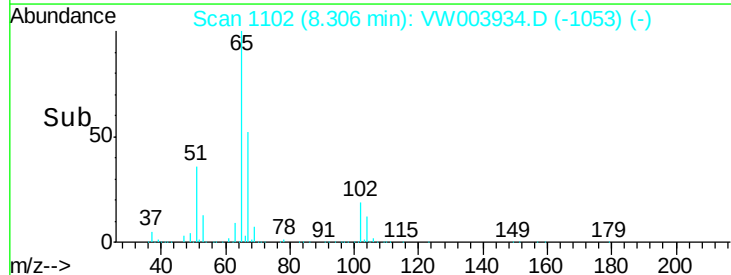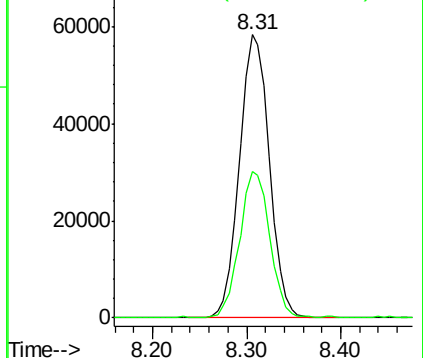


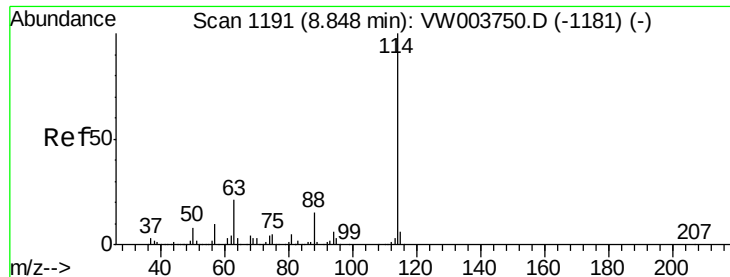

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.85 min Scan# 1191
 Delta R.T. -0.00 min
 Lab File: VW003934.D
 Acq: 13 Jul 2018 23:38

Instrument :
 MSVOA_W
 ClientSampleId :
 BU-02-071218




Tot Ion	Ratio	Lower	Upper
114	100		
63	21.7	0.0	41.8
88	15.2	0.0	30.2

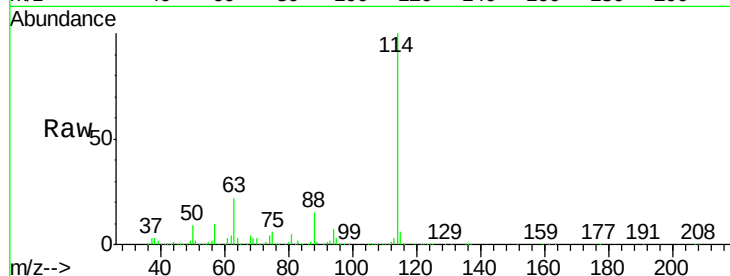

Abundance Ion 113.90 (113.60 to 114.60): V


Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

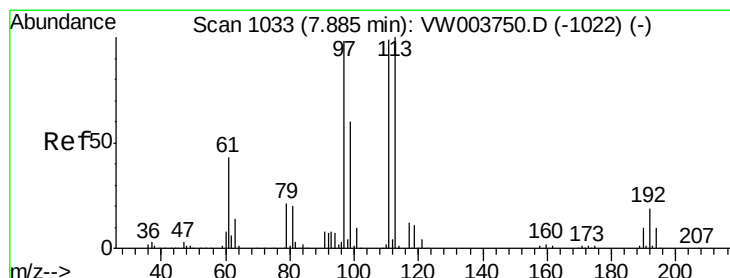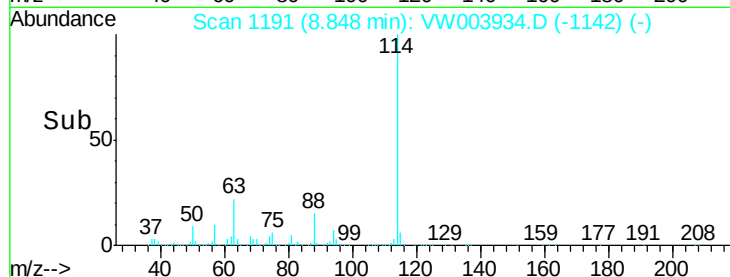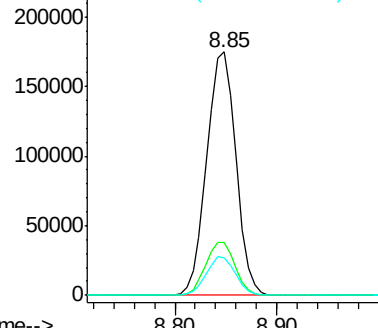

#35
 Dibromofluoromethane
 Concen: 45.31 ug/l
 RT: 7.88 min Scan# 1033
 Delta R.T. -0.00 min
 Lab File: VW003934.D
 Acq: 13 Jul 2018 23:38



Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.7	81.7	122.5
192	19.9	15.8	23.8

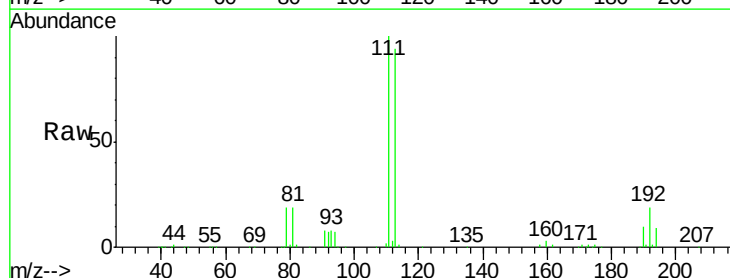


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

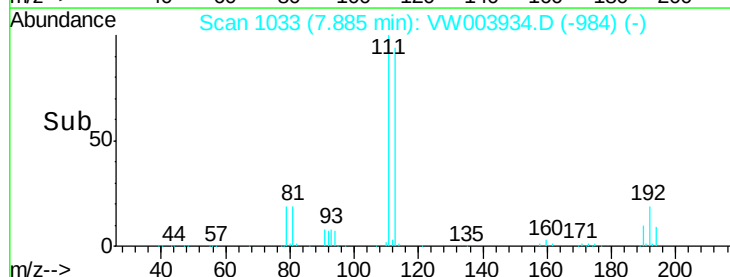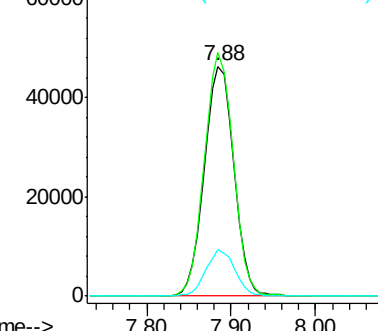

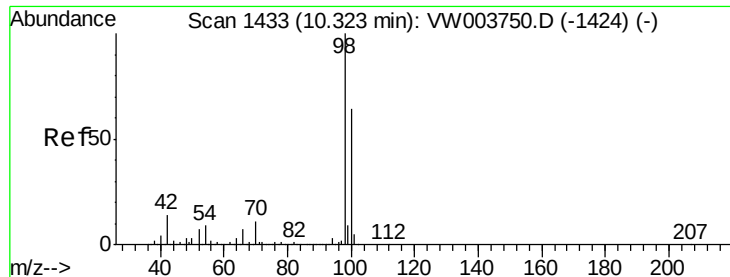

#50

Toluene-d8

Concen: 44.19 ug/l

RT: 10.33 min Scan# 1434

Delta R.T. 0.01 min

Lab File: VW003934.D

Acq: 13 Jul 2018 23:38

Instrument :

MSVOA_W

ClientSampleId :


BU-02-071218

Tot Ion: 98 Resp: 409729

Ion Ratio Lower Upper




98 100

100 63.7 50.8 76.2

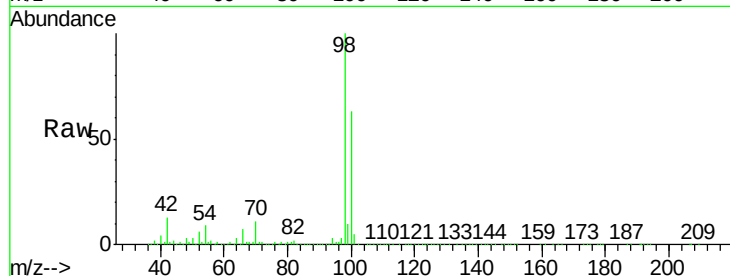

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

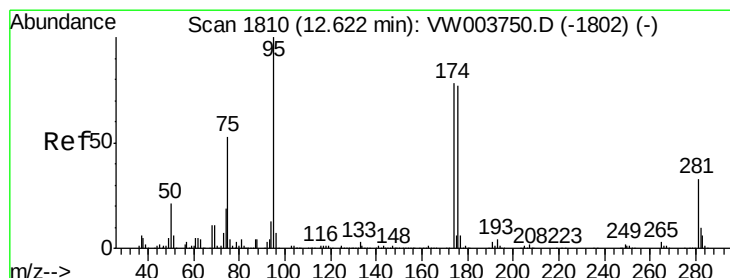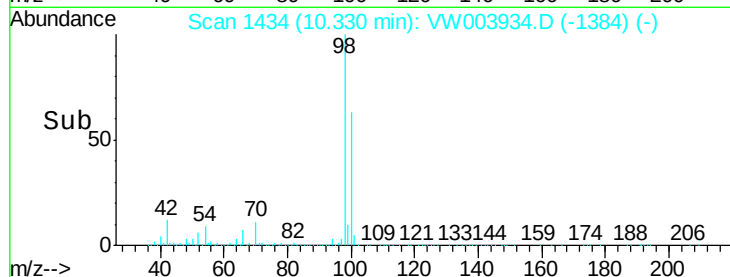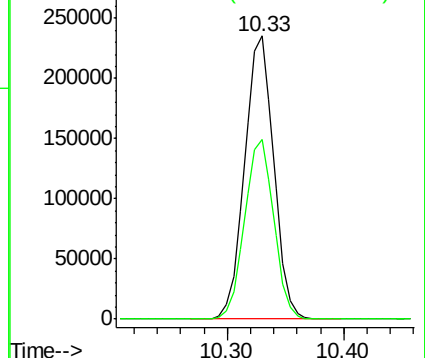

#62

4-Bromofluorobenzene

Concen: 42.05 ug/l

RT: 12.62 min Scan# 1810

Delta R.T. -0.00 min

Lab File: VW003934.D

Acq: 13 Jul 2018 23:38


Tgt Ion: 95 Resp: 141085

Ion Ratio Lower Upper

95 100

174 77.9 0.0 163.4



176 75.4 0.0 156.8

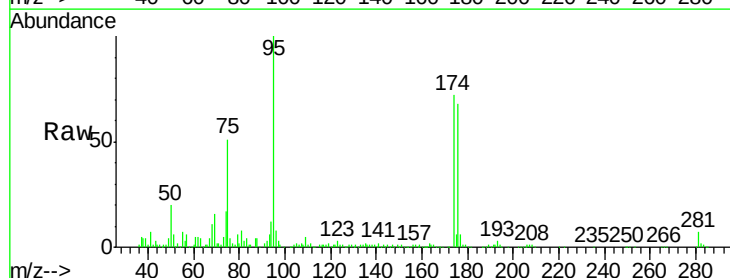


Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW



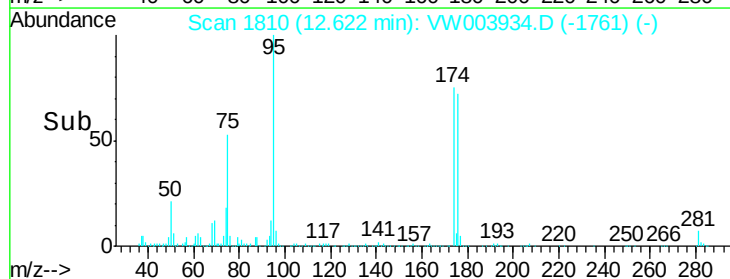
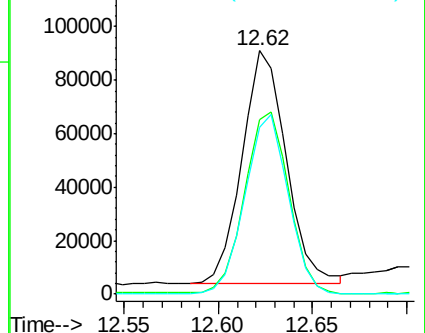


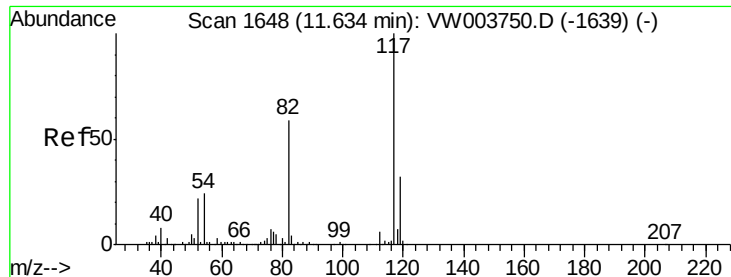

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.63 min Scan# 1648
Delta R.T. -0.00 min
Lab File: VW003934.D
Acq: 13 Jul 2018 23:38

Instrument :
MSVOA_W
ClientSampleId :
BU-02-071218

Tot Ion:117 Resp: 301839
Ion Ratio Lower Upper
117 100
82 59.4 46.9 70.3
119 32.4 25.5 38.3

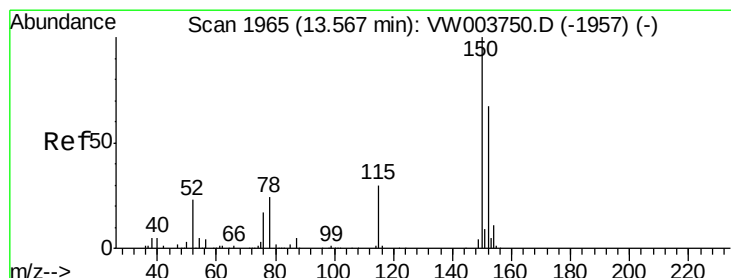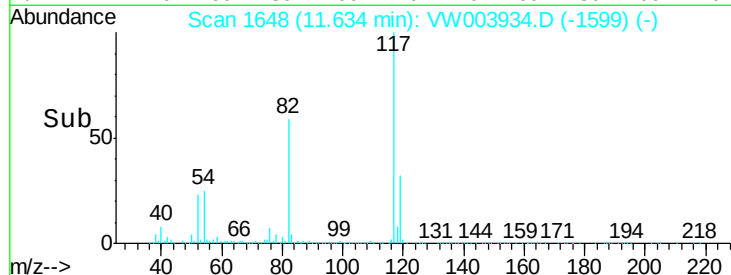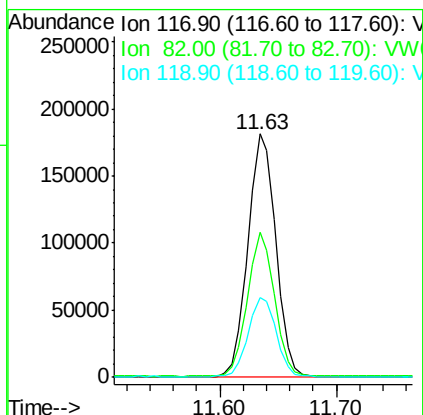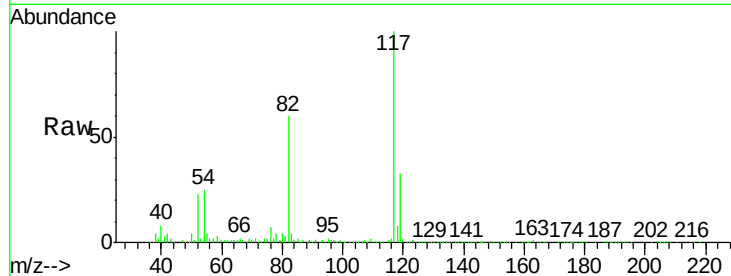

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.57 min Scan# 1965
Delta R.T. -0.00 min
Lab File: VW003934.D
Acq: 13 Jul 2018 23:38

Tgt Ion:152 Resp: 126107
Ion Ratio Lower Upper
152 100
115 58.3 28.9 86.8
150 154.8 0.0 342.4

