


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071318\
 Data File : VW003919.D
 Acq On : 13 Jul 2018 15:56
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070718S.M
 Title : SW846 8260
 Last Update : Sat Jul 07 05:07:25 2018

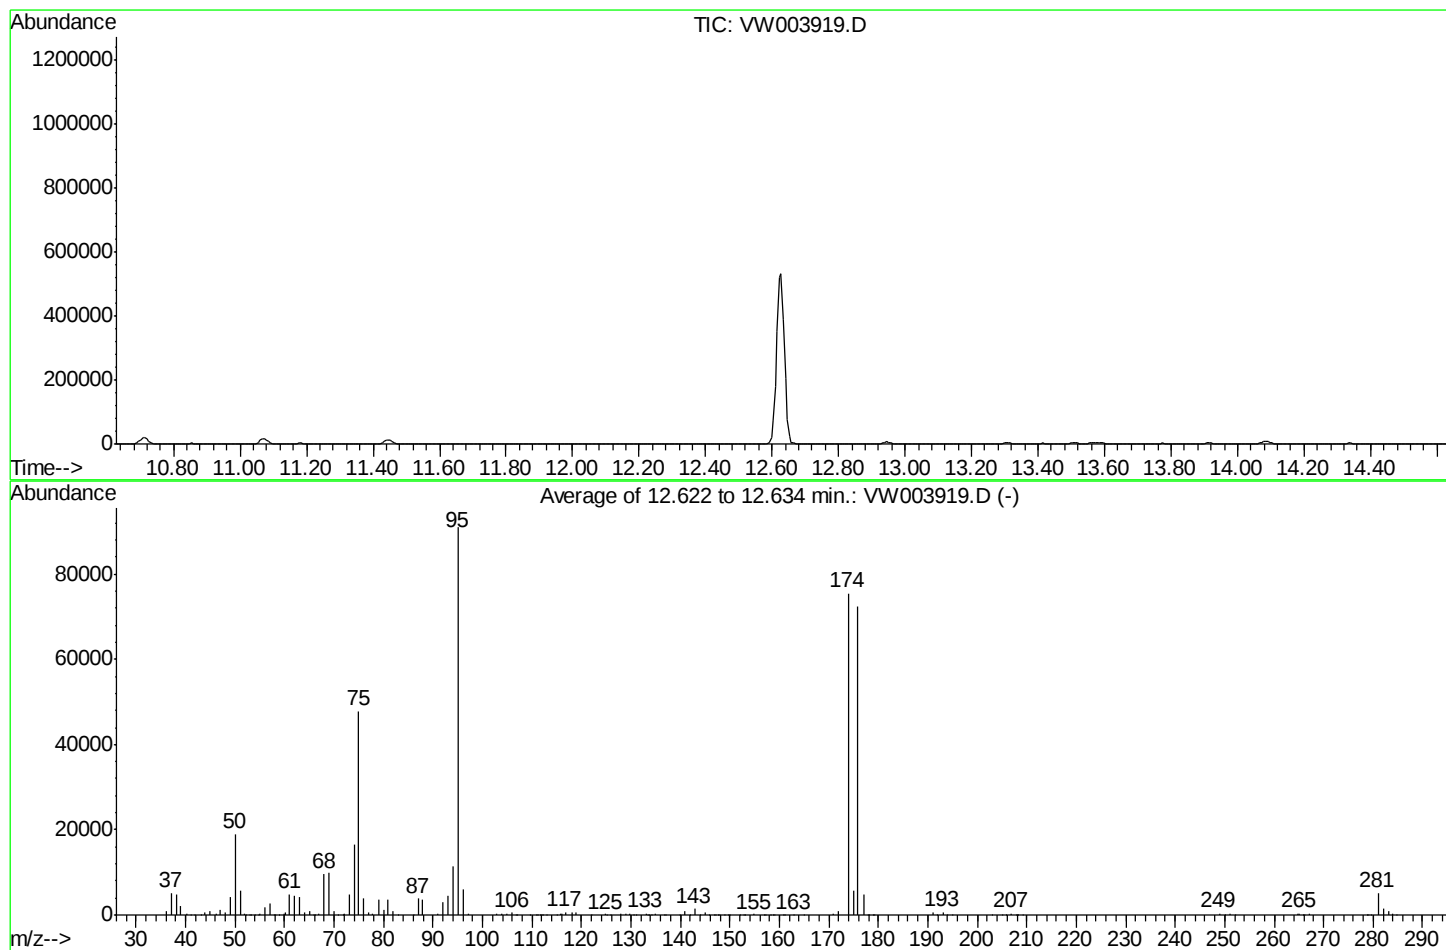

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	19030	PASS
75	95	30	60	52.6	47856	PASS
95	95	100	100	100.0	90946	PASS
96	95	5	9	6.7	6113	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.9	75381	PASS
175	174	5	9	7.6	5722	PASS
176	174	95	101	96.1	72453	PASS
177	176	5	9	6.7	4837	PASS