


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071320\
 Data File : VW015837.D
 Acq On : 13 Jul 2020 09:54
 Operator : SY/VA
 Sample : BFB18
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB18

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071320S.M
 Title : VOC Analysis
 Last Update : Tue Jul 14 03:37:11 2020

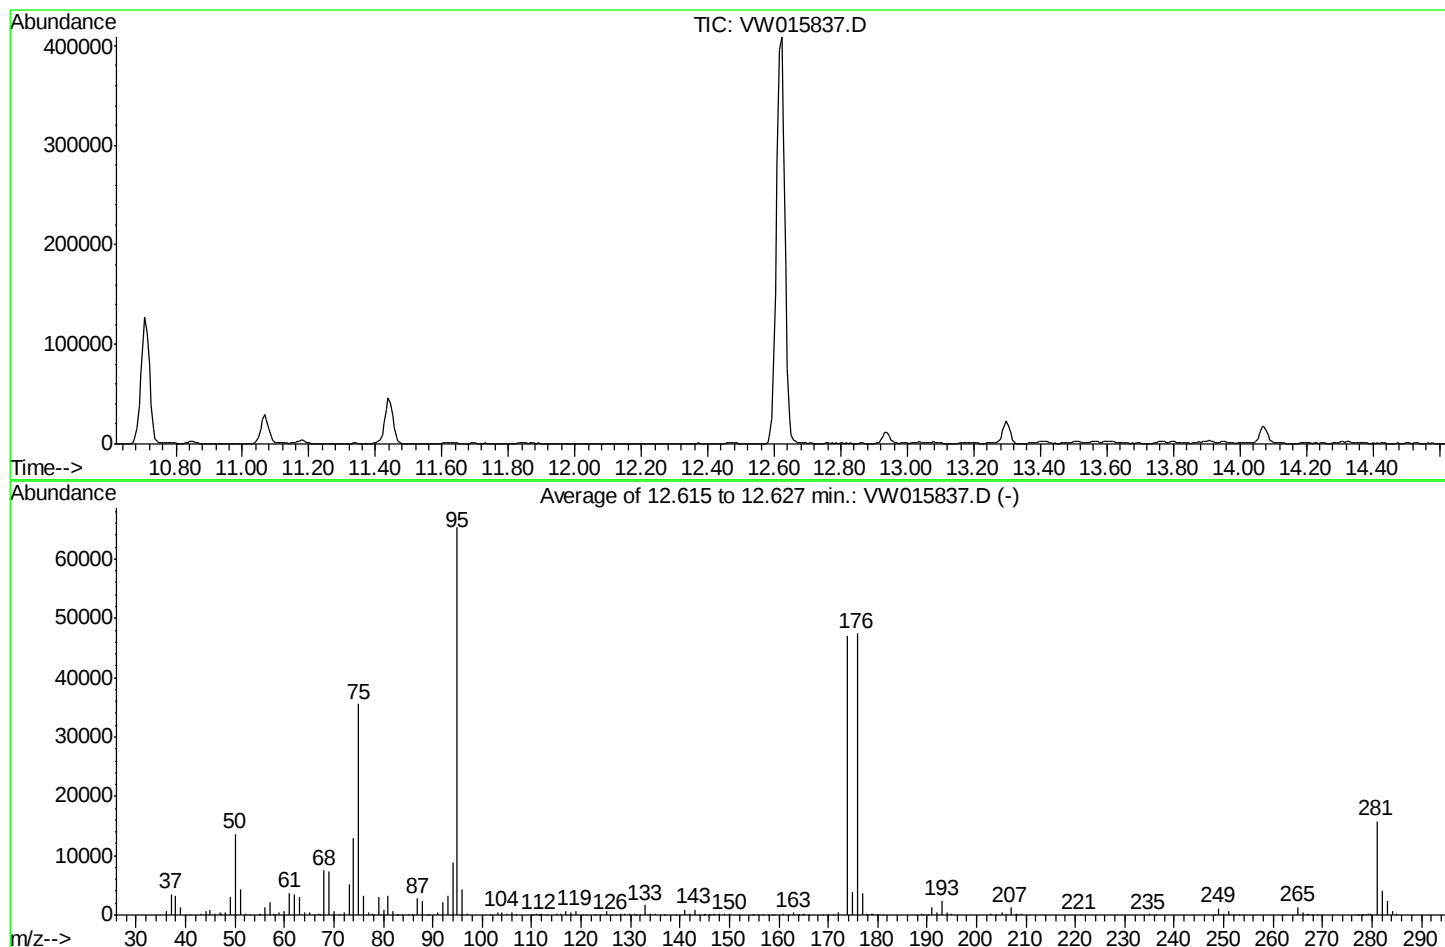

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	13682	PASS
75	95	30	80	54.5	35602	PASS
95	95	100	100	100.0	65346	PASS
96	95	5	9	6.7	4348	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.1	47138	PASS
175	174	5	9	8.2	3853	PASS
176	174	95	101	100.6	47442	PASS
177	176	5	9	7.5	3573	PASS

m/z	Abundance
36.00	879.0
37.00	3732.0
38.00	3765.0
39.10	1668.0
39.90	176.0
40.90	64.0
42.10	53.0
43.00	279.0
44.00	767.0
45.00	1037.0
45.90	237.0
47.00	779.0
47.90	463.0
49.00	3564.0
50.00	14483.0
51.00	4280.0
52.00	235.0
53.00	89.0
54.90	310.0
56.10	1394.0
57.00	2529.0
57.90	230.0
59.00	594.0
60.00	879.0
61.00	4025.0
62.00	3510.0
63.00	3032.0
64.10	337.0
65.00	399.0
66.10	89.0
66.80	272.0
68.00	7500.0
69.00	7629.0
70.00	619.0
71.10	54.0
72.00	408.0
73.00	6318.0
74.00	13177.0
75.00	37072.0
76.10	3589.0
76.90	398.0
77.80	313.0
78.90	2898.0
80.00	896.0
80.90	3295.0
82.00	643.0
82.70	90.0
83.70	83.0
85.10	63.0
85.90	68.0
86.90	3102.0
87.90	2455.0
88.90	191.0
90.90	401.0
92.00	2201.0
93.00	3383.0
94.00	8982.0
95.00	65752.0
96.00	4392.0
97.00	238.0
103.10	478.0
103.90	454.0
105.00	193.0
105.90	409.0
107.00	110.0
109.80	80.0
110.80	181.0
111.50	110.0
112.00	174.0
112.90	85.0
115.10	253.0
115.90	251.0
117.00	516.0
117.90	491.0
118.90	696.0
120.20	58.0
120.90	129.0
125.20	854.0
126.90	75.0
128.00	269.0
128.90	164.0
129.90	270.0
130.90	239.0
131.90	105.0
133.10	2641.0
133.90	720.0
134.80	305.0
137.00	147.0
139.30	61.0
140.90	908.0
142.00	150.0
142.90	989.0

Instrument :
MSVOA_W
ClientSampleId :
BFB18

143.80	64.0
145.10	154.0
146.10	193.0
147.10	366.0
147.80	181.0
149.00	256.0
150.00	156.0
154.80	130.0
158.50	67.0
159.20	158.0
160.90	251.0
162.00	86.0
163.00	534.0
163.90	65.0
165.00	303.0
166.20	63.0
168.80	53.0
172.10	414.0
173.90	45504.0
175.00	3587.0
175.90	43760.0
177.00	3579.0
177.90	348.0
178.90	702.0
179.80	121.0
181.00	98.0
188.90	296.0
191.00	1864.0
192.00	693.0
193.10	3661.0
194.00	751.0
195.00	368.0
203.00	299.0
204.00	129.0
205.10	498.0
206.00	139.0
207.00	1870.0
208.00	451.0
209.10	226.0
220.90	83.0
235.00	281.0
236.10	80.0
249.00	1638.0
250.10	431.0
251.00	906.0
252.10	161.0
253.20	83.0
265.10	1811.0
266.00	569.0
267.10	505.0
268.00	153.0
269.00	70.0
276.60	110.0
277.90	147.0
279.30	307.0
279.90	514.0
281.00	22368.0
282.10	5805.0
283.10	2962.0
284.00	745.0
285.00	314.0

Instrument :
MSVOA_W
ClientSampleId :
BFB18

m/z	Abundance
36.00	723.0
37.00	3990.0
38.00	3536.0
39.00	1359.0
40.00	229.0
40.80	85.0
43.00	225.0
44.00	653.0
45.00	953.0
46.00	127.0
47.20	630.0
47.90	479.0
49.00	2974.0
50.00	14999.0
51.00	4824.0
52.10	182.0
52.80	58.0
55.10	261.0
56.10	1372.0
57.00	2512.0
58.10	84.0
59.00	366.0
60.00	624.0
61.00	4205.0
62.00	3851.0
63.00	3303.0
64.00	416.0
65.00	398.0
66.90	238.0
68.00	8672.0
69.00	8080.0
70.00	679.0
71.90	405.0
73.00	5760.0
74.00	14496.0
75.10	39368.0
76.10	3281.0
77.00	449.0
77.80	373.0
78.90	3390.0
80.00	954.0
80.90	3458.0
82.00	719.0
83.10	180.0
86.10	100.0
87.00	3136.0
88.00	2546.0
91.00	485.0
92.10	2337.0
93.00	3299.0
94.00	10262.0
95.00	72480.0
96.00	4857.0
97.00	160.0
101.70	57.0
103.00	500.0
104.00	452.0
104.80	132.0
106.00	502.0
106.90	138.0
110.00	196.0
110.80	262.0
111.70	202.0
112.00	186.0
113.00	118.0
114.90	159.0
115.90	354.0
117.00	668.0
118.00	553.0
118.90	774.0
123.80	63.0
125.10	545.0
127.90	252.0
128.90	157.0
129.90	344.0
130.90	176.0
131.80	68.0
133.00	1578.0
134.90	302.0
136.70	107.0
139.10	85.0
141.00	893.0
142.00	175.0
143.00	909.0
143.80	109.0
144.80	171.0
145.00	167.0
145.80	107.0
146.90	305.0
147.90	203.0
149.00	133.0
150.10	147.0

Instrument :
MSVOA_W
ClientSampleId :
BFB18

151.80	73.0
155.00	115.0
155.90	60.0
156.80	116.0
157.80	118.0
159.10	83.0
160.90	190.0
163.00	306.0
164.10	53.0
164.90	295.0
166.10	83.0
168.90	50.0
171.10	99.0
171.90	604.0
174.00	50856.0
174.90	4157.0
175.90	51872.0
177.00	4101.0
177.80	136.0
178.10	169.0
179.10	435.0
180.00	117.0
181.10	80.0
188.90	140.0
190.90	1532.0
192.10	471.0
193.00	2342.0
194.00	390.0
194.90	294.0
202.90	203.0
203.80	69.0
205.10	361.0
206.00	115.0
207.00	1192.0
208.00	247.0
209.10	95.0
220.90	91.0
235.00	234.0
236.20	76.0
248.30	139.0
249.10	1086.0
250.00	415.0
251.10	516.0
252.20	88.0
265.00	1424.0
266.00	408.0
267.00	277.0
267.90	134.0
269.00	53.0
277.40	76.0
278.10	98.0
278.60	176.0
279.20	223.0
281.10	17968.0
282.10	4187.0
283.10	2820.0
284.10	734.0
285.10	160.0

Instrument :
MSVOA_W
ClientSampleId :
BFB18

m/z	Abundance
36.10	511.0
37.00	2862.0
38.00	2658.0
39.10	1181.0
40.00	267.0
42.80	84.0
43.10	90.0
44.00	734.0
45.10	591.0
46.10	94.0
47.00	555.0
48.00	394.0
49.10	2668.0
50.00	11564.0
51.00	3566.0
52.00	203.0
52.90	52.0
55.00	236.0
56.00	1209.0
57.10	1845.0
57.90	183.0
59.10	114.0
60.10	485.0
61.00	3111.0
62.10	2847.0
63.10	2452.0
63.90	320.0
65.00	257.0
67.10	193.0
68.00	6394.0
69.00	6347.0
70.00	503.0
72.10	354.0
73.00	3736.0
74.00	11304.0
75.00	30368.0
76.00	2891.0
77.10	408.0
78.00	277.0
79.00	2872.0
80.00	866.0
81.00	2809.0
81.80	642.0
82.90	120.0
87.00	2118.0
88.00	2425.0
89.20	51.0
90.90	333.0
92.00	1978.0
93.00	2913.0
94.00	7270.0
95.00	57808.0
96.00	3796.0
96.90	124.0
102.90	111.0
103.90	472.0
104.70	130.0
106.00	309.0
106.80	80.0
110.20	96.0
110.90	188.0
111.60	86.0
112.10	93.0
113.00	67.0
115.00	129.0
116.00	223.0
116.80	547.0
118.00	285.0
119.00	490.0
122.90	58.0
123.90	74.0
125.00	305.0
126.10	56.0
127.90	361.0
128.90	166.0
129.70	158.0
131.10	123.0
133.00	892.0
133.90	187.0
135.00	182.0
136.90	72.0
140.90	763.0
142.00	56.0
142.90	777.0
143.80	92.0
145.00	128.0
145.90	194.0
146.90	158.0
148.00	152.0
148.80	109.0
150.20	75.0
154.90	126.0

Instrument :
MSVOA_W
ClientSampleId :
BFB18

155.80	84.0
156.90	199.0
159.10	73.0
160.90	113.0
162.90	180.0
164.70	113.0
170.00	98.0
172.00	474.0
174.00	45056.0
175.00	3816.0
175.90	46696.0
177.00	3039.0
178.00	173.0
178.90	215.0
189.10	122.0
190.10	52.0
191.00	787.0
193.00	1387.0
193.90	191.0
195.00	166.0
203.00	108.0
203.90	53.0
205.00	227.0
207.00	709.0
208.20	142.0
208.90	125.0
234.80	96.0
249.00	609.0
250.00	130.0
250.90	229.0
265.10	702.0
265.90	114.0
266.80	90.0
267.10	94.0
277.10	62.0
279.30	154.0
279.70	173.0
281.10	6962.0
282.10	2427.0
283.10	1322.0
284.10	364.0
285.00	153.0

Instrument :
MSVOA_W
ClientSampleId :
BFB18

Scan 1750 (12.573 min): VW015837.D
BFB18

m/z	Abundance
39.20	80.0
39.90	179.0
41.10	100.0
42.30	62.0
44.10	165.0
57.10	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB18