


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071420\
 Data File : VW015851.D
 Acq On : 14 Jul 2020 08:17
 Operator : SY/VA
 Sample : BFB19
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB19

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071320S.M
 Title : VOC Analysis
 Last Update : Wed Jul 15 06:37:42 2020

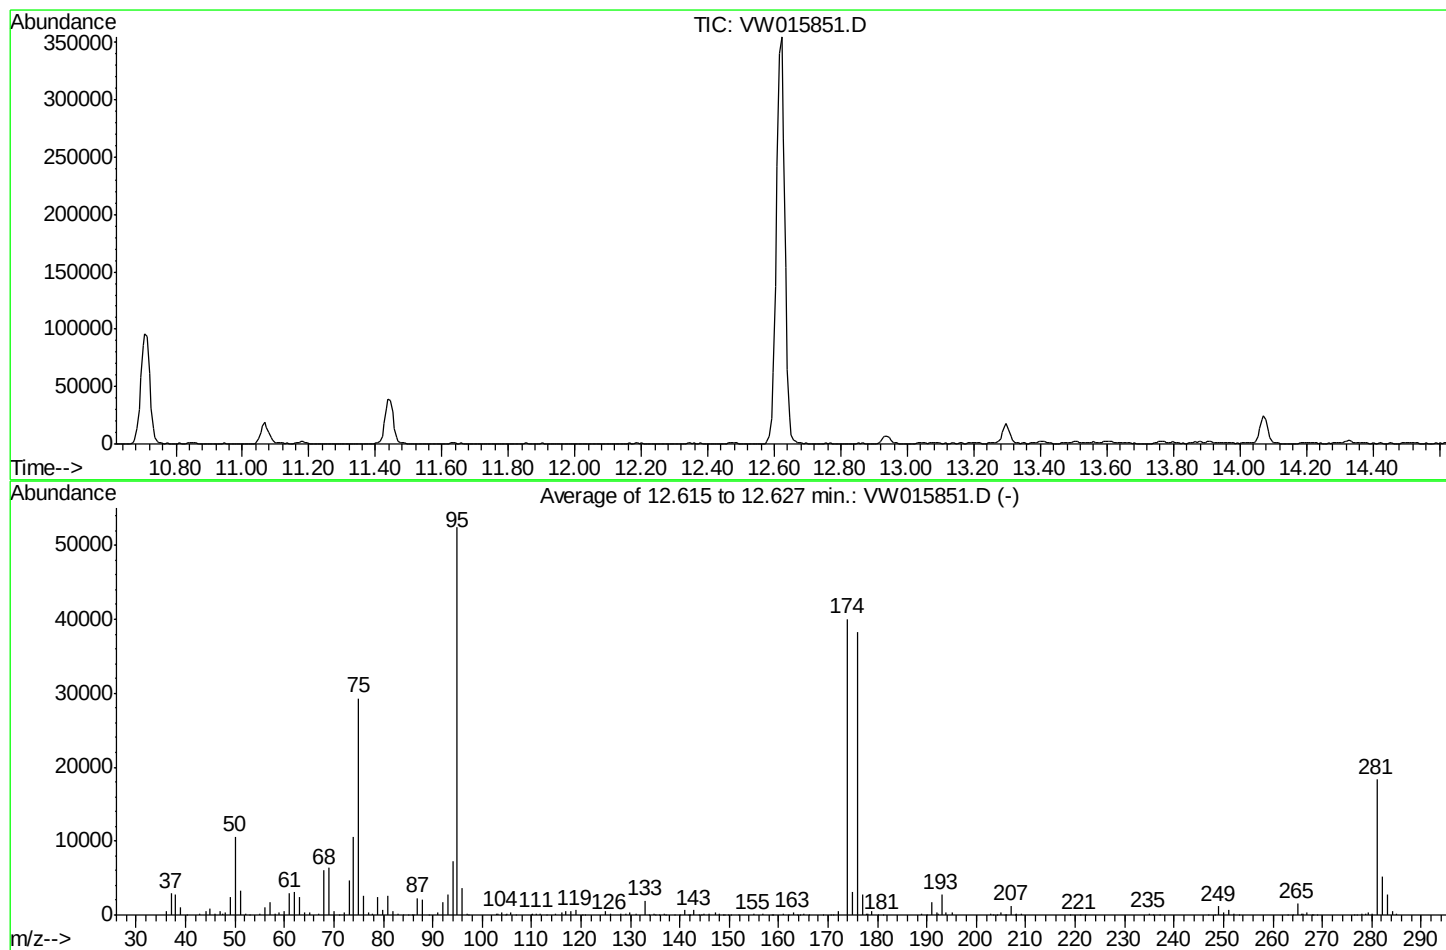

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	10612	PASS
75	95	30	80	55.8	29285	PASS
95	95	100	100	100.0	52440	PASS
96	95	5	9	6.9	3594	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.3	40013	PASS
175	174	5	9	7.9	3143	PASS
176	174	95	101	95.9	38357	PASS
177	176	5	9	7.4	2828	PASS

m/z	Abundance
36.00	656.0
37.00	3009.0
38.00	2971.0
39.00	1136.0
40.10	183.0
42.90	245.0
44.10	746.0
45.10	1166.0
46.00	168.0
46.90	435.0
47.50	301.0
48.00	427.0
49.00	2524.0
50.00	11159.0
51.00	3524.0
52.10	253.0
52.90	122.0
55.00	269.0
56.00	1091.0
57.10	1820.0
58.00	70.0
59.00	643.0
60.00	592.0
61.00	3056.0
62.00	3087.0
63.00	2588.0
64.10	414.0
65.10	335.0
67.00	184.0
68.10	6058.0
69.00	6463.0
70.00	570.0
71.10	69.0
72.10	500.0
73.10	5859.0
74.00	11159.0
75.00	29592.0
76.10	2843.0
77.00	384.0
77.90	278.0
78.90	2583.0
79.90	666.0
81.00	2415.0
81.90	665.0
83.00	124.0
84.10	71.0
85.00	64.0
86.10	69.0
86.90	2140.0
88.00	1963.0
89.10	141.0
91.00	205.0
92.00	1654.0
93.00	2602.0
94.00	6942.0
95.00	52040.0
96.00	3650.0
97.00	195.0
102.80	343.0
103.20	403.0
103.90	401.0
105.00	240.0
105.80	288.0
106.80	60.0
110.10	258.0
111.00	216.0
111.90	178.0
112.90	79.0
114.90	251.0
116.10	343.0
117.00	630.0
118.00	703.0
119.00	774.0
120.90	53.0
125.00	947.0
128.00	185.0
129.00	140.0
129.90	345.0
131.00	126.0
133.00	3116.0
134.90	389.0
135.70	65.0
136.90	197.0
141.00	476.0
142.90	824.0
143.90	81.0
145.00	179.0
145.90	113.0
147.20	323.0
148.00	311.0
149.00	234.0
150.20	101.0

Instrument :
MSVOA_W
ClientSampleId :
BFB19

154.80	151.0
156.80	93.0
158.70	83.0
161.00	196.0
161.90	67.0
163.00	452.0
163.80	125.0
165.10	237.0
170.50	94.0
171.00	141.0
171.90	452.0
174.00	37064.0
175.00	3307.0
175.90	32400.0
177.00	2949.0
177.80	447.0
178.90	805.0
180.00	175.0
181.10	58.0
189.00	292.0
189.90	107.0
191.10	2722.0
192.00	638.0
193.00	4118.0
193.90	725.0
195.10	556.0
203.00	326.0
204.20	124.0
205.00	593.0
205.80	167.0
207.00	1824.0
207.90	272.0
209.00	236.0
218.90	62.0
220.90	142.0
222.00	52.0
234.90	398.0
235.80	98.0
246.90	101.0
249.00	1833.0
250.00	636.0
251.00	987.0
252.10	227.0
253.10	74.0
264.10	101.0
265.00	2261.0
265.90	703.0
267.00	611.0
268.20	117.0
268.90	89.0
276.50	77.0
276.90	109.0
278.00	93.0
278.80	297.0
279.30	442.0
281.10	27496.0
282.00	7729.0
283.10	3816.0
284.20	846.0
285.10	399.0

Instrument :
MSVOA_W
ClientSampleId :
BFB19

m/z	Abundance
36.00	590.0
37.10	3323.0
38.00	3129.0
39.00	1176.0
39.90	208.0
43.00	148.0
44.00	750.0
45.00	862.0
46.10	134.0
47.00	868.0
48.10	239.0
49.00	3148.0
50.00	12107.0
51.00	3579.0
52.10	184.0
52.90	59.0
55.10	274.0
56.00	1239.0
57.10	2005.0
58.00	131.0
58.90	362.0
60.00	735.0
61.10	3507.0
62.00	3550.0
63.10	2983.0
64.00	292.0
65.00	288.0
67.00	216.0
68.00	6705.0
69.00	7213.0
70.00	574.0
72.00	458.0
73.10	4670.0
74.00	11135.0
75.00	31744.0
76.10	2787.0
77.00	384.0
77.90	329.0
78.90	2831.0
80.00	870.0
81.00	2841.0
81.90	558.0
83.00	125.0
85.70	102.0
86.90	2891.0
87.90	2486.0
90.90	415.0
92.00	2123.0
93.00	2977.0
94.00	8409.0
95.00	59384.0
96.00	4133.0
97.00	133.0
102.90	310.0
103.80	504.0
105.00	188.0
105.90	375.0
106.90	104.0
109.80	53.0
110.20	56.0
111.10	229.0
111.70	96.0
112.90	54.0
115.00	242.0
116.00	311.0
116.90	572.0
117.90	447.0
119.00	607.0
120.20	50.0
120.90	55.0
124.90	555.0
125.90	383.0
127.90	330.0
128.90	155.0
129.80	208.0
131.00	145.0
133.00	1762.0
134.80	267.0
136.80	89.0
137.10	97.0
138.80	60.0
139.90	52.0
140.90	746.0
142.00	82.0
142.90	815.0
143.90	60.0
144.90	95.0
145.80	140.0
147.00	378.0
147.90	147.0
148.70	93.0
149.80	75.0

Instrument :
MSVOA_W
ClientSampleId :
BFB19

150.30	50.0
151.80	58.0
154.90	176.0
156.90	130.0
158.90	92.0
160.90	280.0
163.00	291.0
163.80	89.0
164.20	82.0
164.90	333.0
166.20	61.0
169.10	99.0
171.00	71.0
172.00	602.0
173.90	46088.0
175.00	3209.0
175.90	44504.0
176.90	2959.0
178.00	191.0
178.90	681.0
180.00	68.0
188.90	116.0
189.90	93.0
191.10	1525.0
192.10	388.0
193.00	2881.0
194.00	349.0
195.10	384.0
203.00	257.0
205.00	467.0
206.10	108.0
207.10	1227.0
208.10	369.0
209.10	199.0
218.90	67.0
220.90	82.0
235.00	209.0
237.20	81.0
248.10	55.0
249.00	997.0
249.90	248.0
251.10	552.0
252.00	134.0
253.10	81.0
263.00	67.0
265.00	1210.0
266.10	447.0
266.90	354.0
267.80	67.0
268.30	78.0
276.90	66.0
278.10	127.0
279.20	386.0
281.10	18536.0
282.10	5132.0
283.10	3259.0
284.00	553.0
285.10	196.0

Instrument :
MSVOA_W
ClientSampleId :
BFB19

m/z	Abundance
36.00	358.0
37.00	2439.0
38.00	2173.0
39.00	872.0
40.20	181.0
42.90	115.0
44.00	428.0
44.90	420.0
46.00	54.0
47.00	353.0
48.00	334.0
49.00	1822.0
50.00	8571.0
51.00	3042.0
52.10	166.0
55.00	165.0
56.10	773.0
57.00	1365.0
58.00	105.0
59.10	177.0
60.00	492.0
61.00	2470.0
62.00	2593.0
63.00	1943.0
64.00	242.0
65.00	269.0
67.10	88.0
68.00	5628.0
69.00	5791.0
70.00	415.0
72.10	283.0
73.00	3449.0
74.00	9374.0
75.00	26520.0
76.00	2138.0
76.90	374.0
77.90	177.0
78.90	2106.0
80.00	526.0
80.90	2381.0
82.00	594.0
82.90	74.0
86.10	78.0
87.00	1789.0
88.00	1812.0
91.00	183.0
92.00	1627.0
93.00	2571.0
94.00	6589.0
95.00	45896.0
96.10	3000.0
97.20	112.0
103.10	185.0
103.90	372.0
104.70	92.0
105.90	264.0
110.10	87.0
110.90	192.0
111.80	96.0
112.90	115.0
114.80	73.0
116.00	288.0
116.90	339.0
117.90	340.0
118.90	536.0
124.90	185.0
127.90	171.0
128.90	106.0
130.00	274.0
131.10	131.0
133.10	949.0
133.80	204.0
134.70	125.0
135.10	96.0
136.90	112.0
139.90	64.0
140.90	646.0
141.70	71.0
143.00	413.0
144.40	56.0
145.10	92.0
146.00	89.0
147.00	111.0
148.00	199.0
148.80	71.0
149.80	56.0
155.00	171.0
156.90	142.0
158.90	136.0
161.00	120.0
162.90	176.0
165.00	166.0

Instrument :
MSVOA_W
ClientSampleId :
BFB19

169.00	50.0
172.00	325.0
173.90	36888.0
175.00	2914.0
176.00	38168.0
177.00	2578.0
178.10	96.0
179.00	205.0
189.10	131.0
189.70	54.0
191.10	842.0
192.30	310.0
193.00	1132.0
194.10	188.0
195.10	210.0
202.90	76.0
203.30	56.0
205.00	179.0
207.00	618.0
208.00	137.0
209.10	135.0
234.90	109.0
237.10	59.0
249.00	752.0
250.00	174.0
251.00	353.0
252.10	85.0
265.00	1002.0
266.20	261.0
267.00	217.0
268.30	64.0
276.60	57.0
278.00	85.0
278.70	88.0
280.00	406.0
281.10	8946.0
282.10	2702.0
283.00	1491.0
284.10	381.0
285.10	80.0

Instrument :
MSVOA_W
ClientSampleId :
BFB19

Scan 1750 (12.572 min): VW015851.D
BFB19

m/z	Abundance
39.00	65.0
39.90	180.0
43.90	197.0
54.10	58.0
72.80	58.0

Instrument :
MSVOA_W
ClientSampleId :
BFB19