


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071421\
 Data File : VW019473.D
 Acq On : 14 Jul 2021 09:05
 Operator : SY/VA
 Sample : BFB406
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB406

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070921SMA.M
 Title : SFAM01.0
 Last Update : Thu Jul 15 01:04:10 2021

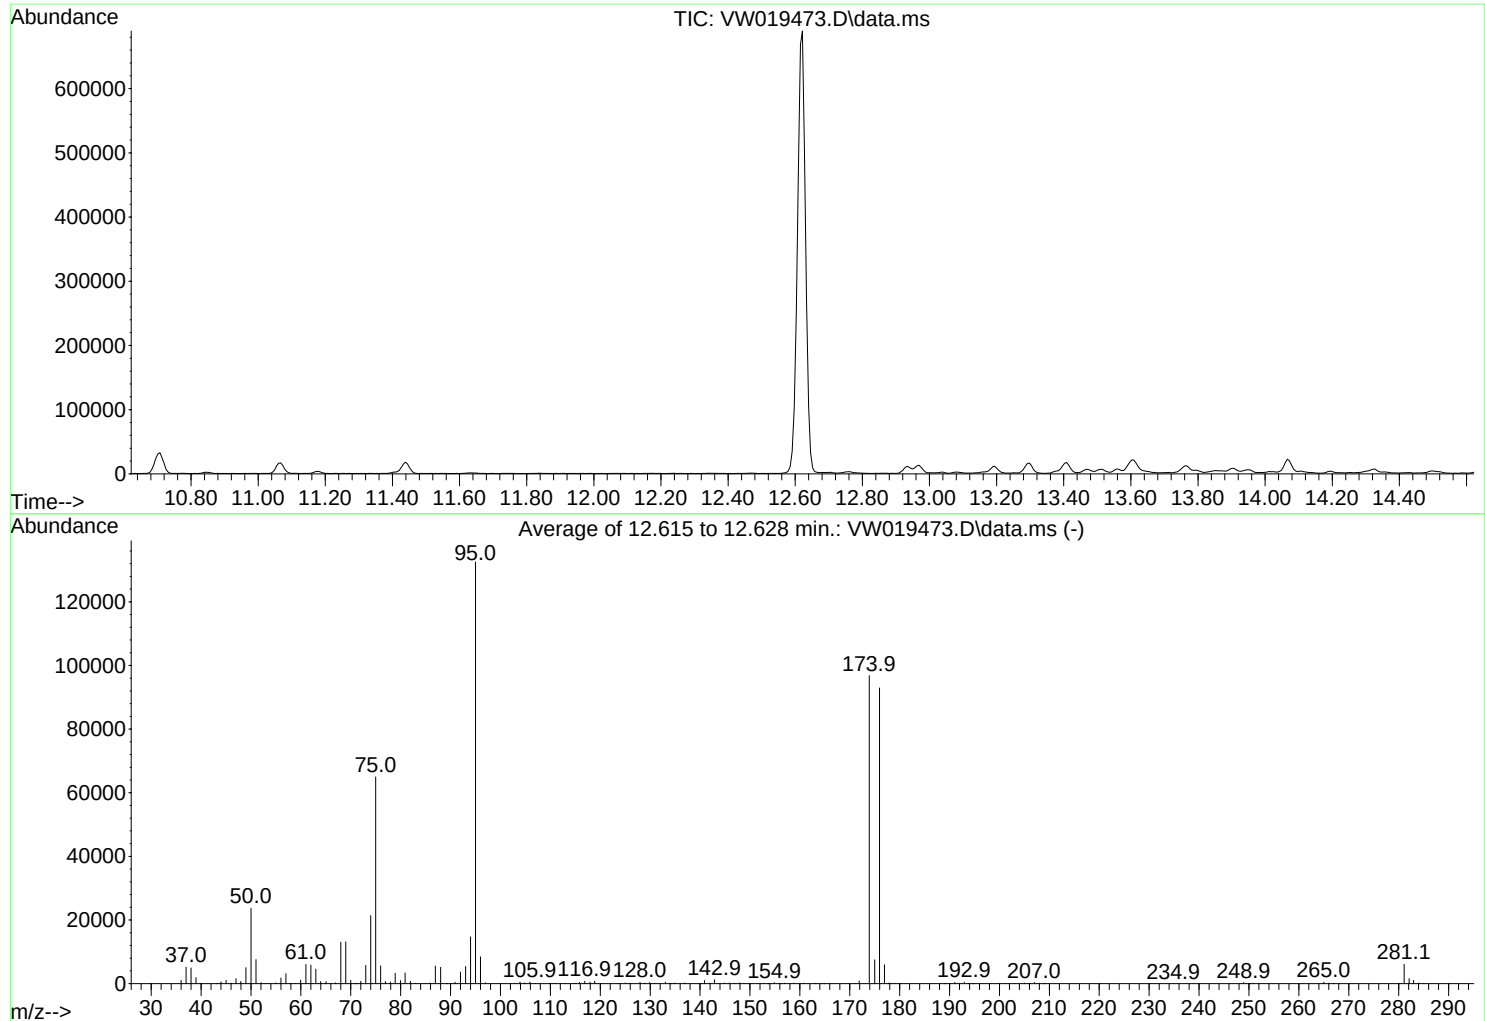

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	23669	PASS
75	95	30	80	49.0	64984	PASS
95	95	100	100	100.0	132568	PASS
96	95	5	9	6.4	8452	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.0	96821	PASS
175	174	5	9	7.7	7487	PASS
176	174	95	105	96.0	92928	PASS
177	176	5	10	6.4	5948	PASS

m/z	Abundance
36.00	1422.0
37.00	5937.0
38.00	5609.0
39.00	2477.0
40.00	299.0
41.10	87.0
42.90	120.0
44.00	1178.0
45.00	1294.0
46.00	199.0
47.00	1959.0
48.00	754.0
49.00	5615.0
50.00	27472.0
51.00	8193.0
52.00	376.0
53.00	135.0
55.10	413.0
56.00	2005.0
57.00	3752.0
57.90	135.0
58.90	188.0
59.90	1324.0
61.00	6671.0
62.00	6762.0
63.00	5014.0
64.00	728.0
65.00	870.0
65.90	123.0
67.00	318.0
68.00	14065.0
69.00	14908.0
70.00	1173.0
70.90	75.0
72.00	764.0
73.00	6700.0
74.00	23056.0
75.00	72328.0
76.00	6374.0
77.00	802.0
78.00	626.0
78.90	3567.0
79.90	1146.0
80.90	3799.0
82.00	795.0
83.00	135.0
84.90	62.0
85.80	209.0
87.00	5635.0
88.00	5680.0
89.20	58.0
91.00	497.0
92.00	3942.0
93.00	5960.0
94.00	16262.0
95.00	144832.0
96.00	9482.0
97.10	268.0
102.80	192.0
103.90	481.0
104.80	226.0
105.90	526.0
107.00	143.0
109.90	142.0
110.70	140.0
112.00	89.0
114.90	170.0
115.80	467.0
116.90	956.0
117.90	654.0
118.90	1001.0
123.80	81.0
125.00	253.0
125.80	136.0
128.00	389.0
129.00	186.0
130.00	349.0
130.90	220.0
133.00	915.0
134.60	190.0
135.00	241.0
136.90	203.0
140.00	116.0
140.90	1131.0
142.00	152.0
142.90	1490.0
143.80	109.0
144.90	293.0
145.80	159.0
147.00	183.0
147.90	358.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

m/z	Abundance
35.90	75.0
39.10	60.0
40.00	262.0
41.10	109.0
43.00	79.0
44.00	457.0
55.10	59.0
56.00	83.0
57.10	183.0
71.00	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

148.90	136.0
150.00	115.0
152.90	90.0
153.60	70.0
154.90	238.0
156.90	197.0
158.80	114.0
160.80	147.0
162.90	176.0
164.80	81.0
171.10	167.0
171.90	998.0
173.90	97712.0
175.00	7408.0
175.90	87464.0
177.00	6771.0
177.90	248.0
179.00	207.0
179.90	53.0
189.00	75.0
191.00	701.0
192.00	192.0
193.00	777.0
193.90	157.0
194.70	52.0
203.00	113.0
205.00	253.0
205.90	53.0
207.10	571.0
207.90	132.0
208.90	59.0
234.90	108.0
249.00	574.0
249.90	179.0
250.90	271.0
265.10	634.0
266.00	198.0
266.90	226.0
281.10	9688.0
282.10	2447.0
283.00	1460.0
284.10	290.0
285.10	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

m/z	Abundance
36.10	1204.0
37.00	5814.0
38.00	5633.0
39.00	2062.0
39.90	281.0
43.00	113.0
44.00	1133.0
45.00	1089.0
45.90	208.0
47.00	1674.0
47.90	714.0
49.00	5440.0
50.00	25680.0
51.00	8465.0
52.10	302.0
52.90	87.0
54.90	359.0
56.00	2178.0
57.00	3610.0
58.10	110.0
58.90	82.0
60.00	1262.0
61.00	6631.0
62.00	6270.0
63.00	5307.0
64.00	611.0
65.10	729.0
66.90	266.0
68.00	15154.0
69.00	14229.0
70.00	1124.0
71.00	82.0
72.00	899.0
73.00	6208.0
74.00	23664.0
75.00	72728.0
76.00	6030.0
76.90	770.0
77.90	562.0
78.90	3637.0
79.90	1004.0
80.90	3739.0
81.90	881.0
83.00	67.0
85.00	53.0
85.90	185.0
87.00	6316.0
88.00	5495.0
90.80	506.0
92.00	4200.0
93.00	5718.0
94.00	16000.0
95.00	147392.0
96.00	9265.0
97.10	303.0
103.10	183.0
103.90	583.0
104.90	204.0
105.90	585.0
106.90	110.0
110.00	70.0
110.90	118.0
112.00	90.0
112.90	89.0
114.90	162.0
115.90	459.0
116.90	817.0
118.00	439.0
118.90	836.0
123.70	56.0
125.00	221.0
125.80	132.0
128.00	468.0
129.00	204.0
129.90	482.0
130.90	221.0
133.10	419.0
133.90	116.0
134.90	249.0
137.00	222.0
140.00	81.0
140.90	1114.0
141.80	162.0
142.90	1198.0
143.80	68.0
144.90	229.0
145.90	203.0
146.80	108.0
148.00	221.0
148.70	99.0
149.80	139.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

m/z	Abundance
36.00	800.0
37.00	3807.0
38.00	3579.0
39.00	1312.0
40.00	266.0
43.10	70.0
44.00	809.0
45.00	829.0
46.10	113.0
47.00	995.0
48.00	631.0
49.00	3972.0
50.00	17856.0
51.00	5938.0
52.00	223.0
52.90	120.0
55.00	208.0
55.90	1340.0
57.00	2612.0
58.10	128.0
60.00	735.0
61.00	4863.0
62.00	4432.0
63.00	3382.0
63.90	557.0
65.00	449.0
67.00	210.0
68.00	9928.0
69.00	10231.0
70.00	719.0
71.00	64.0
72.00	551.0
73.00	4362.0
74.00	17368.0
75.00	49896.0
76.00	4288.0
76.90	614.0
77.90	360.0
78.90	2549.0
80.00	789.0
80.90	2646.0
81.90	510.0
82.80	71.0
86.00	159.0
86.90	4653.0
88.00	4209.0
90.90	328.0
92.00	2695.0
93.00	4505.0
94.00	11849.0
95.00	105480.0
96.00	6608.0
96.90	203.0
102.80	81.0
103.90	441.0
104.90	148.0
105.90	412.0
107.10	86.0
110.00	69.0
111.00	102.0
112.90	62.0
114.90	109.0
115.90	283.0
116.90	565.0
118.00	331.0
118.90	444.0
124.90	77.0
125.90	87.0
127.80	374.0
128.90	185.0
129.80	284.0
130.80	108.0
132.90	173.0
134.10	73.0
134.90	159.0
136.90	185.0
140.90	865.0
141.90	126.0
142.90	930.0
144.90	158.0
146.00	195.0
146.90	90.0
148.00	210.0
148.80	64.0
149.70	99.0
152.90	80.0
153.80	52.0
154.90	240.0
156.90	166.0
158.90	127.0
160.90	140.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

152.80	114.0
153.80	83.0
154.90	417.0
156.00	51.0
157.00	182.0
158.90	152.0
160.60	120.0
160.90	114.0
163.10	56.0
171.00	125.0
171.90	910.0
173.90	106144.0
175.00	8507.0
176.00	109168.0
177.00	6364.0
177.80	168.0
178.10	164.0
178.90	73.0
191.10	424.0
192.00	136.0
192.90	437.0
193.80	95.0
203.00	72.0
205.00	143.0
206.90	372.0
208.00	81.0
248.90	310.0
250.10	94.0
251.00	106.0
264.90	491.0
266.10	129.0
267.00	112.0
281.10	6361.0
282.10	1554.0
283.00	969.0
284.10	180.0
285.00	50.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406

170.90	60.0
171.90	645.0
173.90	86608.0
175.00	6547.0
175.90	82152.0
176.90	4710.0
177.90	194.0
178.80	67.0
191.10	143.0
191.90	51.0
192.90	192.0
205.10	70.0
207.10	144.0
208.00	79.0
249.00	183.0
264.90	274.0
266.00	57.0
267.10	65.0
280.20	106.0
281.10	2194.0
282.10	736.0
283.00	537.0
283.90	92.0
285.10	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB406