
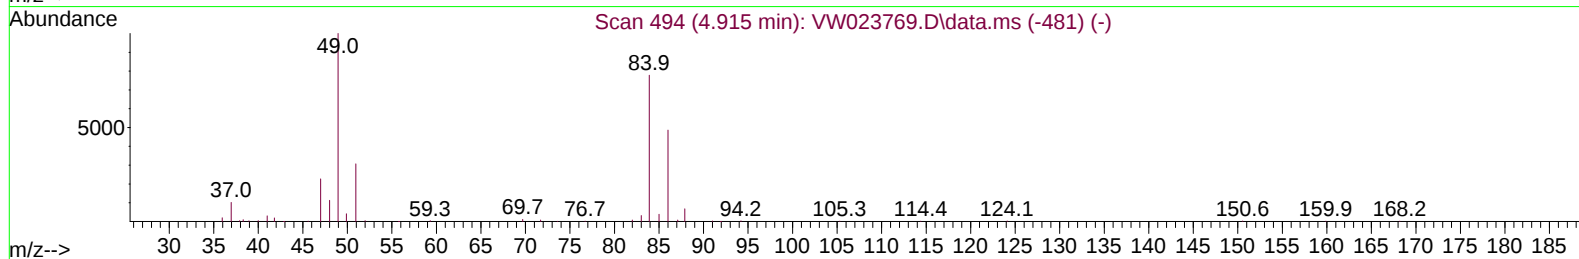
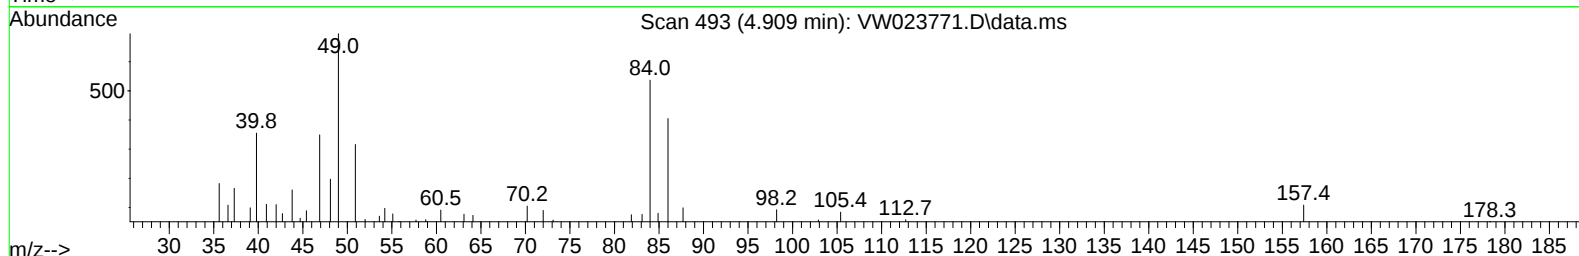


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023771.D
Acq On : 16 Jul 2022 02:21
Operator : SY/VA
Sample : N3700-15RE
Misc : 5.65g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 04:46:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 16 01:30:01 2022
Response via : Initial Calibration

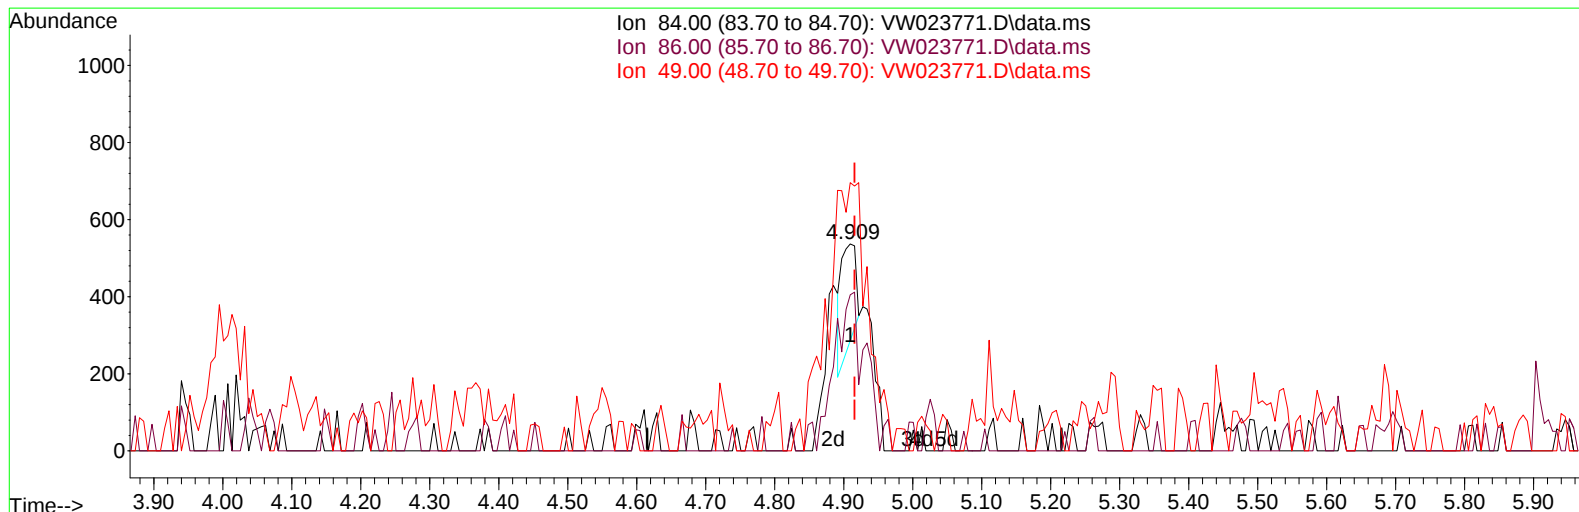

TIC: VW023771.D\data.ms

(16) Methylene chloride (T)

4.909min (-0.006) 0.82 ug/L

response 399

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	75.42
49.00	122.00	129.61
0.00	0.00	0.00