

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023761.D
 Acq On : 15 Jul 2022 21:51
 Operator : SY/VA
 Sample : N3698-16
 Misc : 5.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C03

Quant Time: Jul 15 22:19:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	190735	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	187256	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	78745	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	91199	18.721	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.880%
7) Chloroethane-d5	2.879	69	71871	22.115	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.440%
11) 1,1-Dichloroethene-d2	4.007	63	47814	12.053	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.200%
21) 2-Butanone-d5	7.086	46	34864	46.139	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.280%
24) Chloroform-d	7.647	84	119517	21.522	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.080%
26) 1,2-Dichloroethane-d4	8.305	65	71378	21.016	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.080%
32) Benzene-d6	8.275	84	214281	22.013	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.040%
36) 1,2-Dichloropropane-d6	9.274	67	68006	23.193	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.760%
41) Toluene-d8	10.323	98	194773	19.727	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.920%
43) trans-1,3-Dichloroprop...	10.579	79	24291	17.674	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.680%
47) 2-Hexanone-d5	10.920	63	26617	43.170	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.340%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	65971	20.359	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	64875	23.079	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.320%
Target Compounds						
13) Acetone	4.129	43	9699	18.155	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023761.D
Acq On : 15 Jul 2022 21:51
Operator : SY/VA
Sample : N3698-16
Misc : 5.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C03

Quant Time: Jul 15 22:19:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

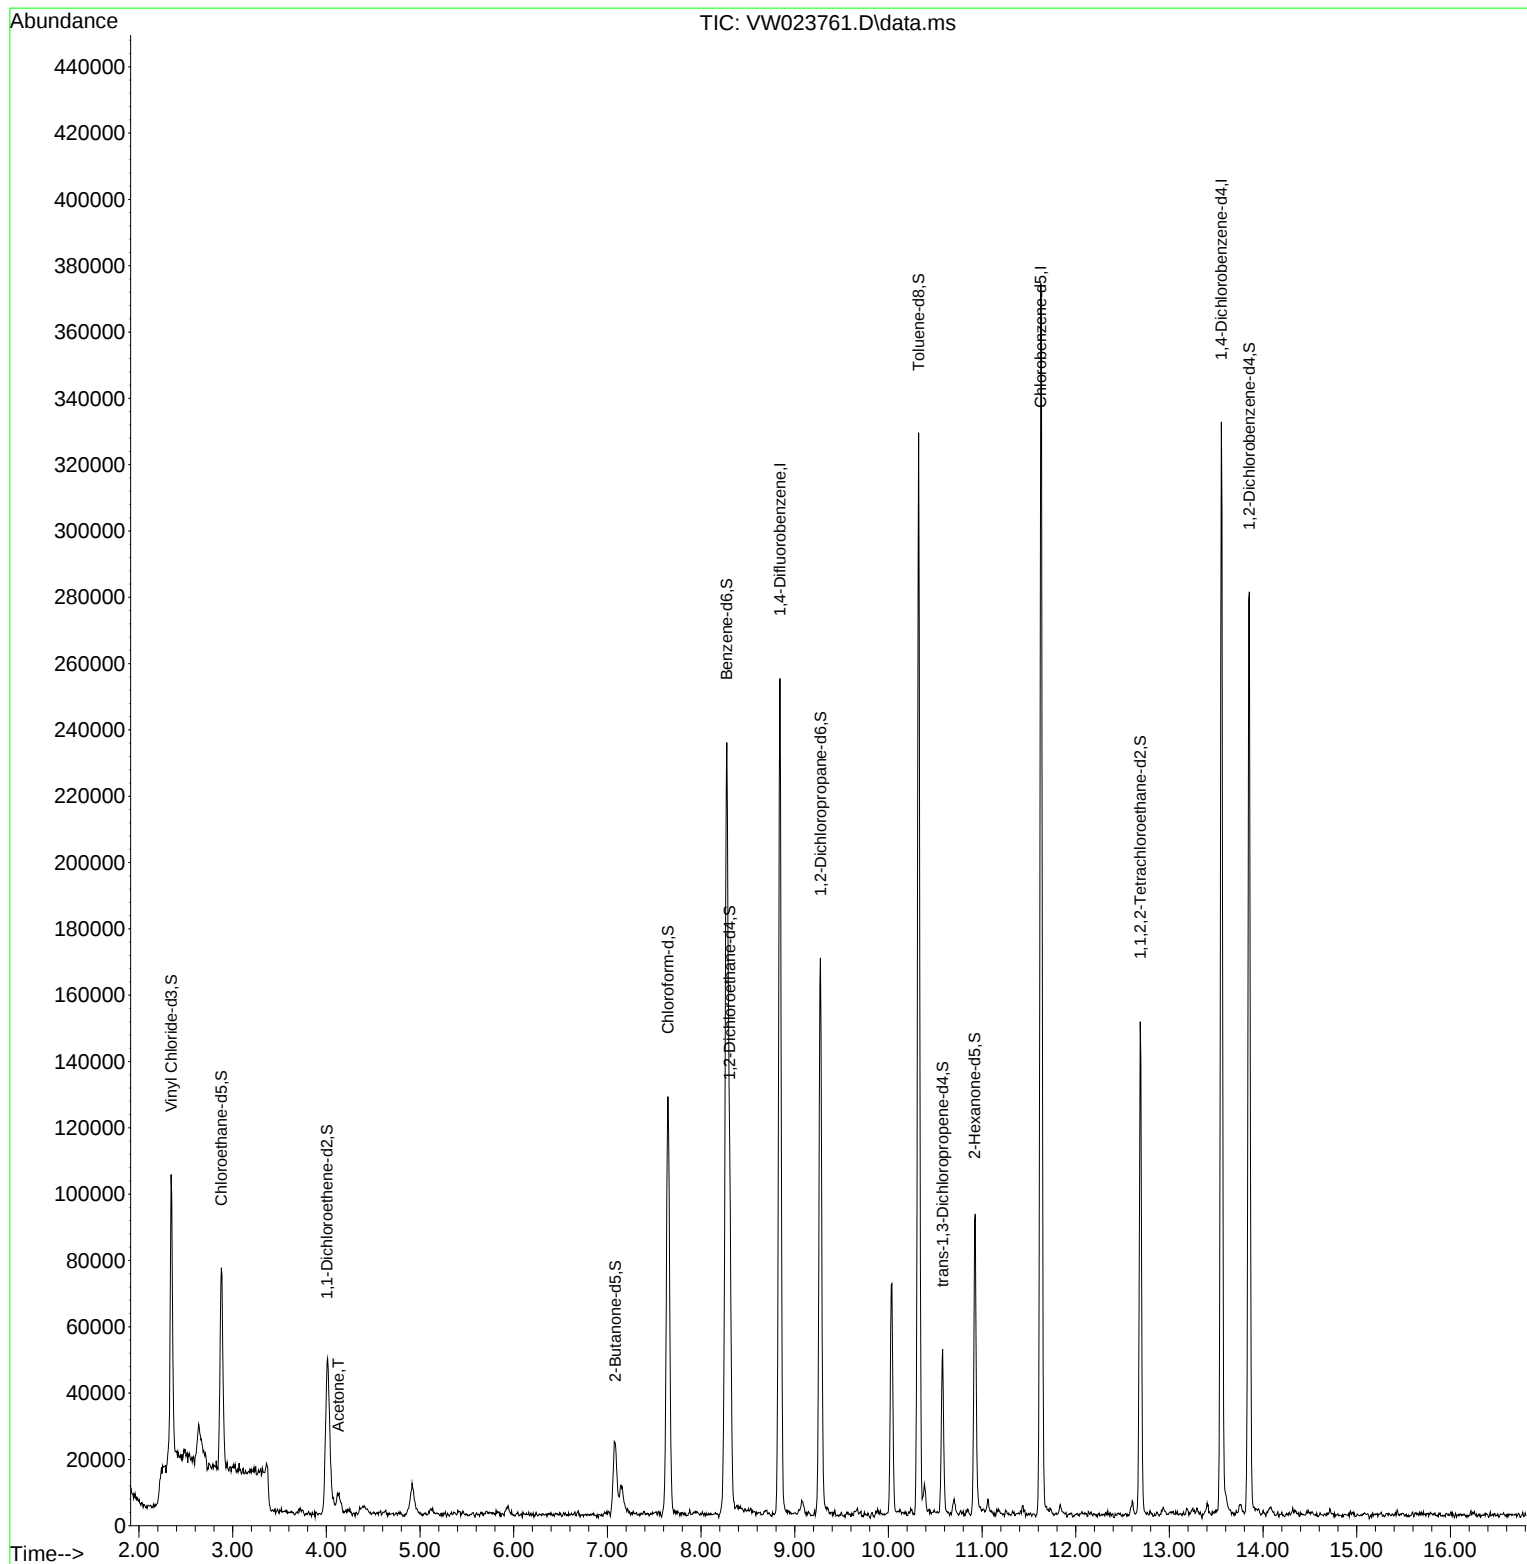

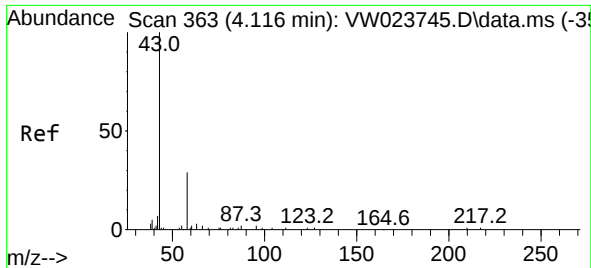

#13
 Acetone
 Concen: 18.155 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.013 min
 Lab File: VW023761.D
 Acq: 15 Jul 2022 21:51

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C03

Tgt Ion: 43 Resp: 9699
 Ion Ratio Lower Upper
 43 100
 58 26.8 0.0 64.2

