




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023747.D
 Acq On : 15 Jul 2022 16:07
 Operator : SY/VA
 Sample : N3678-20
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:16:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

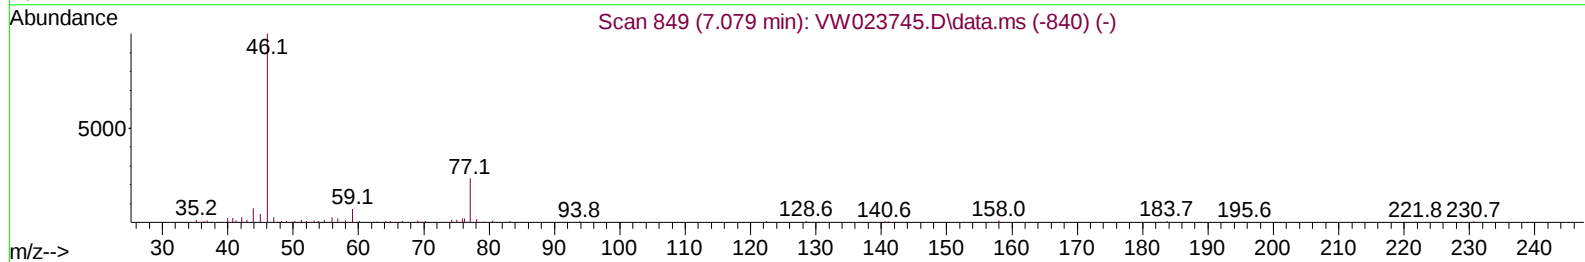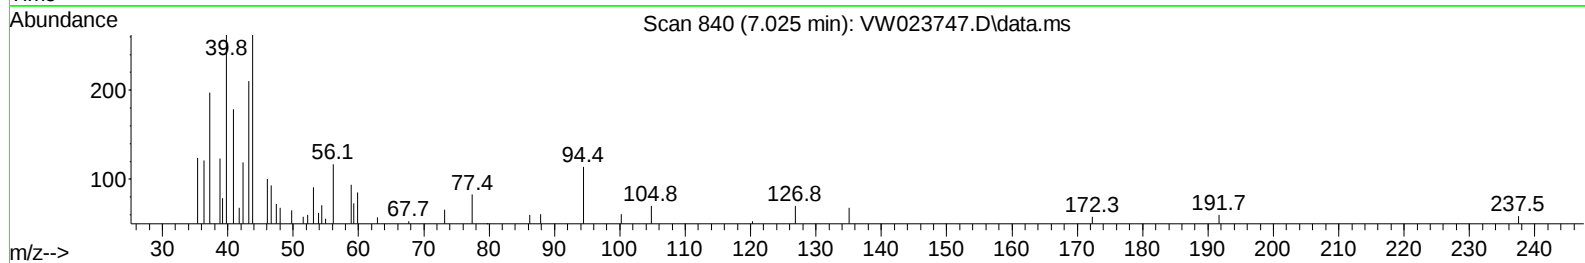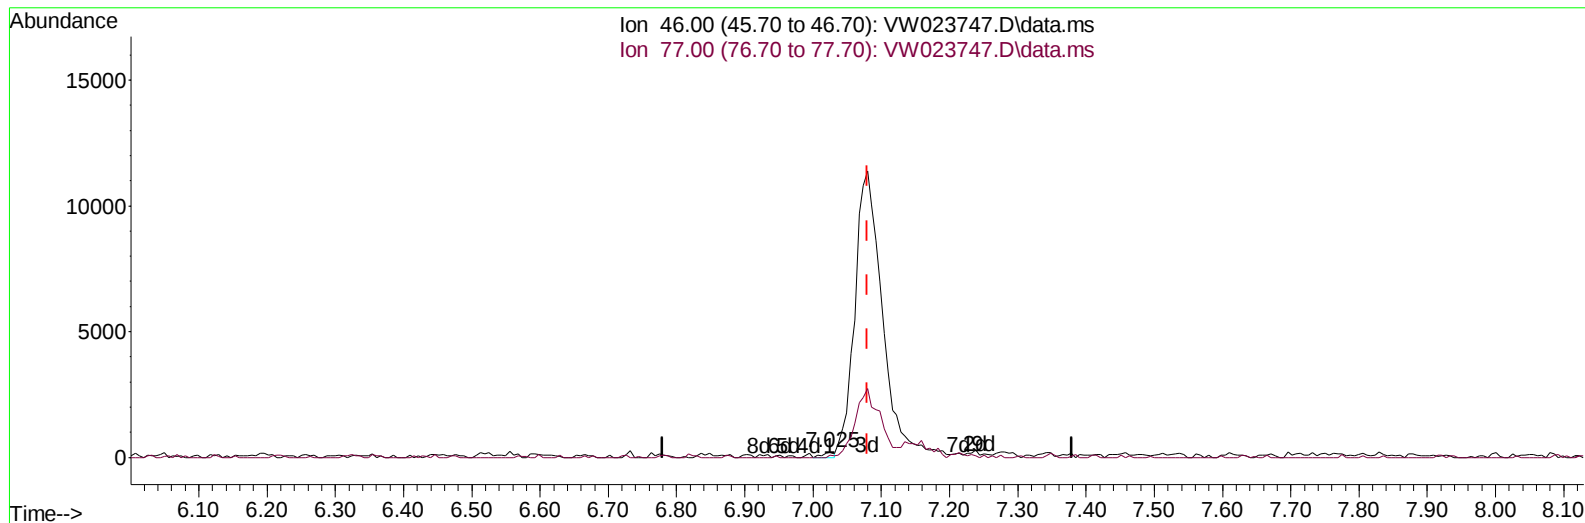

TIC: VW023747.D\data.ms

(21) 2-Butanone-d5 (S)

7.025min (-0.054) 0.39 ug/L

response	251
Ion	Exp% Act%
46.00	100.00 100.00
77.00	25.70 21.12
0.00	0.00 0.00
0.00	0.00 0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023747.D
 Acq On : 15 Jul 2022 16:07
 Operator : SY/VA
 Sample : N3678-20
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:16:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

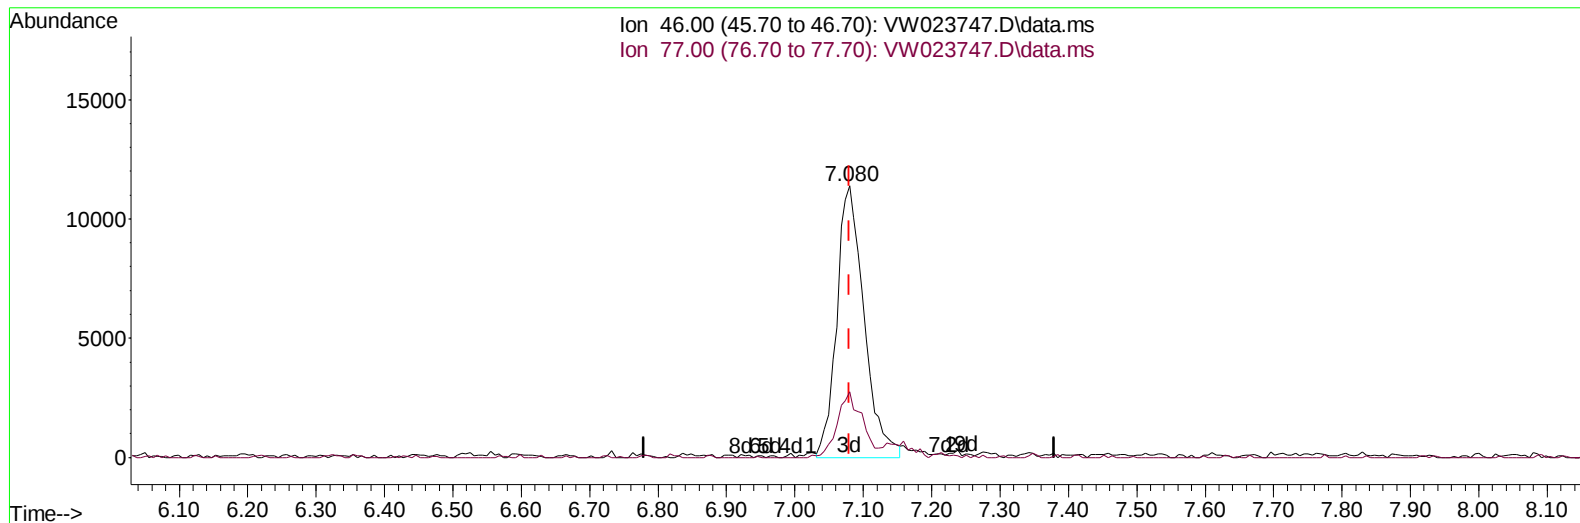

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023747.D
 Acq On : 15 Jul 2022 16:07
 Operator : SY/VA
 Sample : N3678-20
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:16:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		162134	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		166395	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		74538	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		133062	32.133	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	128.520%	
7) Chloroethane-d5	2.879	69		84271	30.505	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	122.000%	
11) 1,1-Dichloroethene-d2	4.007	63		54693	16.220	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	64.880%	
21) 2-Butanone-d5	7.080	46		31475m	49.002	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	98.000%	
24) Chloroform-d	7.647	84		110948	23.504	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	94.000%	
26) 1,2-Dichloroethane-d4	8.305	65		69896	24.210	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	96.840%	
32) Benzene-d6	8.275	84		217468	25.142	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	100.560%	
36) 1,2-Dichloropropane-d6	9.275	67		65227	25.035	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	100.120%	
41) Toluene-d8	10.323	98		201316	22.946	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	91.800%	
43) trans-1,3-Dichloroprop...	10.573	79		27775	22.743	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	90.960%	
47) 2-Hexanone-d5	10.921	63		24933	45.509	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	91.020%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		59839	20.782	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	83.120%	
66) 1,2-Dichlorobenzene-d4	13.847	152		69266	26.032	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	104.120%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023747.D
Acq On : 15 Jul 2022 16:07
Operator : SY/VA
Sample : N3678-20
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:16:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

