




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023752.D
 Acq On : 15 Jul 2022 18:10
 Operator : SY/VA
 Sample : N3658-11
 Misc : 6.74g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AH1

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:17:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

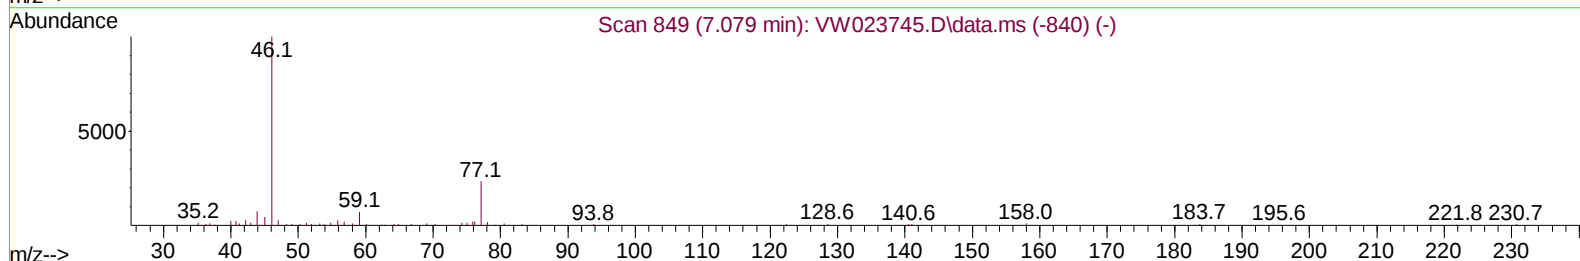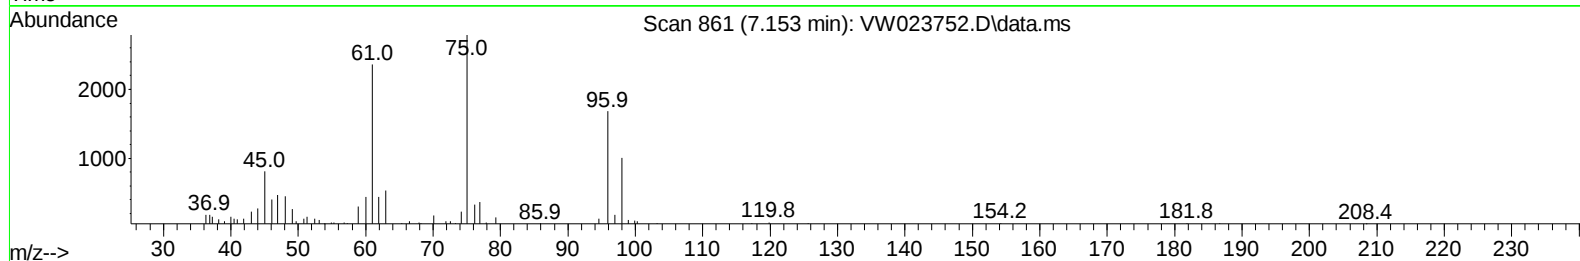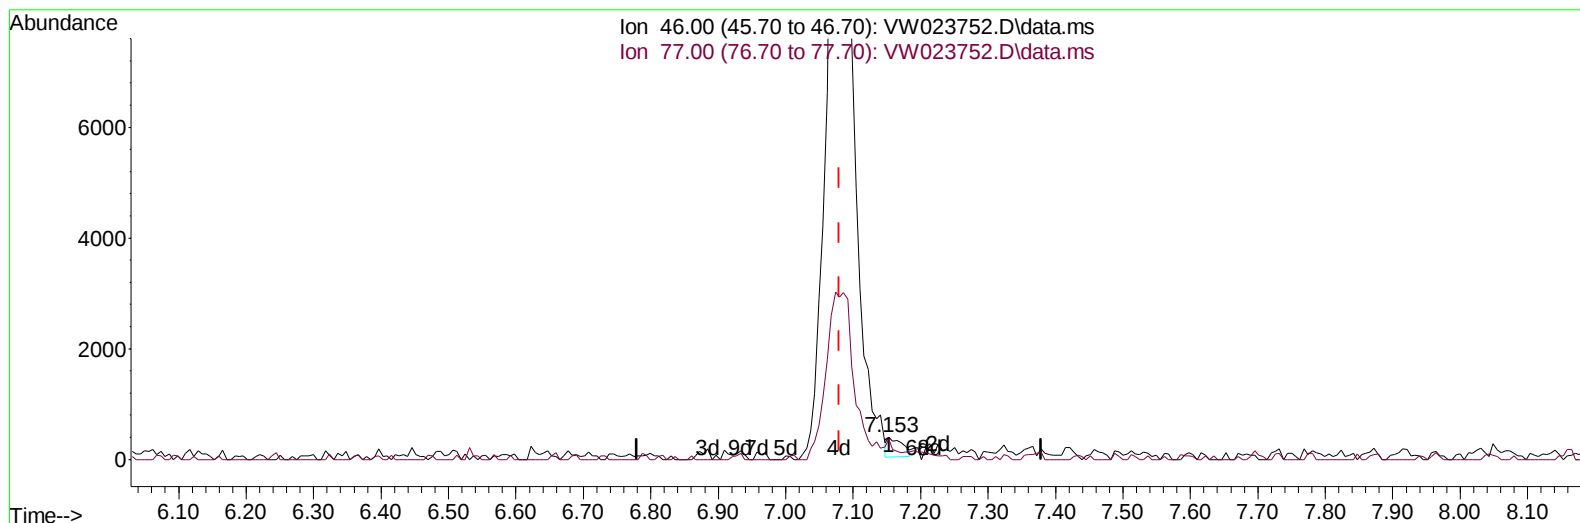

TIC: VW023752.D\data.ms

(21) 2-Butanone-d5 (S)

7.153min (+ 0.074) 0.89 ug/L

response 550

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	30.73
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023752.D
 Acq On : 15 Jul 2022 18:10
 Operator : SY/VA
 Sample : N3658-11
 Misc : 6.74g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AH1

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:17:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

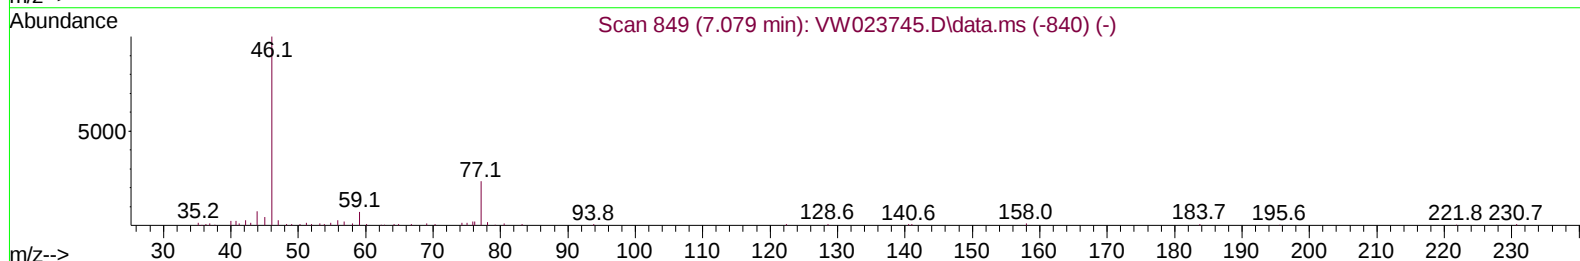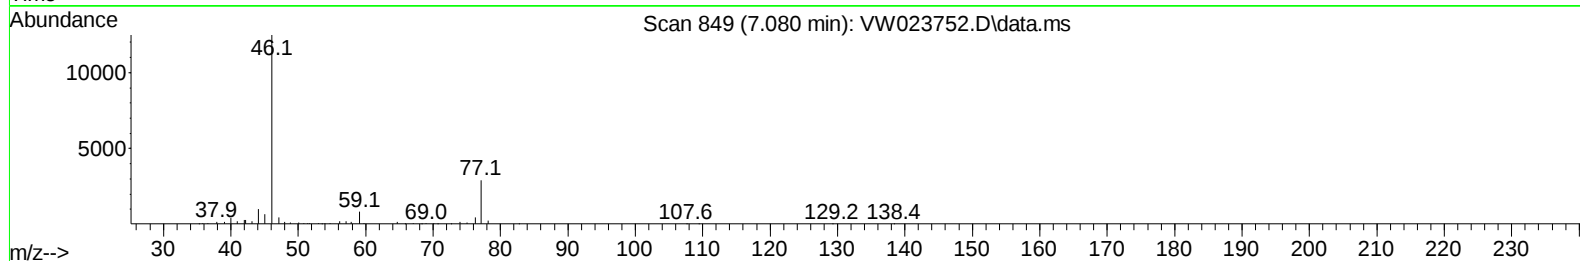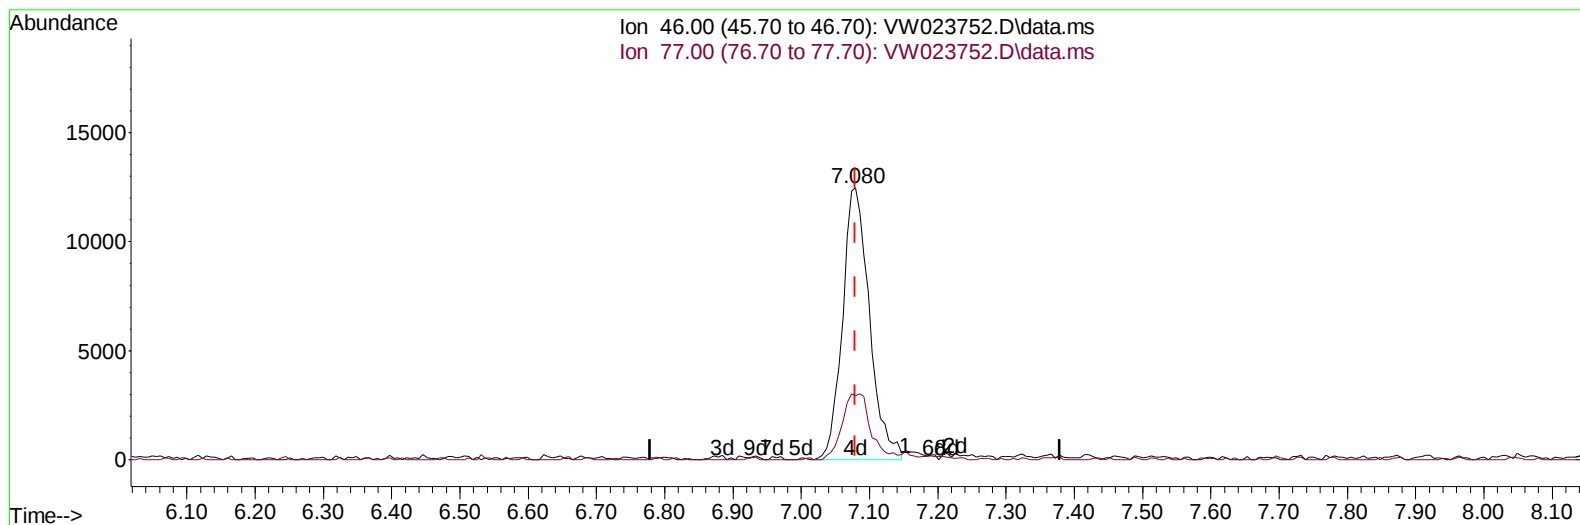

TIC: VW023752.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.000) 55.22 ug/L m

response 34139

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	0.50#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023752.D
 Acq On : 15 Jul 2022 18:10
 Operator : SY/VA
 Sample : N3658-11
 Misc : 6.74g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 COAH1

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:17:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	156069	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	156663	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	68351	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	74301	18.640	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.560%	
7) Chloroethane-d5	2.879	69	57137	21.486	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	85.960%	
11) 1,1-Dichloroethene-d2	4.007	63	37320	11.498	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	46.000%	
21) 2-Butanone-d5	7.080	46	34139m	55.215	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	110.440%	
24) Chloroform-d	7.647	84	94460	20.788	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	83.160%	
26) 1,2-Dichloroethane-d4	8.305	65	60077	21.618	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	86.480%	
32) Benzene-d6	8.275	84	164175	20.159	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	80.640%	
36) 1,2-Dichloropropane-d6	9.268	67	55406	22.586	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	90.360%	
41) Toluene-d8	10.323	98	152162	18.420	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	73.680%	
43) trans-1,3-Dichloroprop...	10.579	79	20924	18.197	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	72.800%	
47) 2-Hexanone-d5	10.920	63	24845	48.165	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	96.320%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	62007	22.873	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	91.480%	
66) 1,2-Dichlorobenzene-d4	13.853	152	58689	24.053	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	96.200%	
Target Compounds						
					Qvalue	
20) cis-1,2-Dichloroethene	7.165	96	5926	2.665	ug/L #	88
34) Trichloroethene	9.092	95	3011	1.281	ug/L	80
46) Tetrachloroethene	10.860	164	11662	6.415	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023752.D
Acq On : 15 Jul 2022 18:10
Operator : SY/VA
Sample : N3658-11
Misc : 6.74g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AH1

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 22:17:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

