




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023757.D
 Acq On : 15 Jul 2022 20:13
 Operator : SY/VA
 Sample : N3698-12
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B99

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:18:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

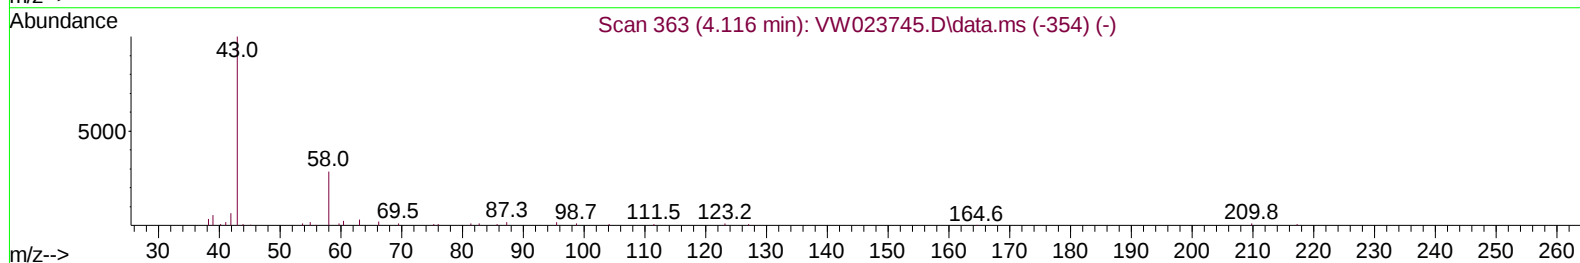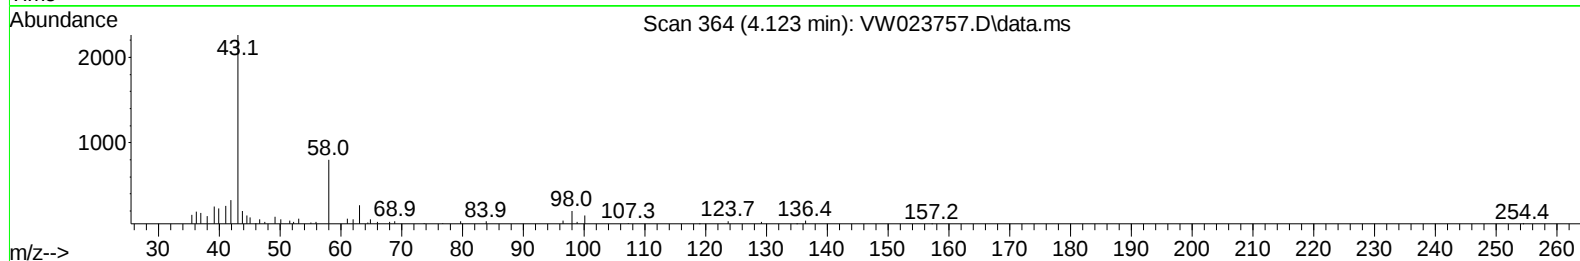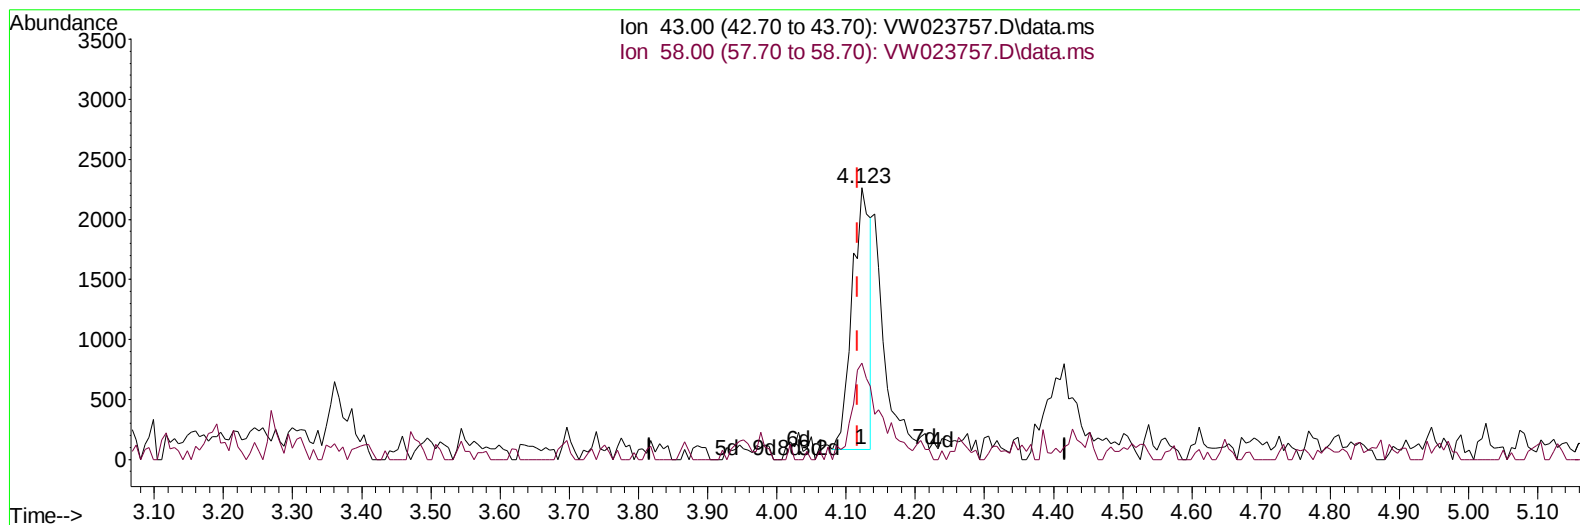

TIC: VW023757.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 6.98 ug/L

response 3965

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	31.63
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023757.D
 Acq On : 15 Jul 2022 20:13
 Operator : SY/VA
 Sample : N3698-12
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B99

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:18:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

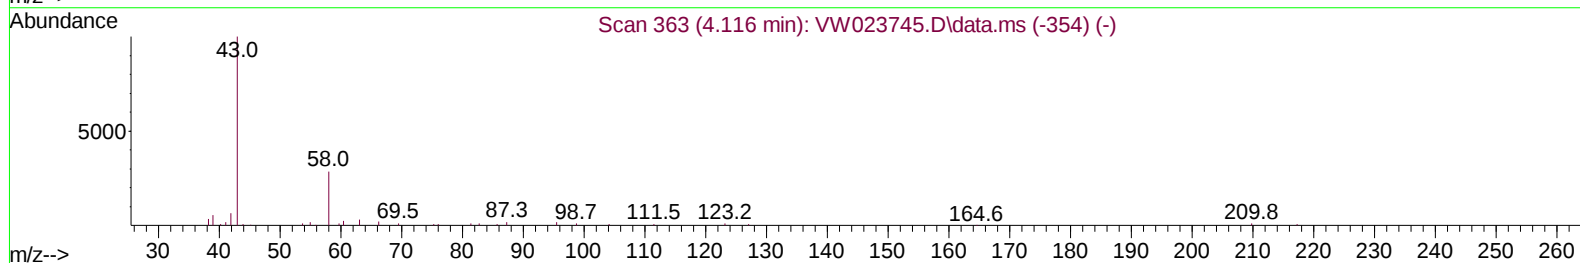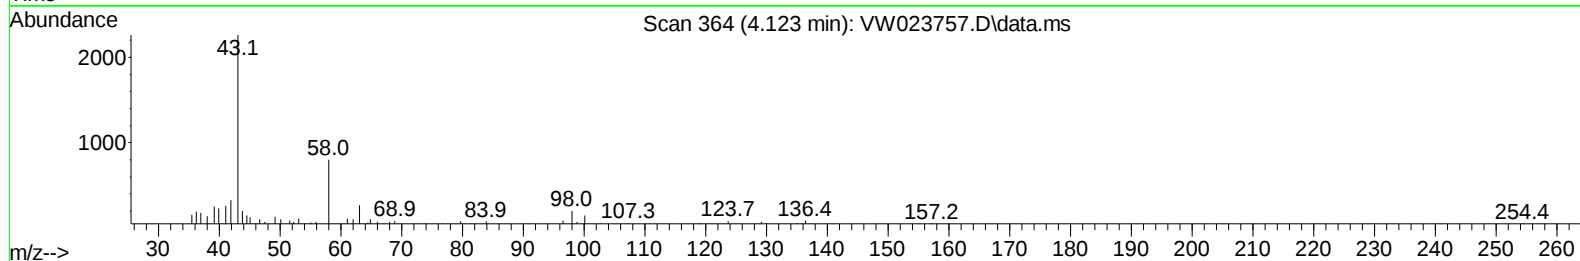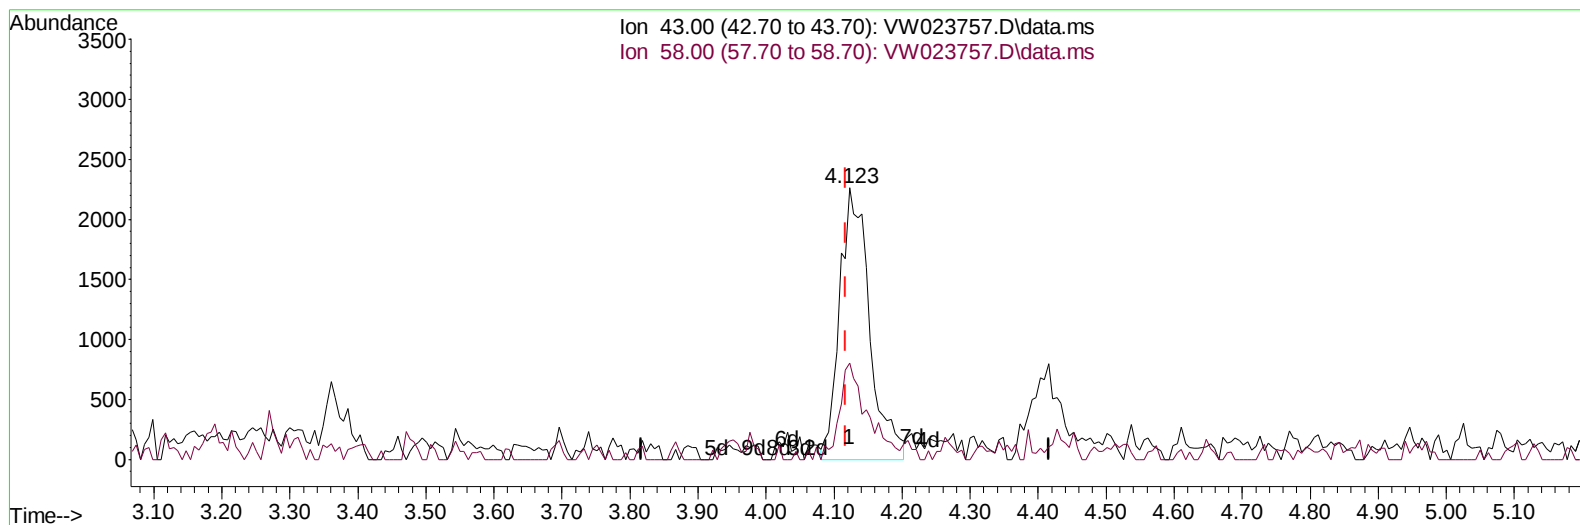

TIC: VW023757.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 12.10 ug/L m

response 6873

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	18.25
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023757.D
 Acq On : 15 Jul 2022 20:13
 Operator : SY/VA
 Sample : N3698-12
 Misc : 6.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B99

Manual IntegrationsAPPROVED

Quant Time: Jul 15 22:18:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		202844	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		190237	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		79165	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		93631	18.073	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	72.280%	
7) Chloroethane-d5	2.879	69		74394	21.525	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	86.080%	
11) 1,1-Dichloroethene-d2	4.007	63		48546	11.507	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	46.040%	
21) 2-Butanone-d5	7.080	46		29884	37.188	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	74.380%	
24) Chloroform-d	7.647	84		116169	19.671	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	78.680%	
26) 1,2-Dichloroethane-d4	8.305	65		68277	18.903	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	75.600%	
32) Benzene-d6	8.275	84		205631	20.794	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	83.160%	
36) 1,2-Dichloropropane-d6	9.274	67		66534	22.336	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	89.360%	
41) Toluene-d8	10.323	98		189285	18.870	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	75.480%	
43) trans-1,3-Dichloroprop...	10.579	79		21732	15.564	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	62.240%	
47) 2-Hexanone-d5	10.927	63		23881	38.126	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	76.260%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		61464	18.671	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	74.680%	
66) 1,2-Dichlorobenzene-d4	13.847	152		61121	21.628	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	86.520%	
Target Compounds							
13) Acetone	4.123	43		6873m	12.097	ug/L	
14) Carbon disulfide	4.379	76		15377	2.431	ug/L #	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023757.D
Acq On : 15 Jul 2022 20:13
Operator : SY/VA
Sample : N3698-12
Misc : 6.45g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B99

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 22:18:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

