




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023766.D
 Acq On : 15 Jul 2022 23:54
 Operator : SY/VA
 Sample : N3700-06RE
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C13RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:32:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

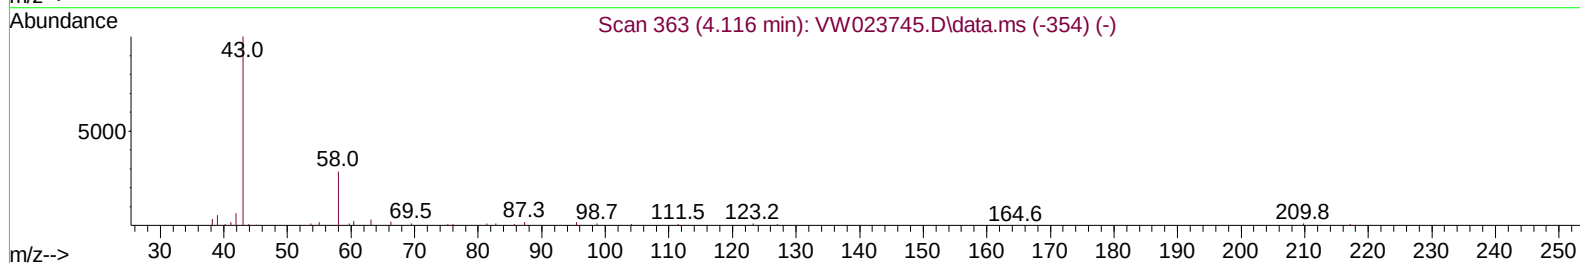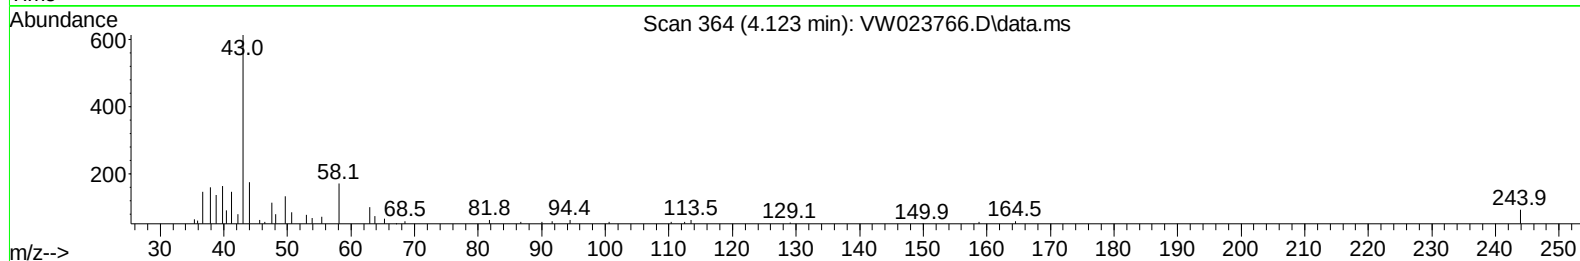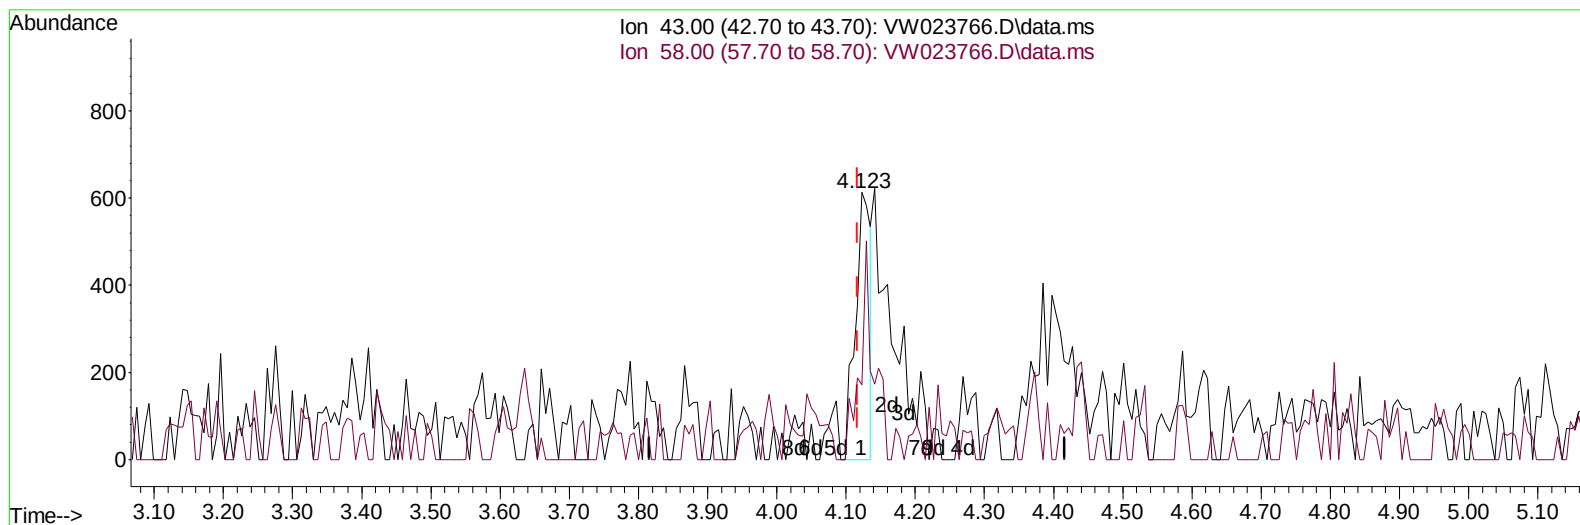

TIC: VW023766.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 26.59 ug/L

response 928

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	57.87
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023766.D
 Acq On : 15 Jul 2022 23:54
 Operator : SY/VA
 Sample : N3700-06RE
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C13RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:32:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

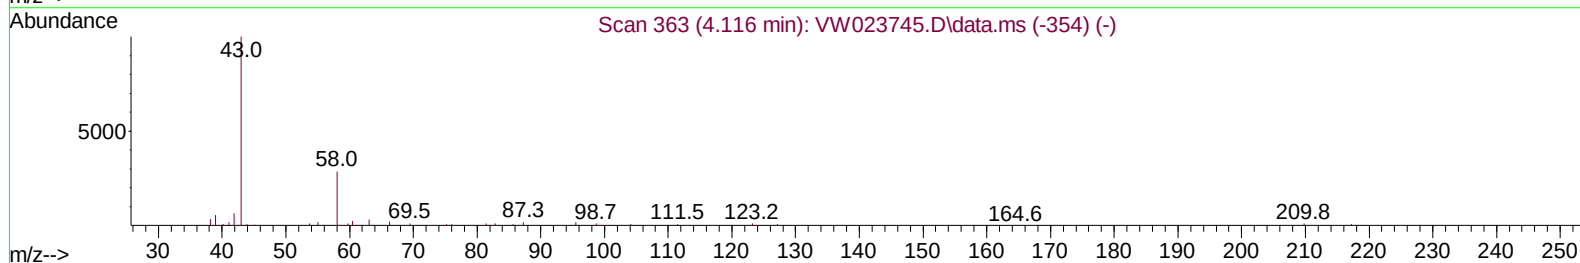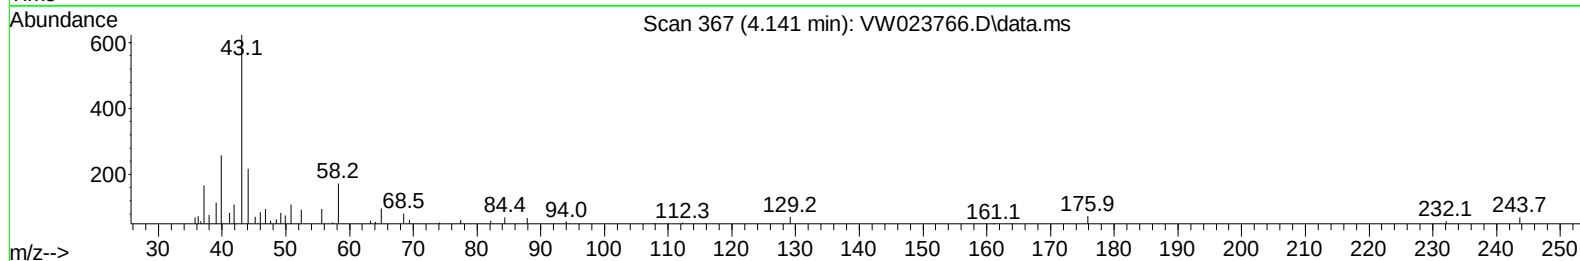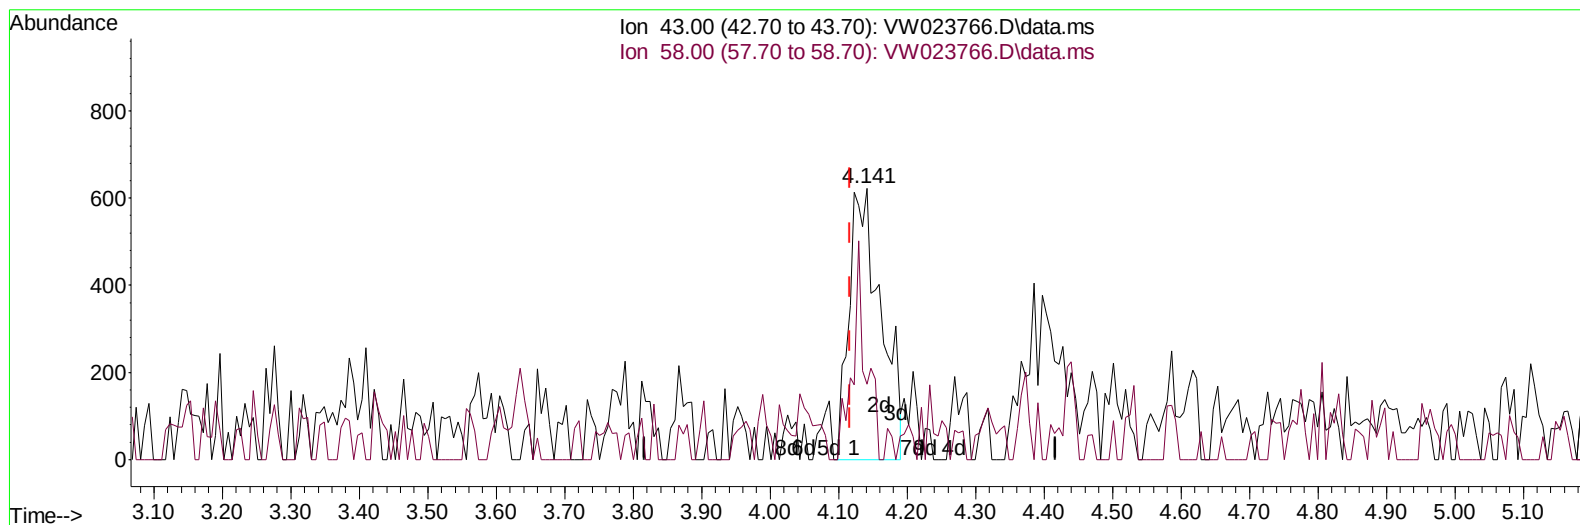

TIC: VW023766.D\data.ms

(13) Acetone (T)

4.141min (+ 0.025) 57.34 ug/L m

response	2001	
Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	26.84
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023766.D
 Acq On : 15 Jul 2022 23:54
 Operator : SY/VA
 Sample : N3700-06RE
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C13RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:32:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

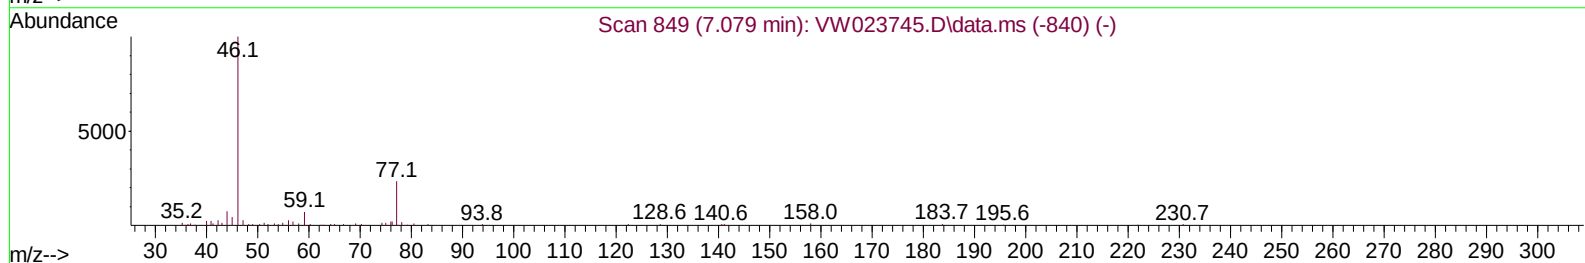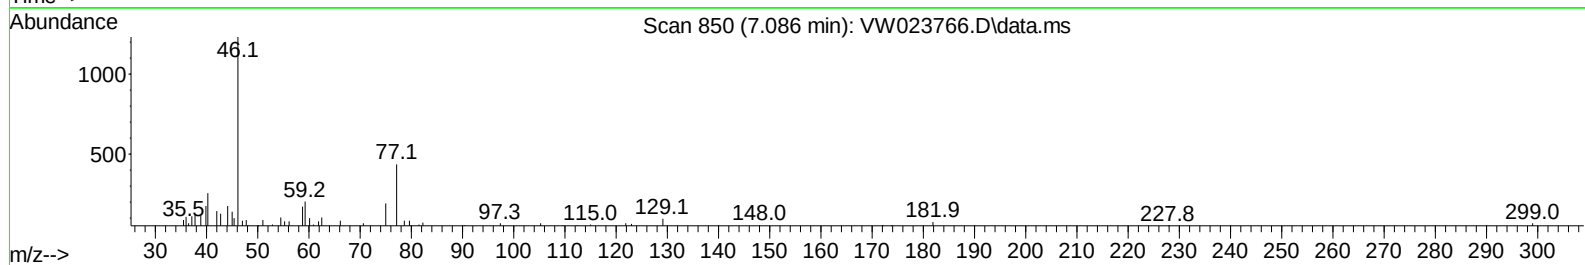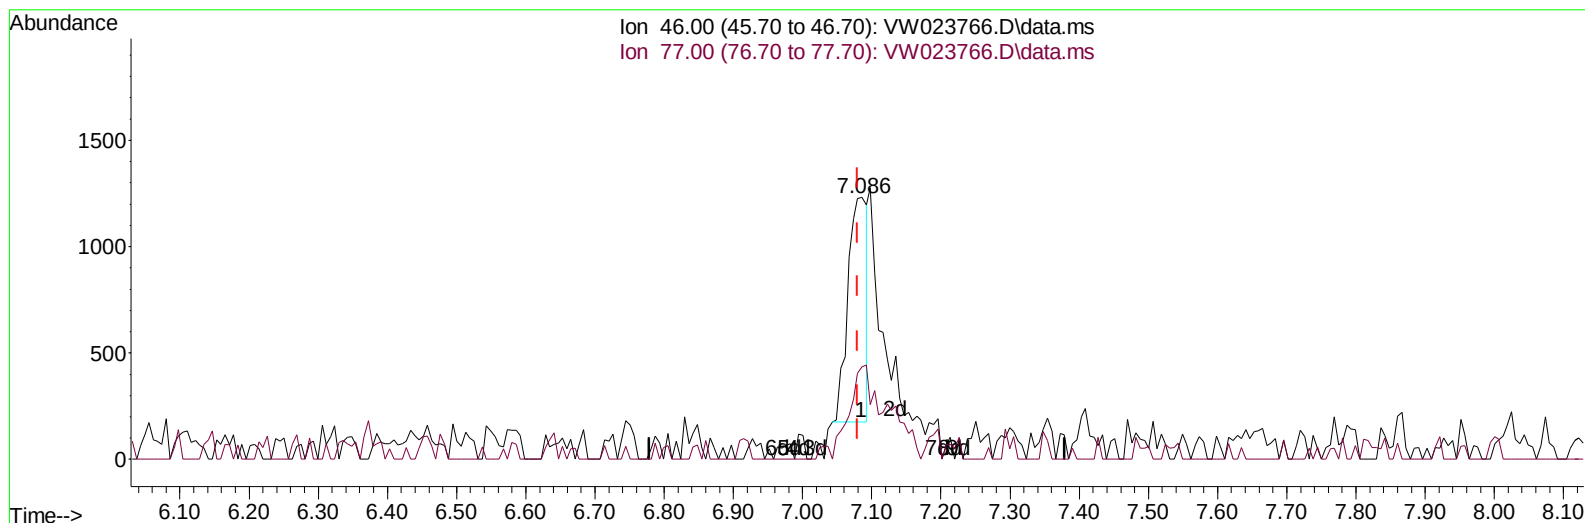

TIC: VW023766.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 40.27 ug/L

response 1988

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	54.73#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023766.D
 Acq On : 15 Jul 2022 23:54
 Operator : SY/VA
 Sample : N3700-06RE
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C13RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:32:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

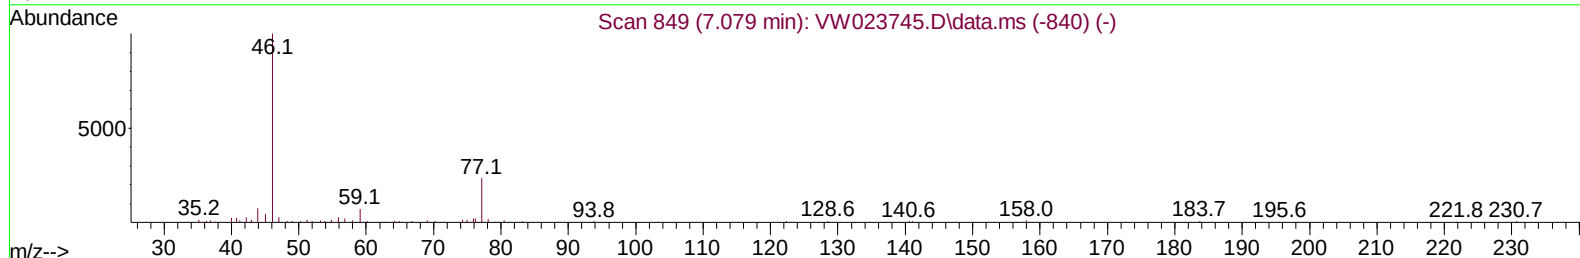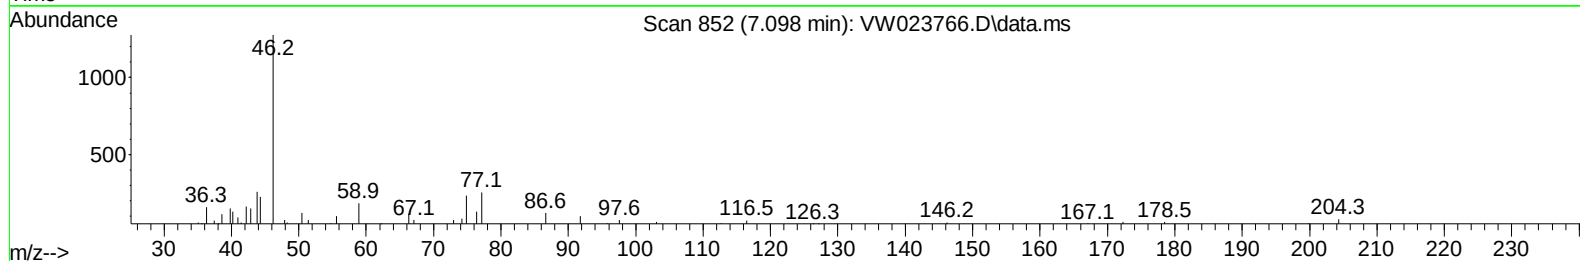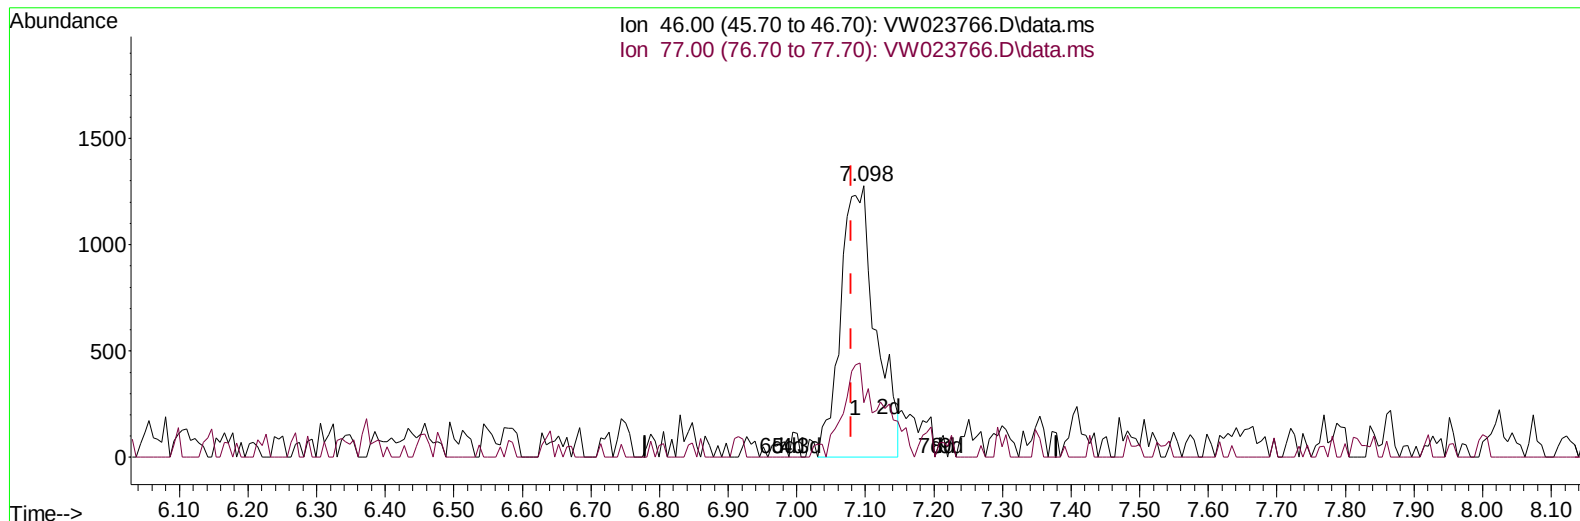

TIC: VW023766.D\data.ms

(21) 2-Butanone-d5 (S)

7.098min (+ 0.019) 91.35 ug/L m

response 4509

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	24.13
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023766.D
Acq On : 15 Jul 2022 23:54
Operator : SY/VA
Sample : N3700-06RE
Misc : 6.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C13RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:32:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

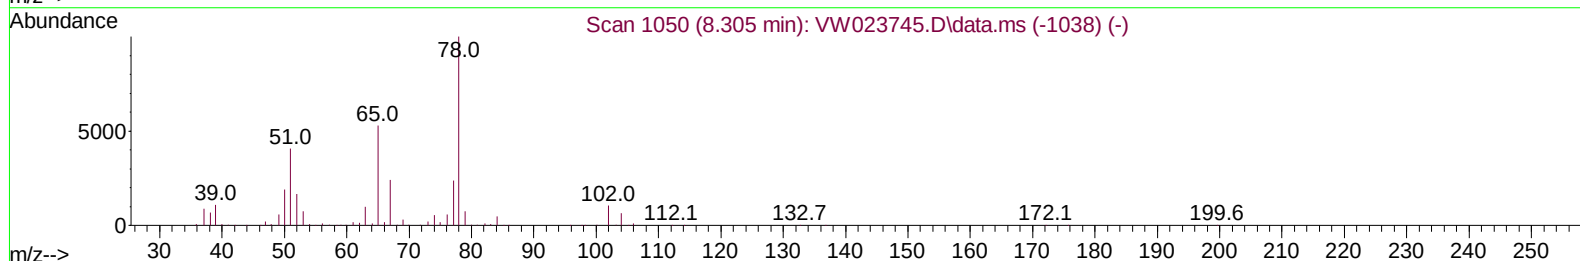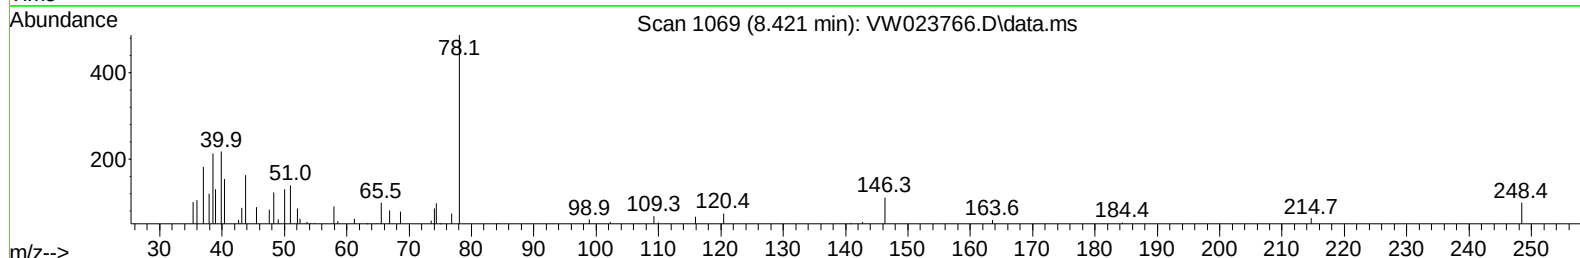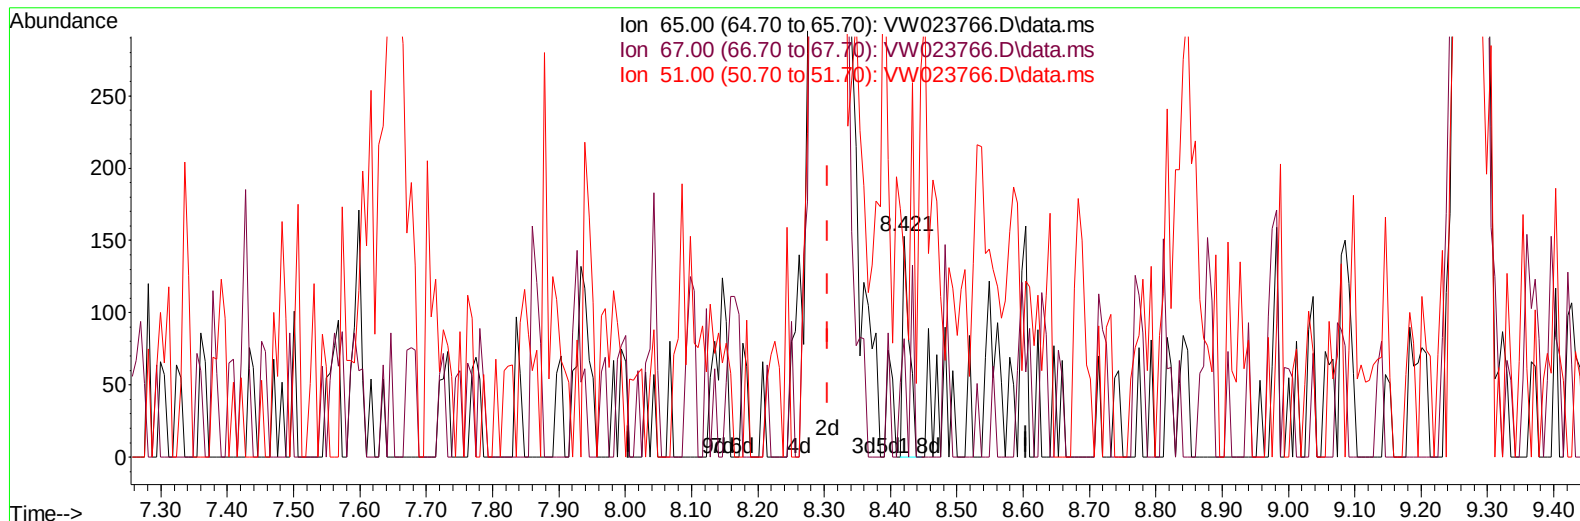

TIC: VW023766.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.421min (+ 0.116) 0.48 ug/L

response 107

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	45.79
51.00	92.20	92.52
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023766.D
Acq On : 15 Jul 2022 23:54
Operator : SY/VA
Sample : N3700-06RE
Misc : 6.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C13RE

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 16 00:32:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

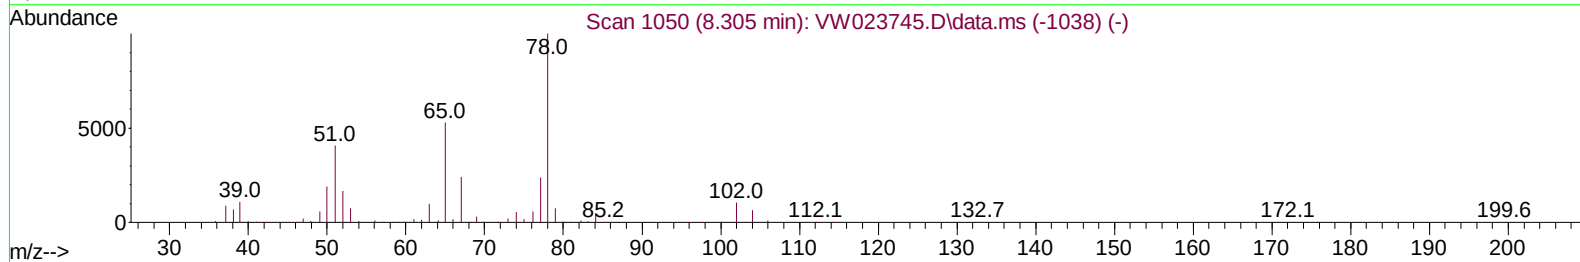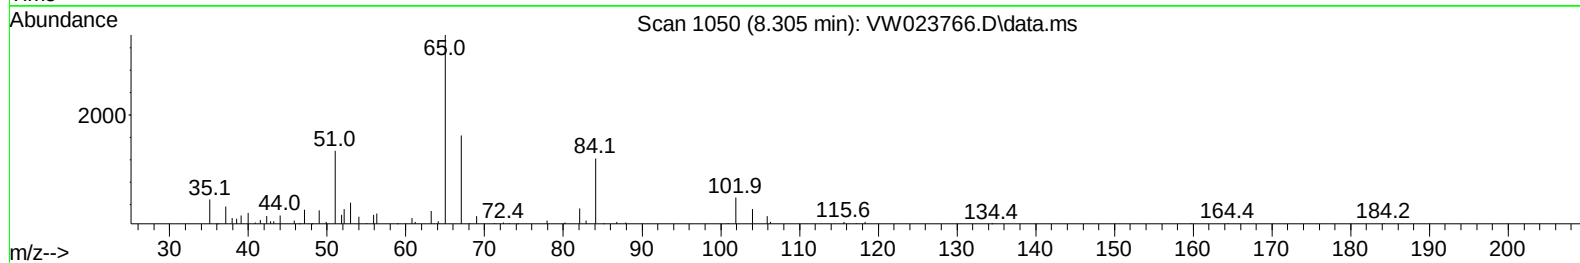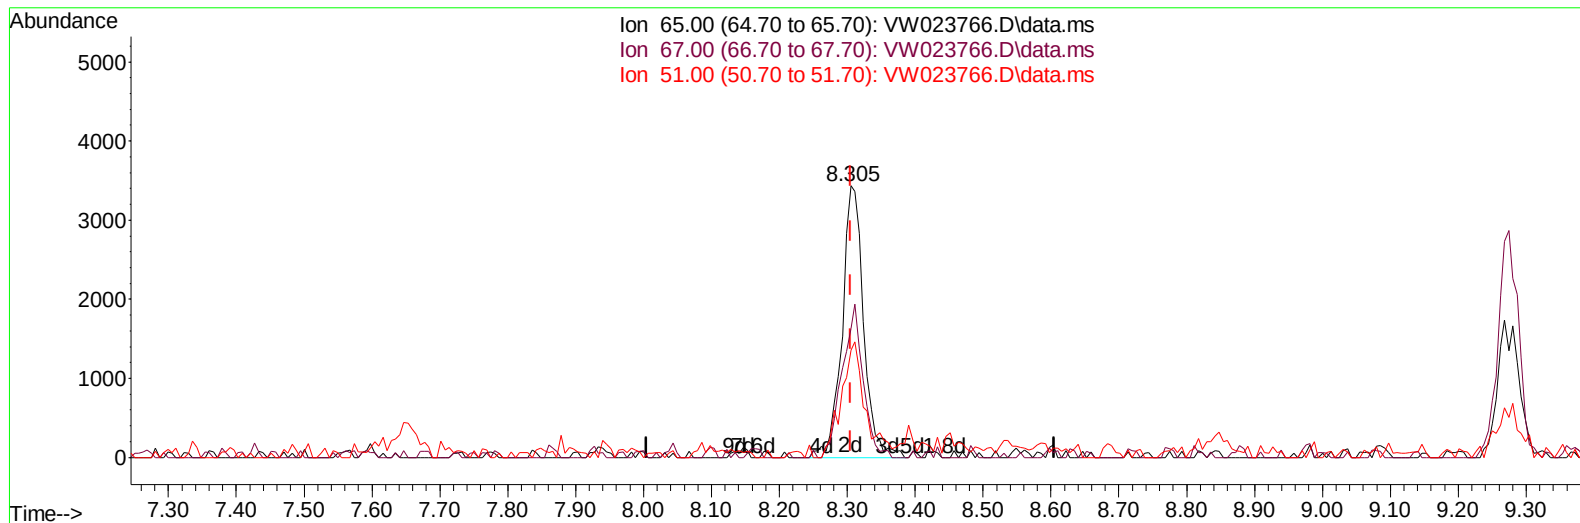

TIC: VW023766.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 34.11 ug/L m

response 7569

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.65#
51.00	92.20	1.31#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023766.D
 Acq On : 15 Jul 2022 23:54
 Operator : SY/VA
 Sample : N3700-06RE
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C13RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:32:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	12460	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	13054	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	4404	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	6432	20.211	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	80.840%	
7) Chloroethane-d5	2.873	69	6480	30.522	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	122.080%	
11) 1,1-Dichloroethene-d2	4.019	63	4409	17.014	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	68.040%	
21) 2-Butanone-d5	7.098	46	4509m	91.345	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	182.700%#	
24) Chloroform-d	7.647	84	10649	29.355	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	117.400%	
26) 1,2-Dichloroethane-d4	8.305	65	7569m	34.114	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	136.440%#	
32) Benzene-d6	8.275	84	16158	23.811	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	95.240%	
36) 1,2-Dichloropropane-d6	9.274	67	5980	29.256	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	117.040%	
41) Toluene-d8	10.317	98	11349	16.488	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	65.960%	
43) trans-1,3-Dichloroprop...	10.585	79	1932	20.165	ug/L	0.01
Spiked Amount 25.000	Range 30	- 135	Recovery	=	80.640%	
47) 2-Hexanone-d5	10.921	63	1970	45.833	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.660%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	7149	31.648	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	126.600%#	
66) 1,2-Dichlorobenzene-d4	13.847	152	3920	24.934	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	99.720%	
Target Compounds						
13) Acetone	4.141	43	2001m	57.336	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023766.D
Acq On : 15 Jul 2022 23:54
Operator : SY/VA
Sample : N3700-06RE
Misc : 6.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C13RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 00:32:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

