




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023768.D
 Acq On : 16 Jul 2022 00:43
 Operator : SY/VA
 Sample : N3700-12RE
 Misc : 6.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C19RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:02:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

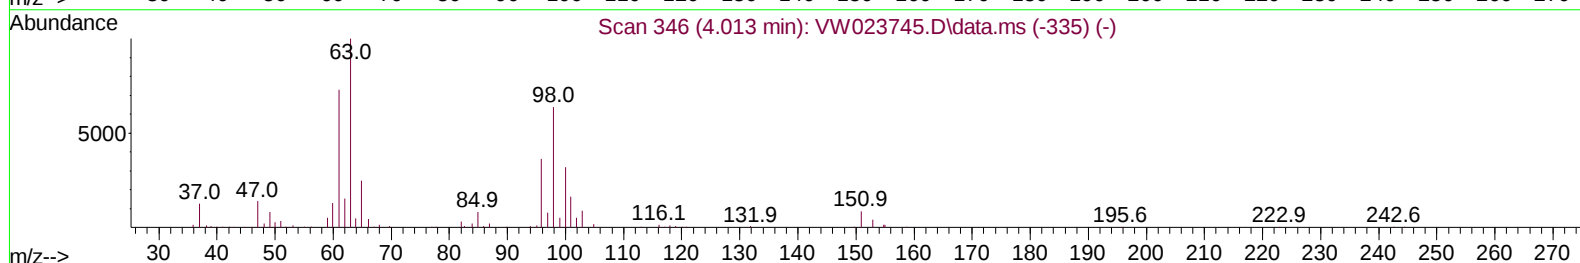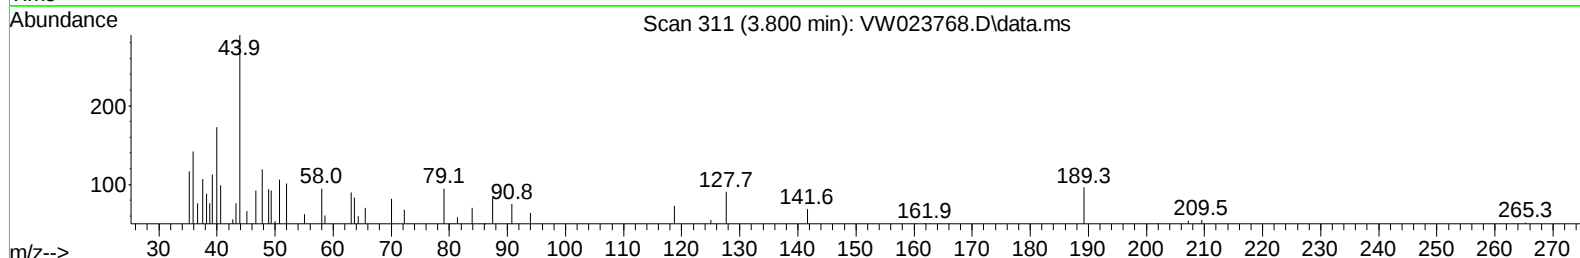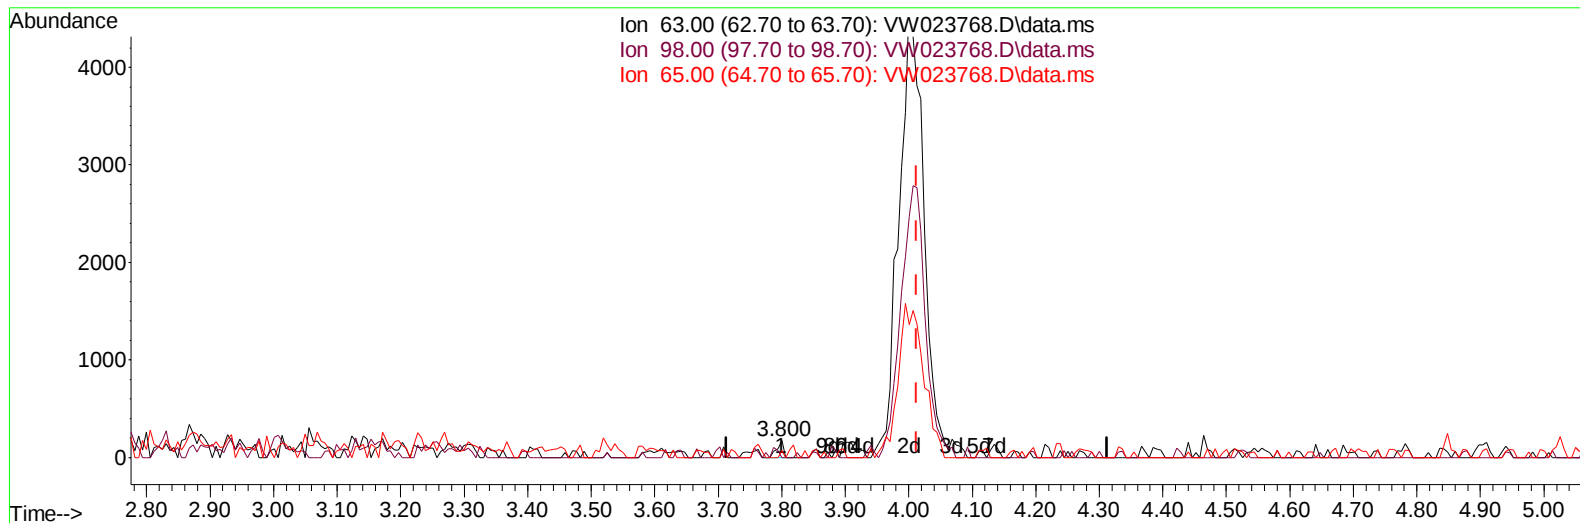

TIC: VW023768.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.800min (-0.213) 0.19 ug/L

response 118

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.20	52.54
65.00	24.10	22.03
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023768.D
 Acq On : 16 Jul 2022 00:43
 Operator : SY/VA
 Sample : N3700-12RE
 Misc : 6.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C19RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:02:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

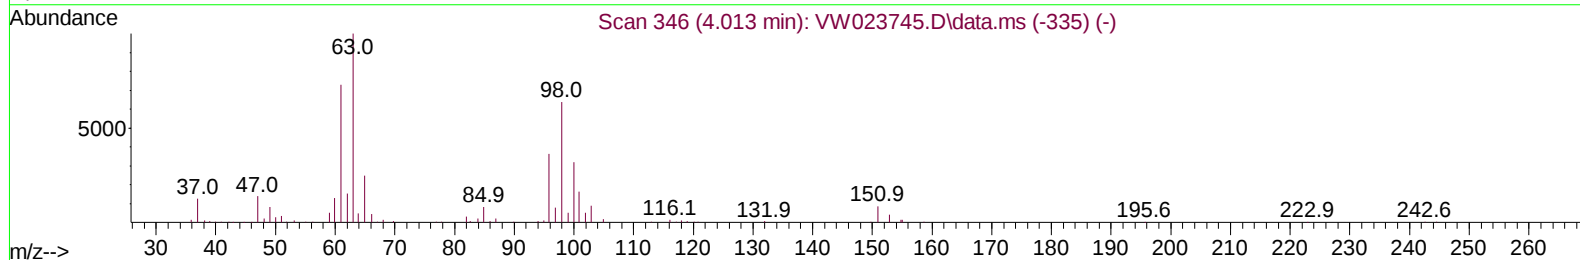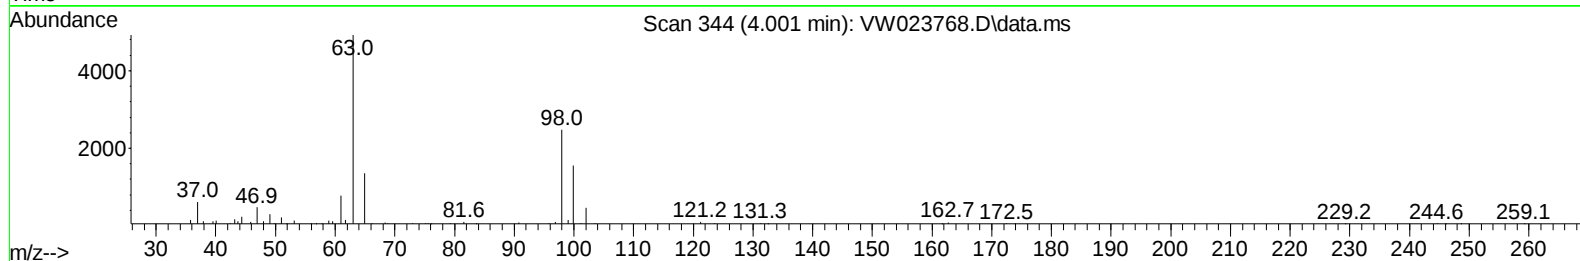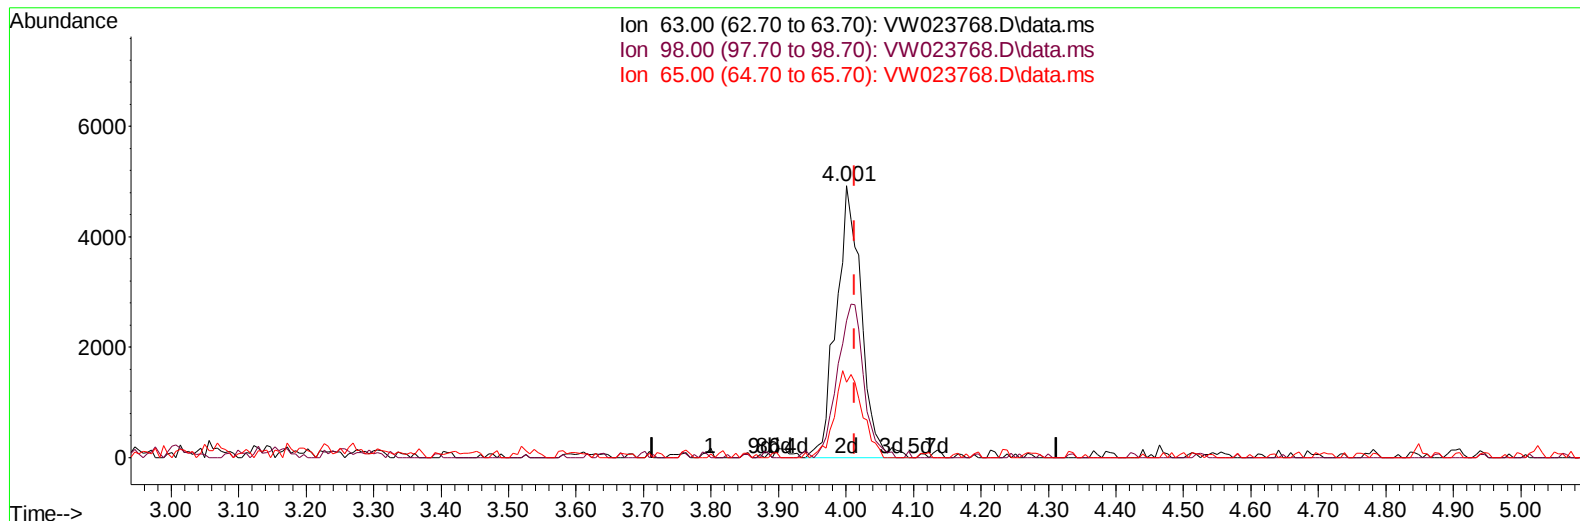

TIC: VW023768.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.001min (-0.012) 20.75 ug/L m

response 12662

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.20	0.49#
65.00	24.10	0.21#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023768.D
 Acq On : 16 Jul 2022 00:43
 Operator : SY/VA
 Sample : N3700-12RE
 Misc : 6.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C19RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:02:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

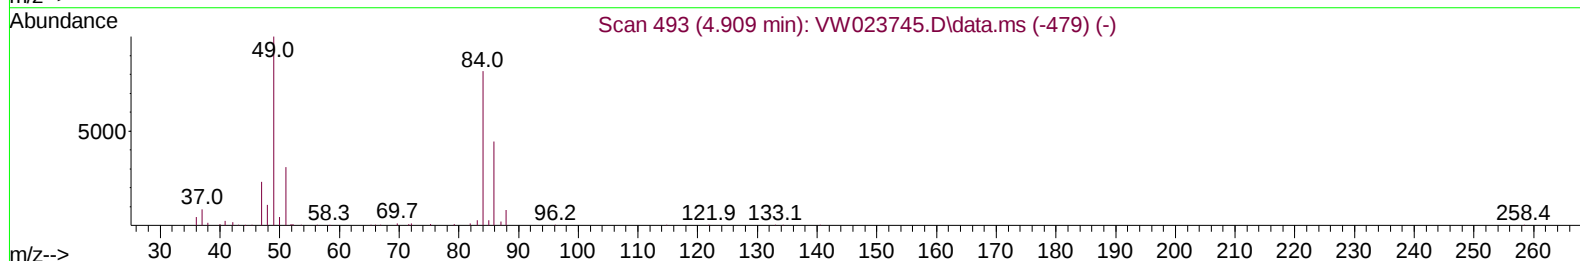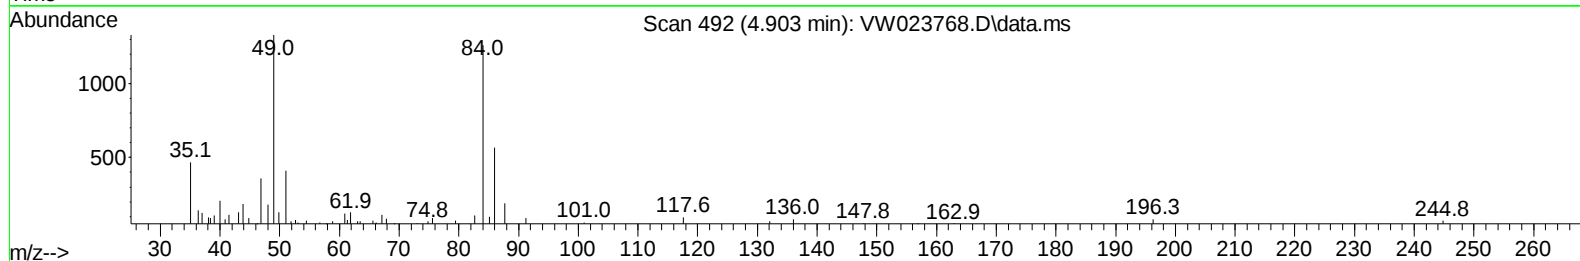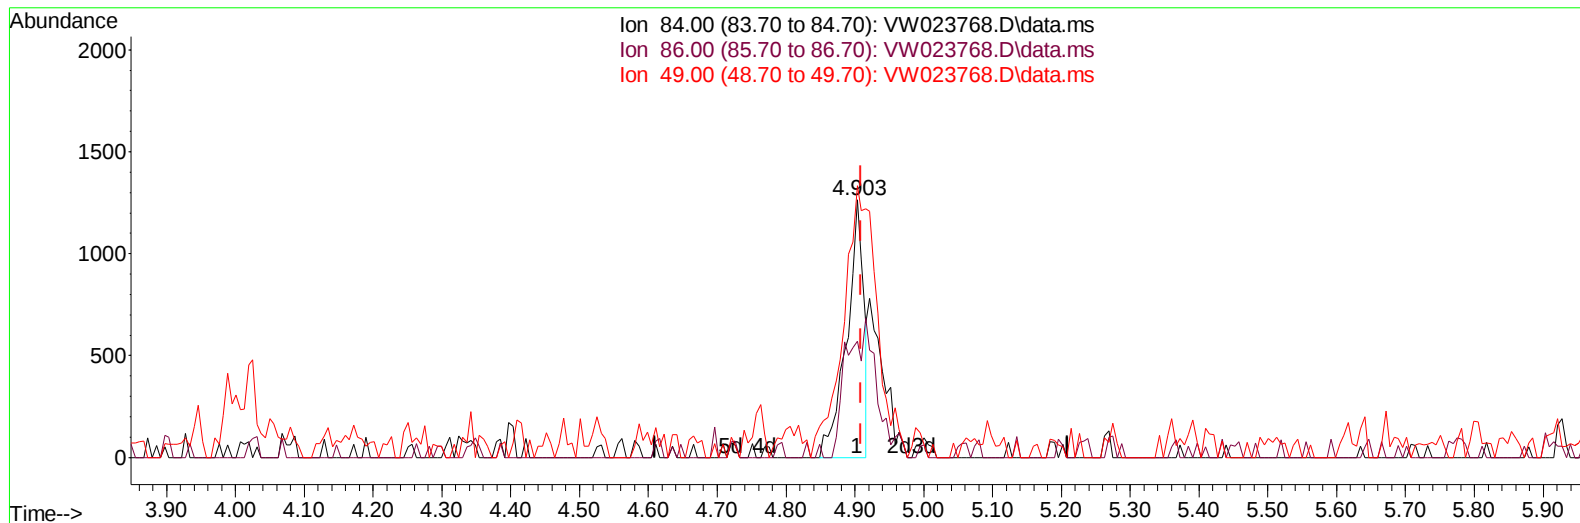

TIC: VW023768.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.006) 4.72 ug/L

response 2164

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	45.05
49.00	122.00	105.46
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023768.D
Acq On : 16 Jul 2022 00:43
Operator : SY/VA
Sample : N3700-12RE
Misc : 6.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C19RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:02:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

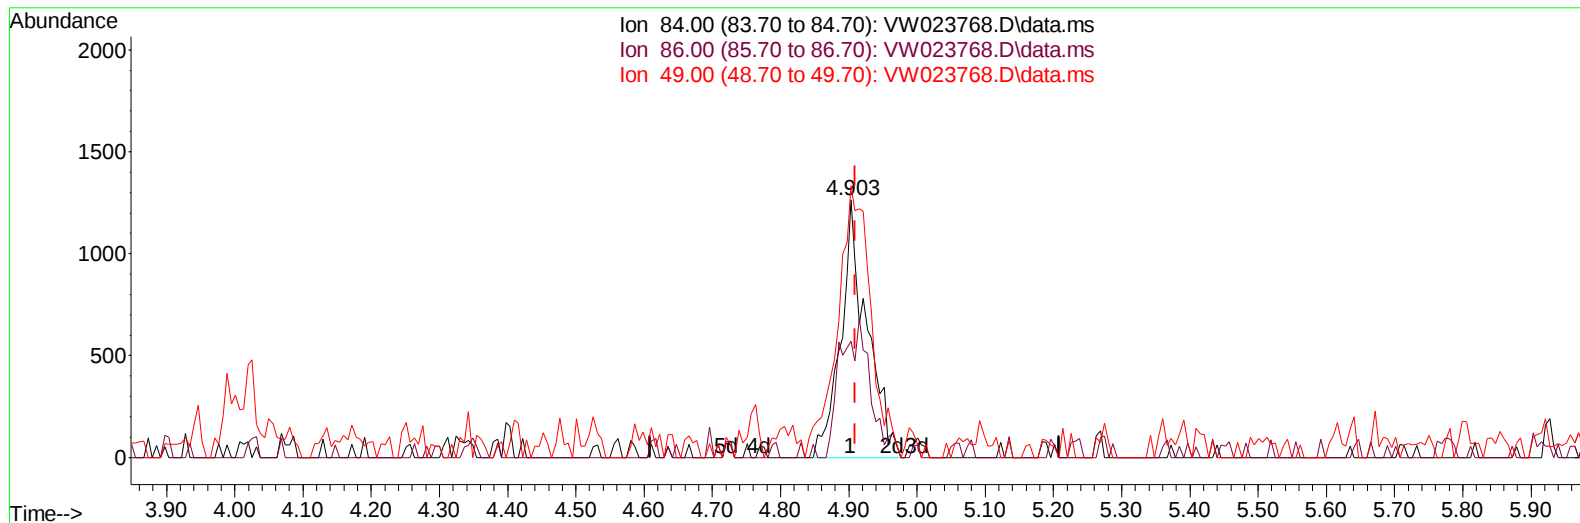




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023768.D
 Acq On : 16 Jul 2022 00:43
 Operator : SY/VA
 Sample : N3700-12RE
 Misc : 6.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C19RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:02:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

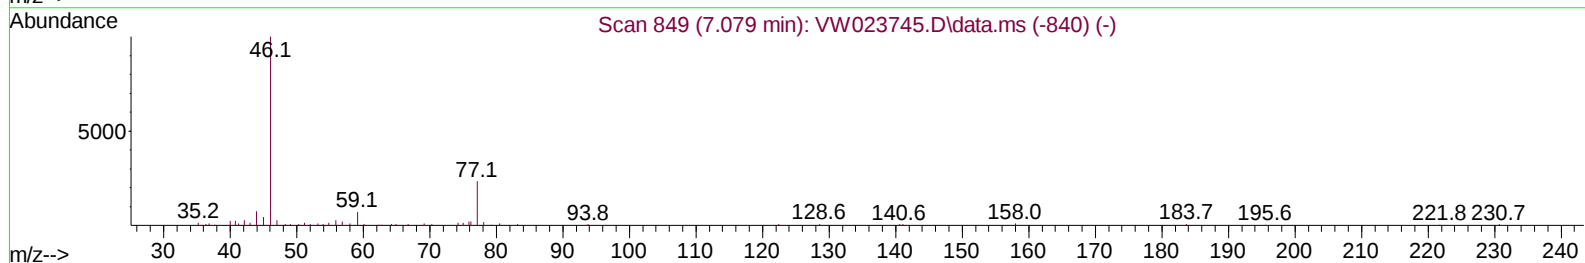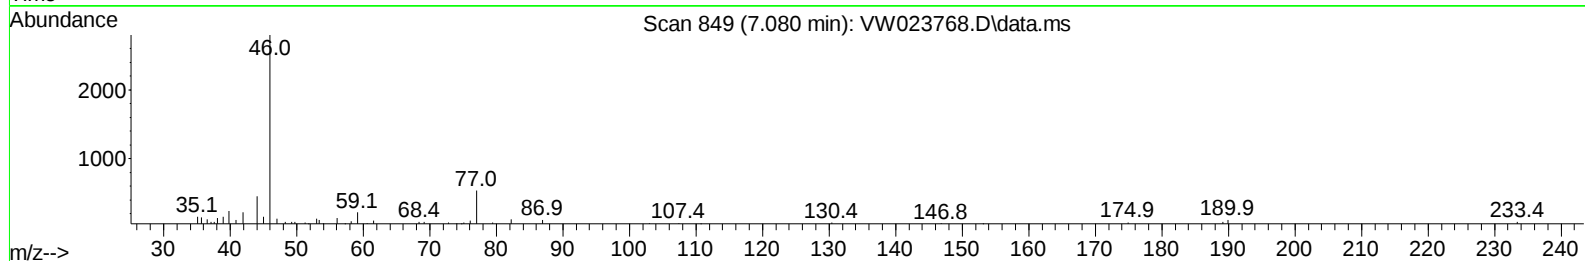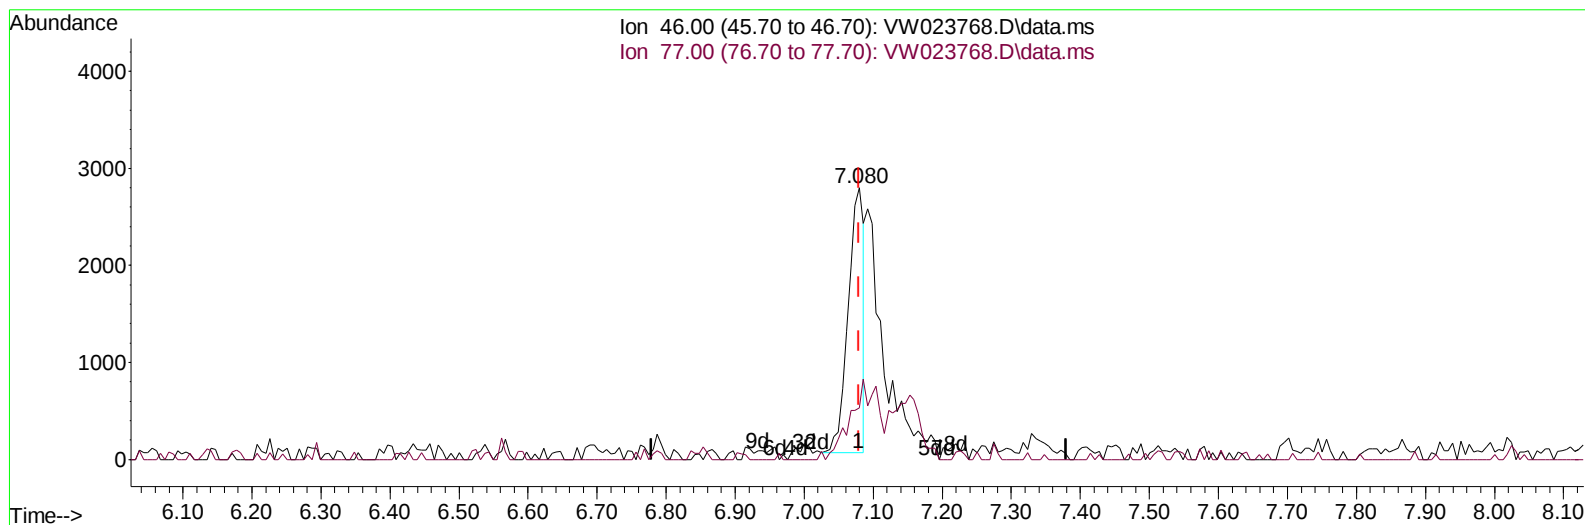

TIC: VW023768.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.000) 37.36 ug/L

response 4342

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	16.12#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023768.D
 Acq On : 16 Jul 2022 00:43
 Operator : SY/VA
 Sample : N3700-12RE
 Misc : 6.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C19RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:02:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

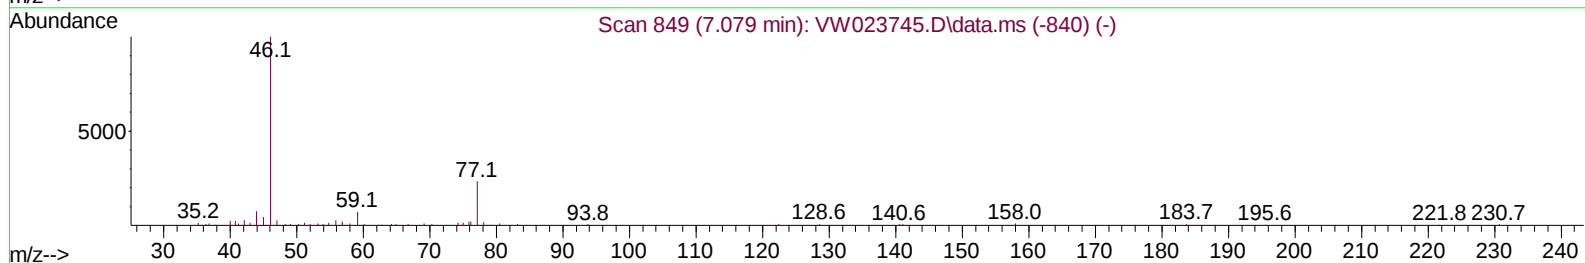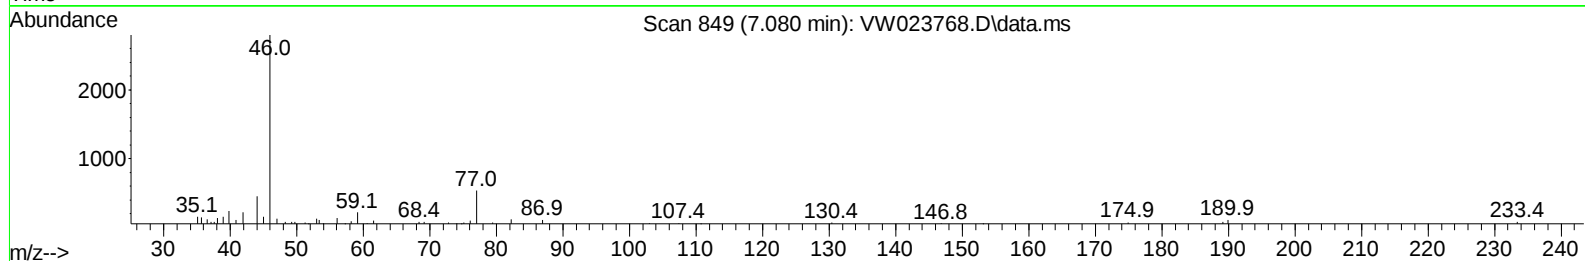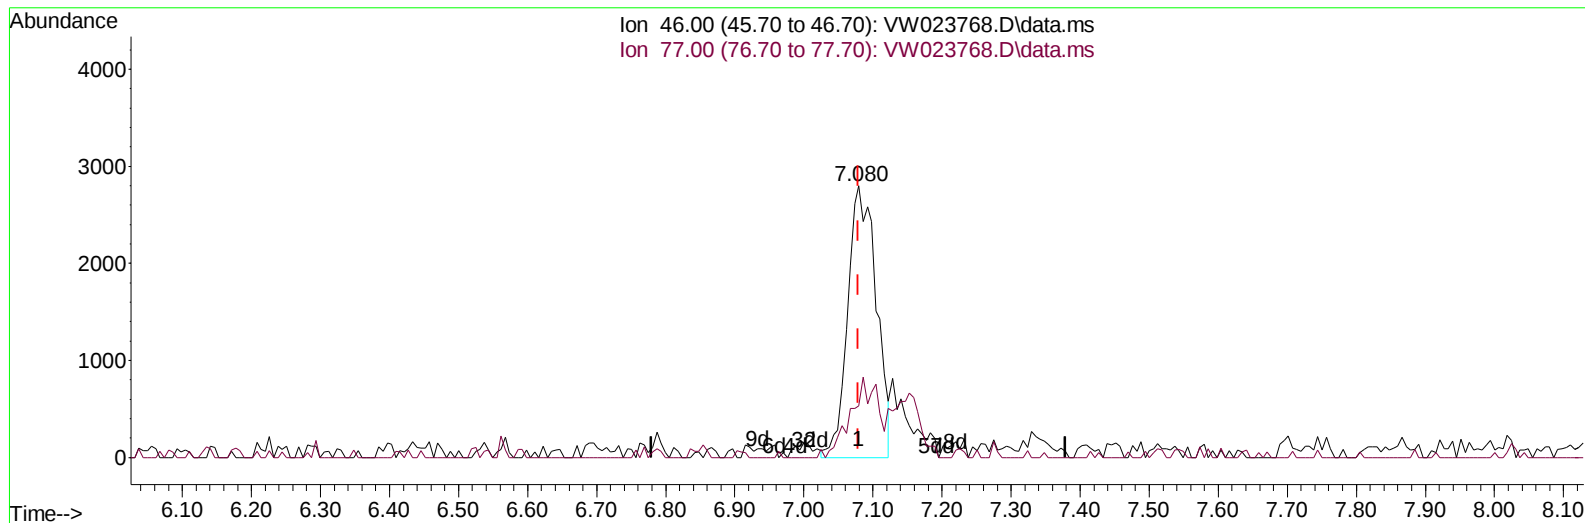

TIC: VW023768.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.000) 69.10 ug/L m

response 8032

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	8.72#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023768.D
 Acq On : 16 Jul 2022 00:43
 Operator : SY/VA
 Sample : N3700-12RE
 Misc : 6.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C19RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 01:02:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	29340	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	26474	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	8123	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	19832	26.465	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	105.840%	
7) Chloroethane-d5	2.873	69	17000	34.006	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	136.040%	
11) 1,1-Dichloroethene-d2	4.001	63	12662m	20.750	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	83.000%	
21) 2-Butanone-d5	7.080	46	8032m	69.102	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	138.200%#	
24) Chloroform-d	7.641	84	23351	27.336	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	109.360%	
26) 1,2-Dichloroethane-d4	8.305	65	14120	27.026	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	108.120%	
32) Benzene-d6	8.275	84	36973	26.866	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	107.480%	
36) 1,2-Dichloropropane-d6	9.274	67	12910	31.143	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	124.560%#	
41) Toluene-d8	10.323	98	28099	20.129	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	80.520%	
43) trans-1,3-Dichloroprop...	10.579	79	3456	17.786	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.160%	
47) 2-Hexanone-d5	10.920	63	4161	47.735	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	95.460%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	12495	27.275	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	109.080%	
66) 1,2-Dichlorobenzene-d4	13.847	152	6926	23.885	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	95.520%	
Target Compounds						Qvalue
13) Acetone	4.135	43	6473	78.767	ug/L	93
16) Methylene chloride	4.903	84	3380m	7.367	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023768.D
Acq On : 16 Jul 2022 00:43
Operator : SY/VA
Sample : N3700-12RE
Misc : 6.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C19RE

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 16 01:02:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

