




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023772.D
 Acq On : 16 Jul 2022 02:45
 Operator : SY/VA
 Sample : N3700-16RE
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B57RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

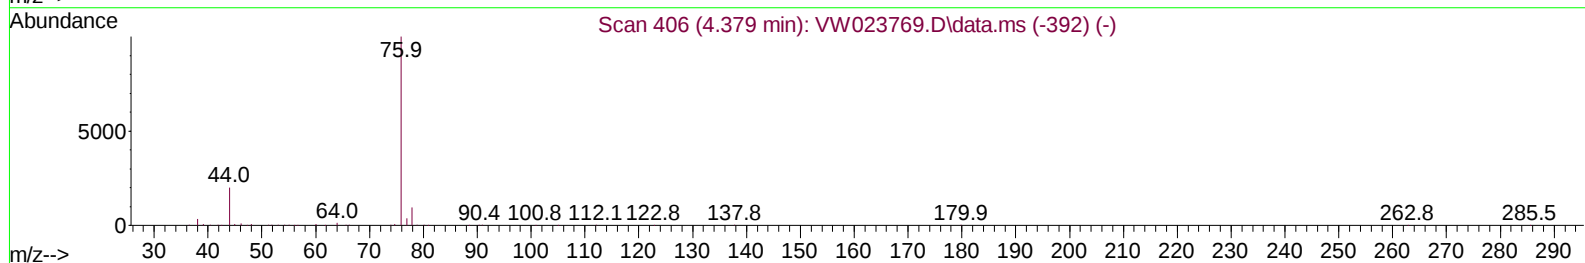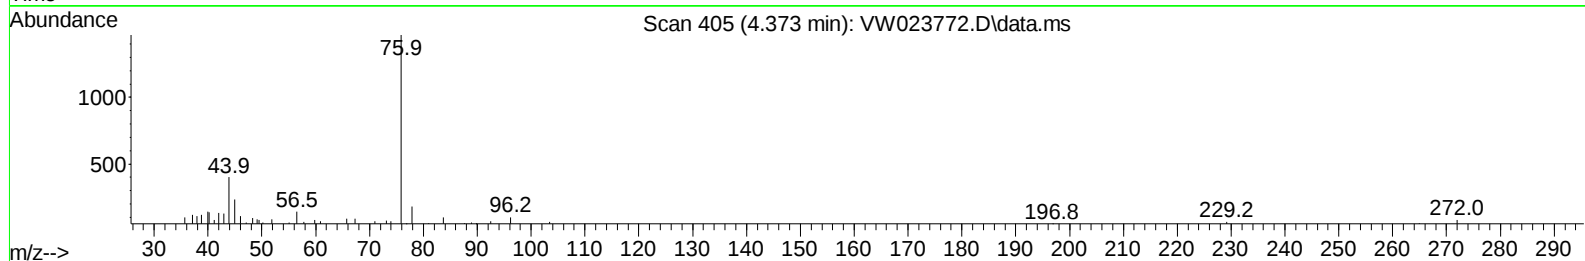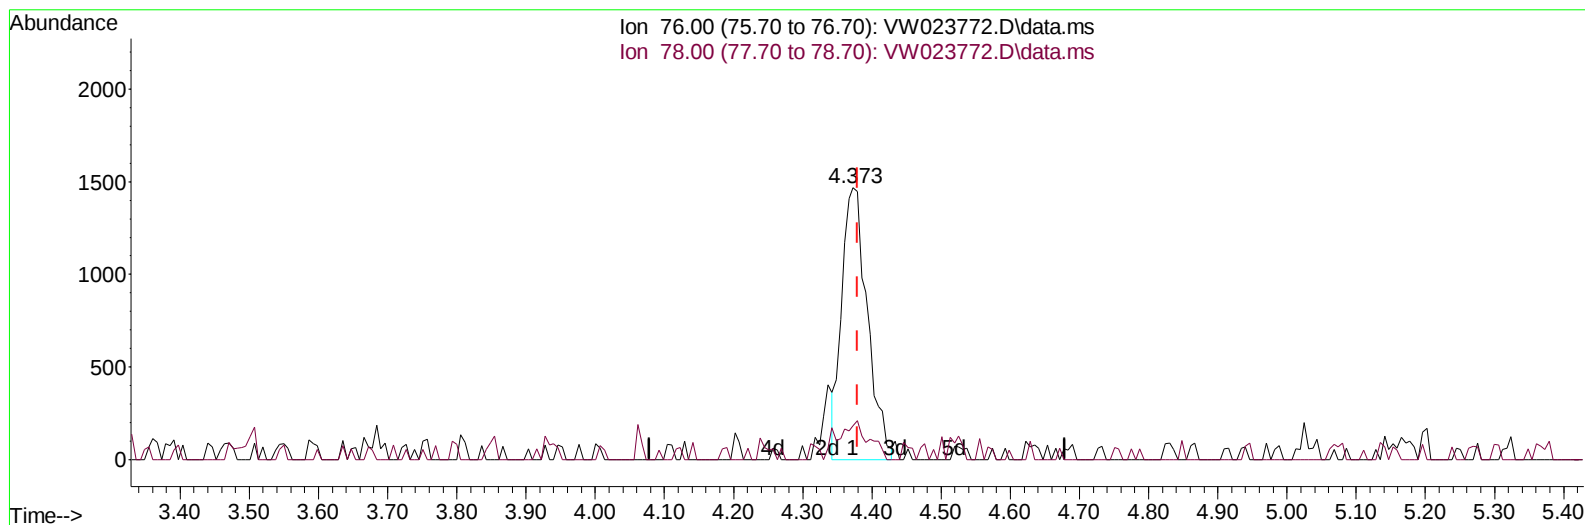

TIC: VW023772.D\data.ms

(14) Carbon disulfide (T)

4.373min (-0.006) 4.35 ug/L

response 3756

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.00	12.41#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023772.D
 Acq On : 16 Jul 2022 02:45
 Operator : SY/VA
 Sample : N3700-16RE
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B57RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

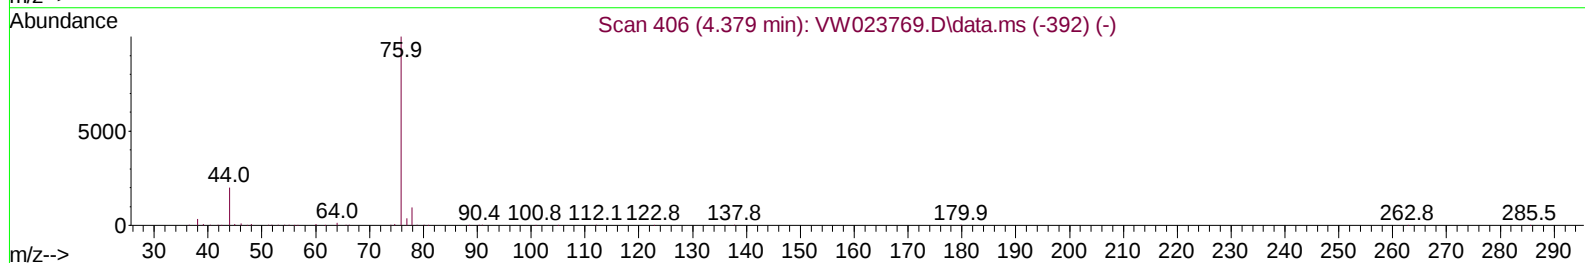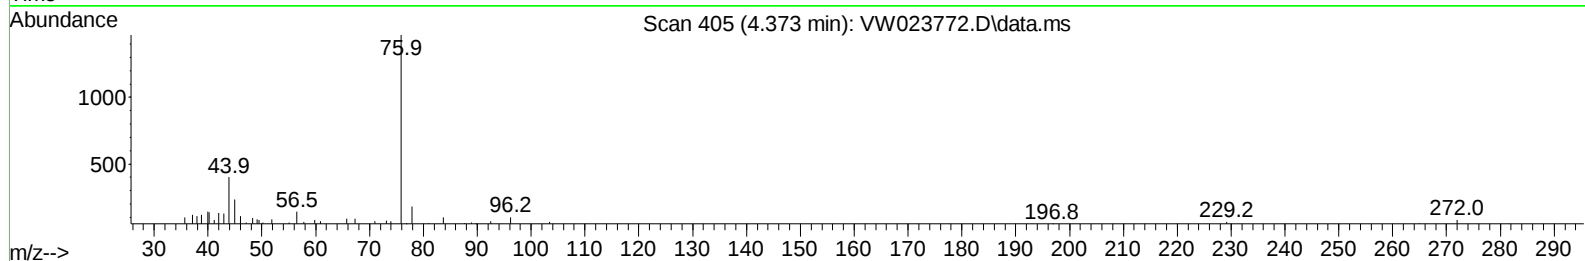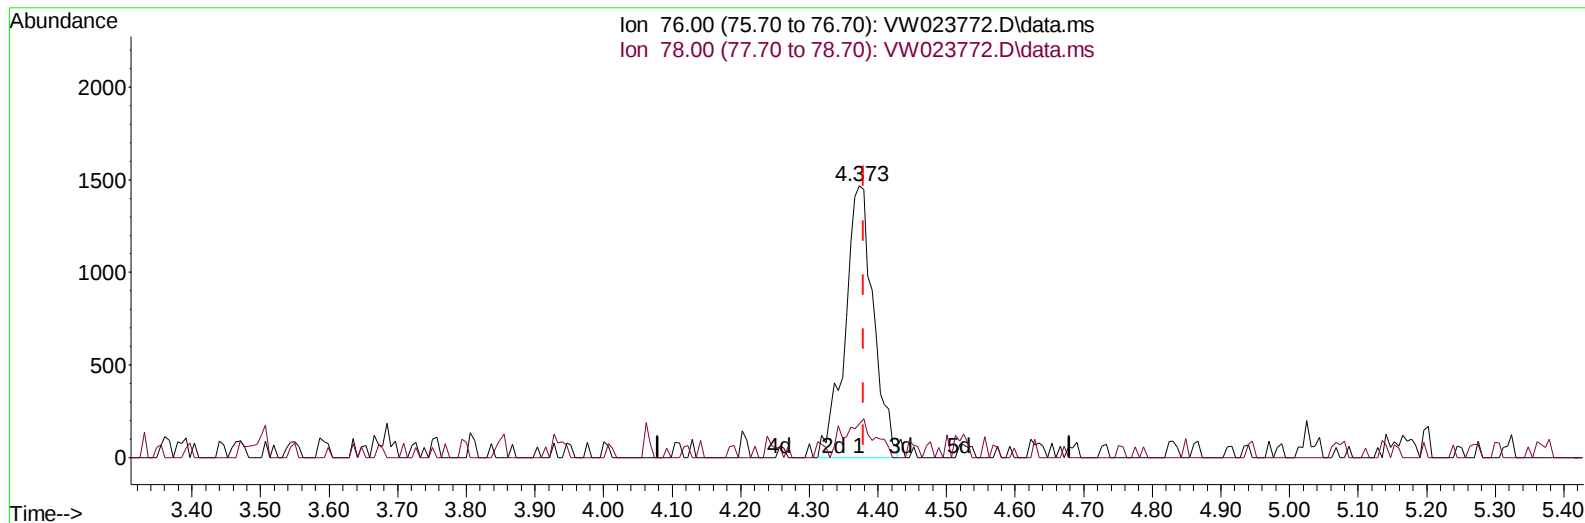

TIC: VW023772.D\data.ms

(14) Carbon disulfide (T)

4.373min (-0.006) 4.85 ug/L m

response 4192

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.00	12.41#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023772.D
 Acq On : 16 Jul 2022 02:45
 Operator : SY/VA
 Sample : N3700-16RE
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B57RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

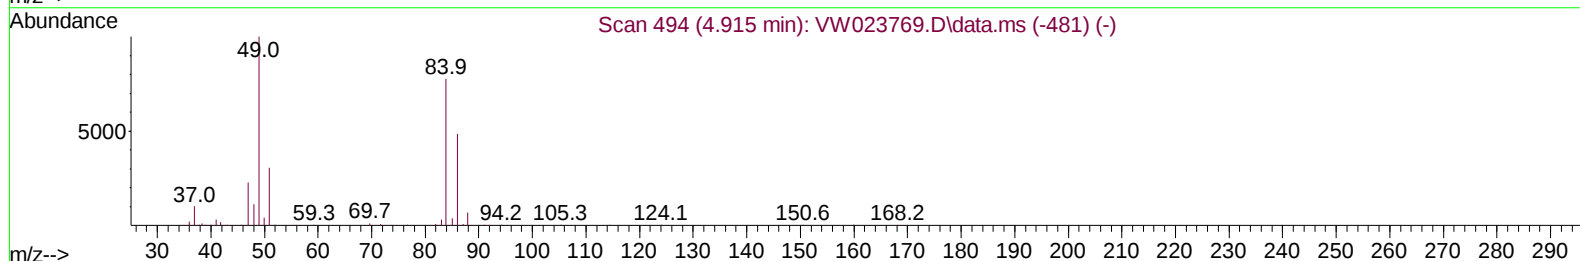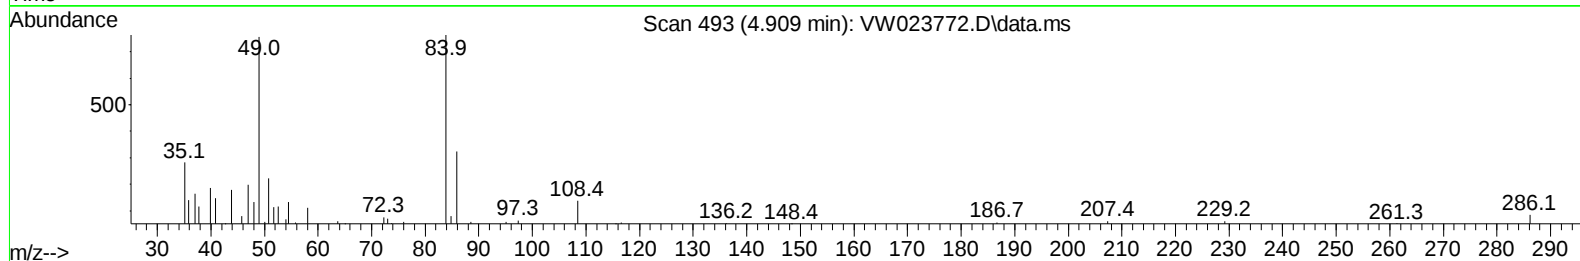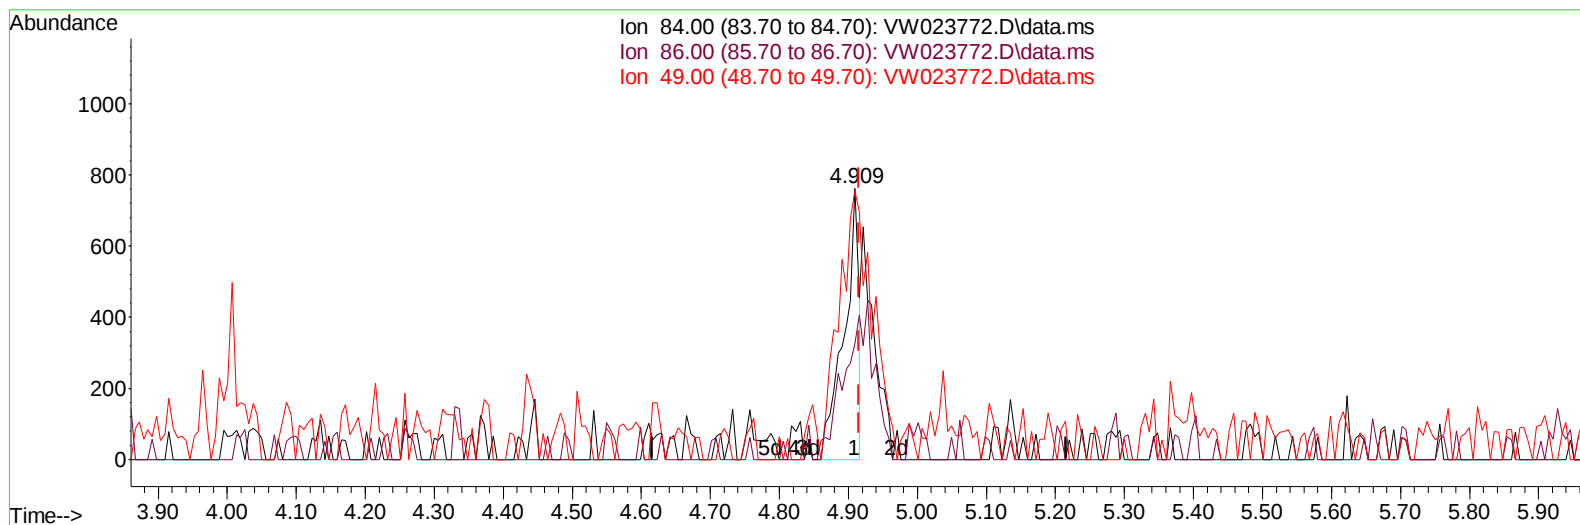

TIC: VW023772.D\data.ms

(16) Methylene chloride (T)

4.909min (-0.006) 2.60 ug/L

response 1126

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	42.60#
49.00	122.00	98.95
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023772.D
 Acq On : 16 Jul 2022 02:45
 Operator : SY/VA
 Sample : N3700-16RE
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B57RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

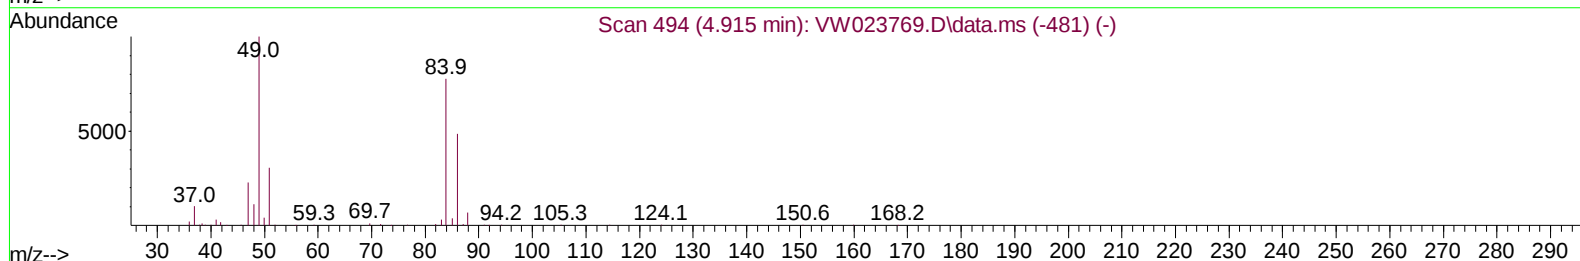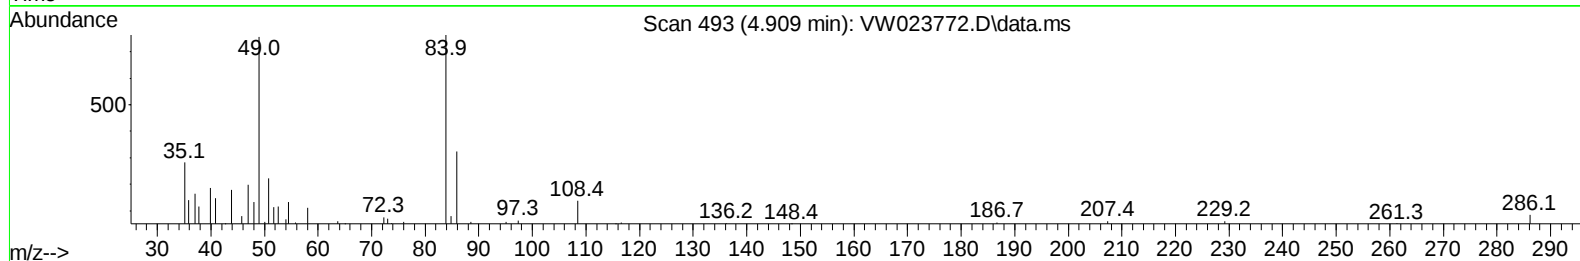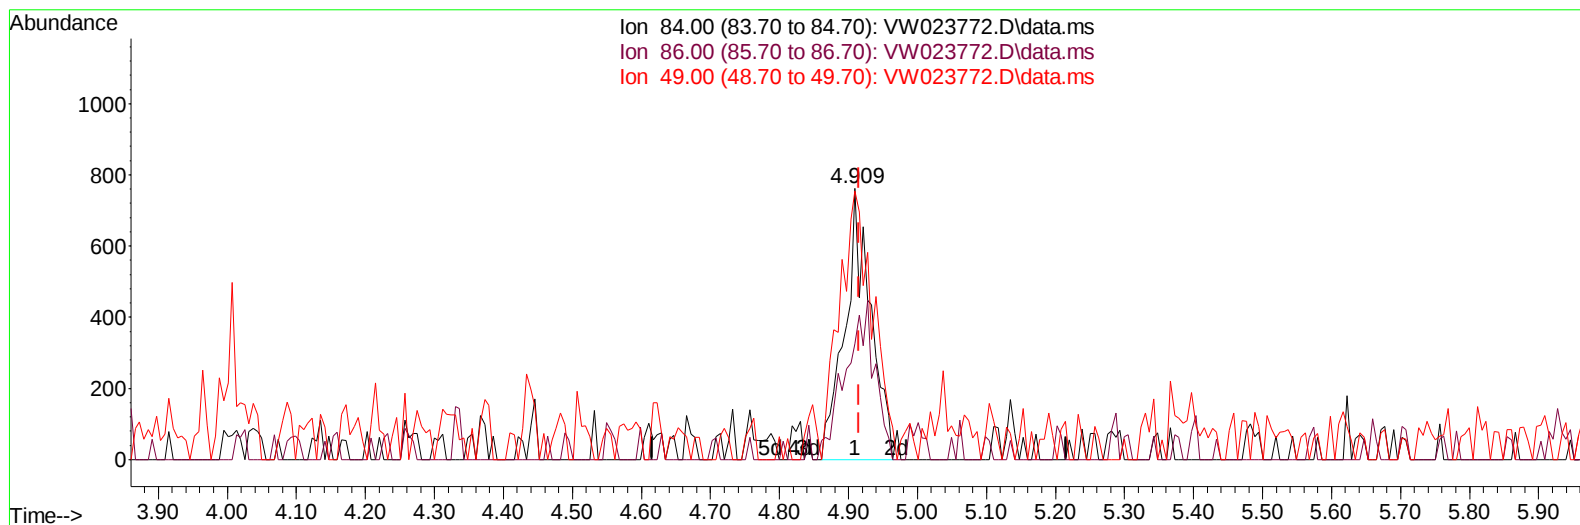

TIC: VW023772.D\data.ms

(16) Methylene chloride (T)

4.909min (-0.006) 4.58 ug/L m

response 1985

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	42.60#
49.00	122.00	98.95
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023772.D
 Acq On : 16 Jul 2022 02:45
 Operator : SY/VA
 Sample : N3700-16RE
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B57RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

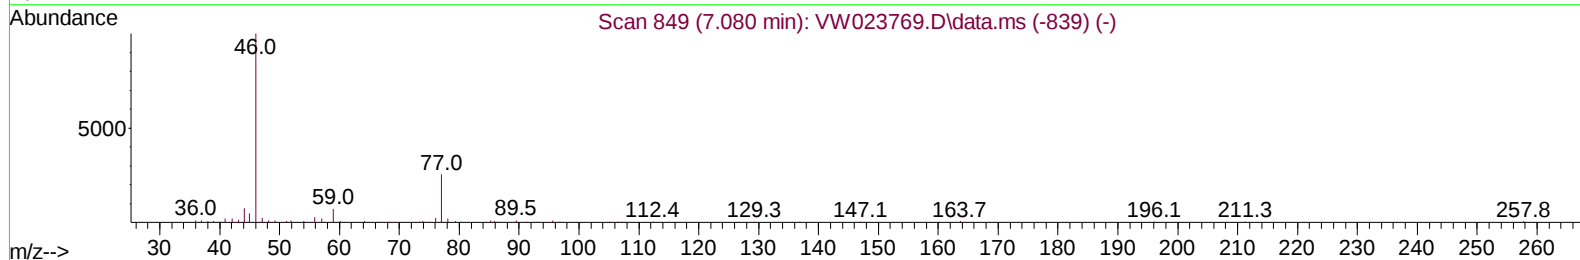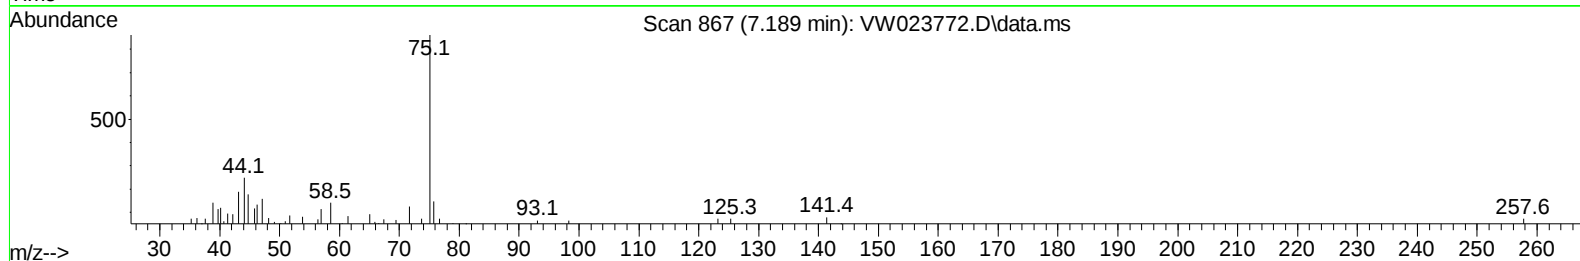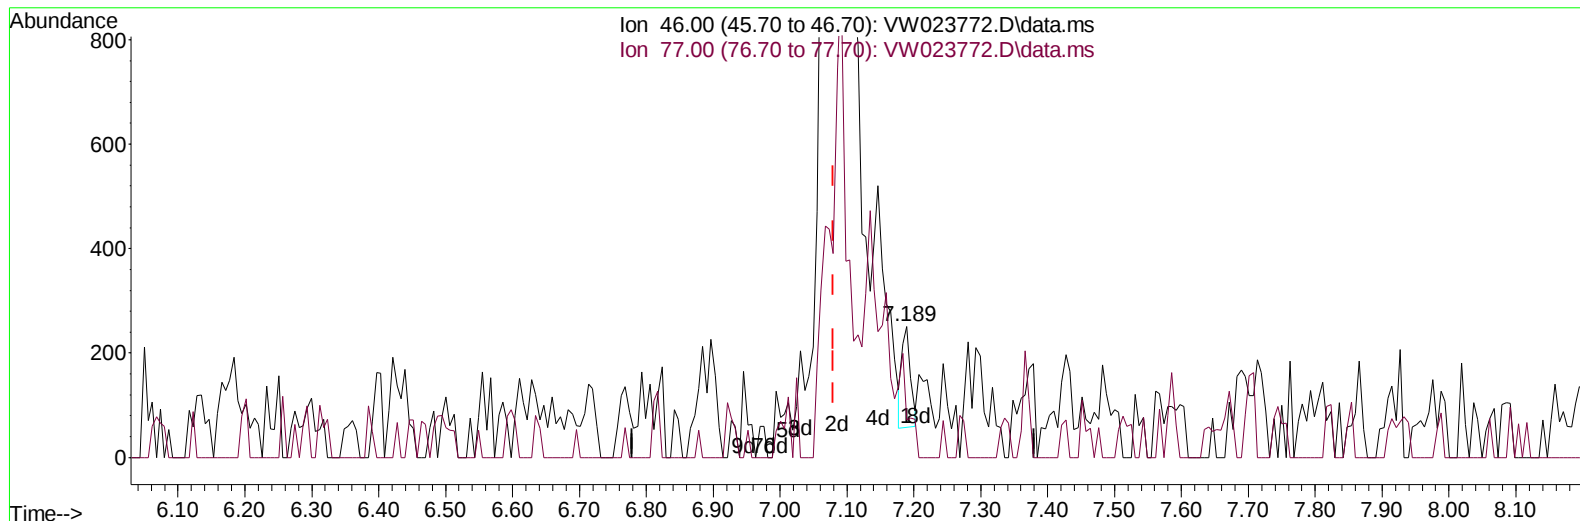

TIC: VW023772.D\data.ms

(21) 2-Butanone-d5 (S)

7.189min (+ 0.110) 1.58 ug/L

response 174

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	31.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023772.D
 Acq On : 16 Jul 2022 02:45
 Operator : SY/VA
 Sample : N3700-16RE
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B57RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

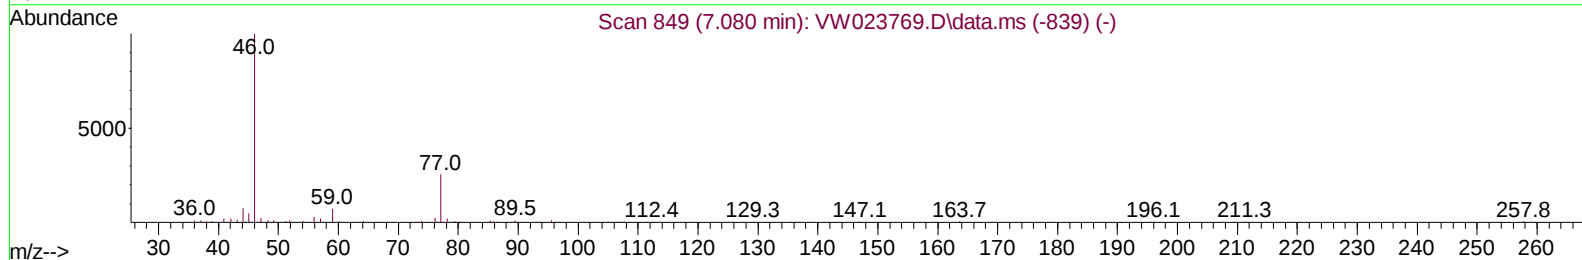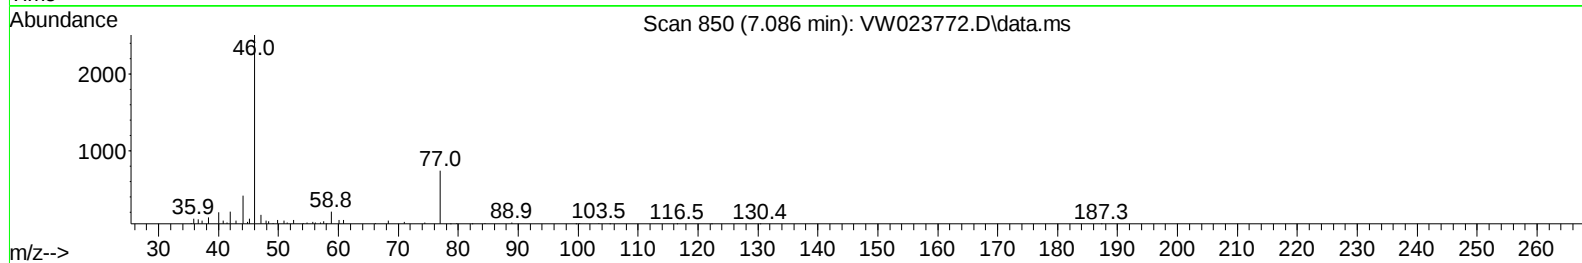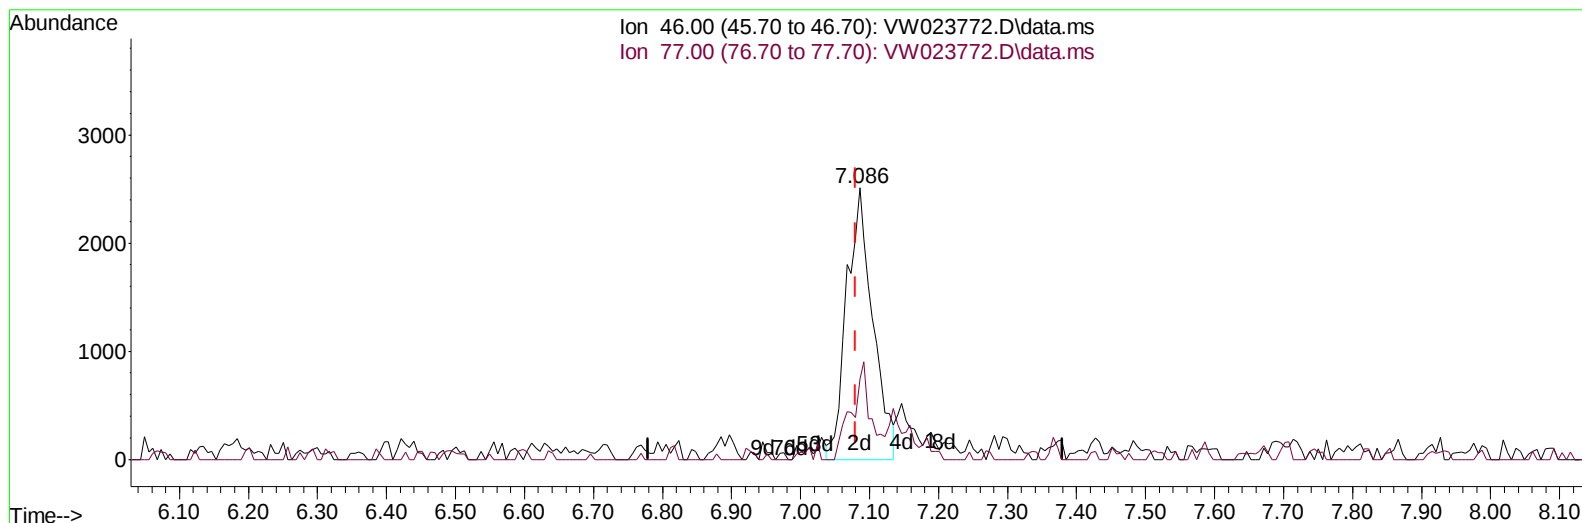

TIC: VW023772.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 60.00 ug/L m

response 6587

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	0.82#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023772.D
 Acq On : 16 Jul 2022 02:45
 Operator : SY/VA
 Sample : N3700-16RE
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B57RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	27711	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	29058	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	10927	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	12826	18.122	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	72.480%	
7) Chloroethane-d5	2.879	69	14751	31.241	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	124.960%	
11) 1,1-Dichloroethene-d2	4.007	63	9182	15.932	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	63.720%	
21) 2-Butanone-d5	7.086	46	6587m	60.001	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.000%	
24) Chloroform-d	7.647	84	20388	25.270	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	101.080%	
26) 1,2-Dichloroethane-d4	8.305	65	12342	25.012	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	100.040%	
32) Benzene-d6	8.281	84	30573	20.240	ug/L	0.01
Spiked Amount 25.000	Range 20	- 135	Recovery	=	80.960%	
36) 1,2-Dichloropropane-d6	9.274	67	11822	25.982	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	103.920%	
41) Toluene-d8	10.323	98	24617	16.067	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	64.280%	
43) trans-1,3-Dichloroprop...	10.579	79	3496	16.392	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	65.560%	
47) 2-Hexanone-d5	10.927	63	3648	38.128	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	76.260%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	11972	23.809	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	95.240%	
66) 1,2-Dichlorobenzene-d4	13.847	152	8898	22.811	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	91.240%	
Target Compounds						
13) Acetone	4.129	43	3918	50.479	ug/L	Qvalue 64
14) Carbon disulfide	4.373	76	4192m	4.851	ug/L	
16) Methylene chloride	4.909	84	1985m	4.581	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023772.D
Acq On : 16 Jul 2022 02:45
Operator : SY/VA
Sample : N3700-16RE
Misc : 5.61g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B57RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 16 01:30:01 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

