




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023773.D
Acq On : 16 Jul 2022 03:09
Operator : SY/VA
Sample : N3700-18RE
Misc : 6.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B59RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 16 01:30:01 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

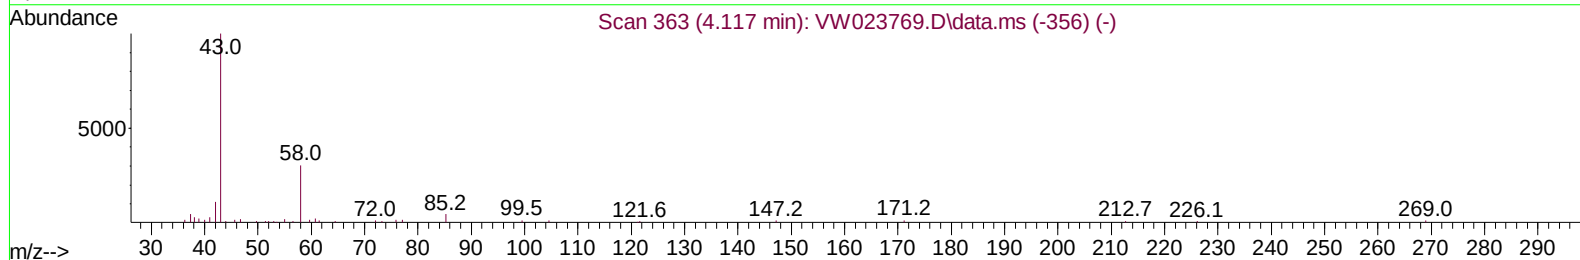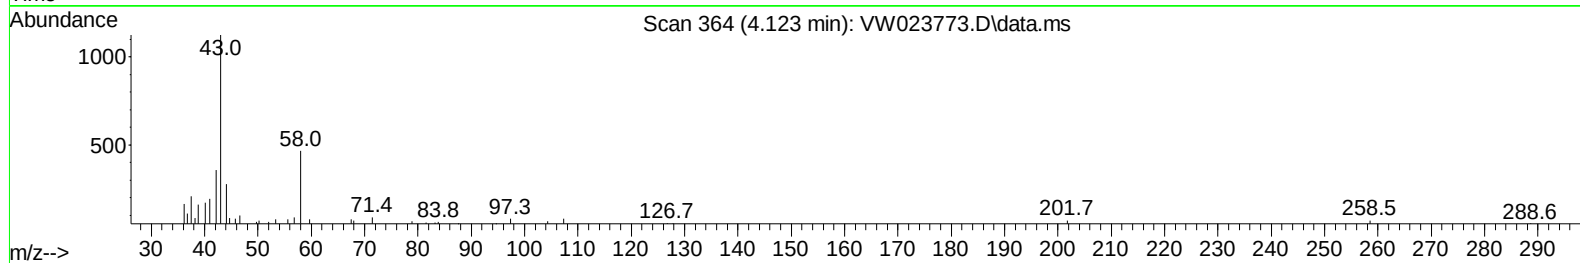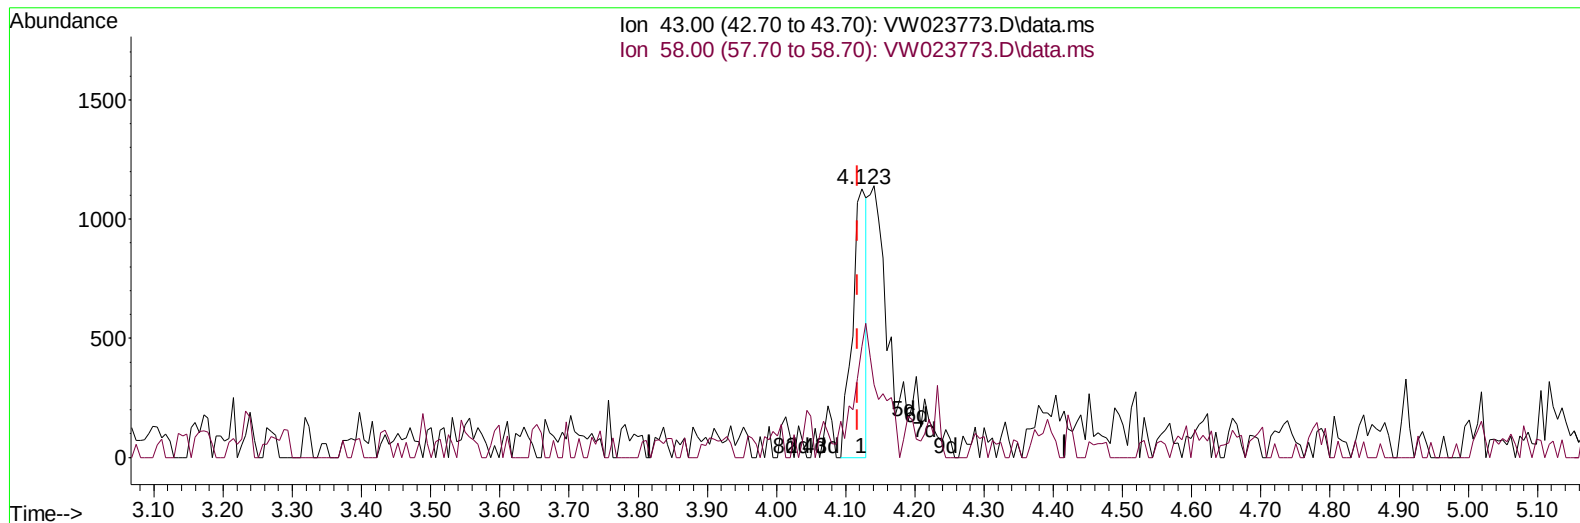

TIC: VW023773.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 24.43 ug/L

response 1621

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	54.78
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023773.D
 Acq On : 16 Jul 2022 03:09
 Operator : SY/VA
 Sample : N3700-18RE
 Misc : 6.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B59RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

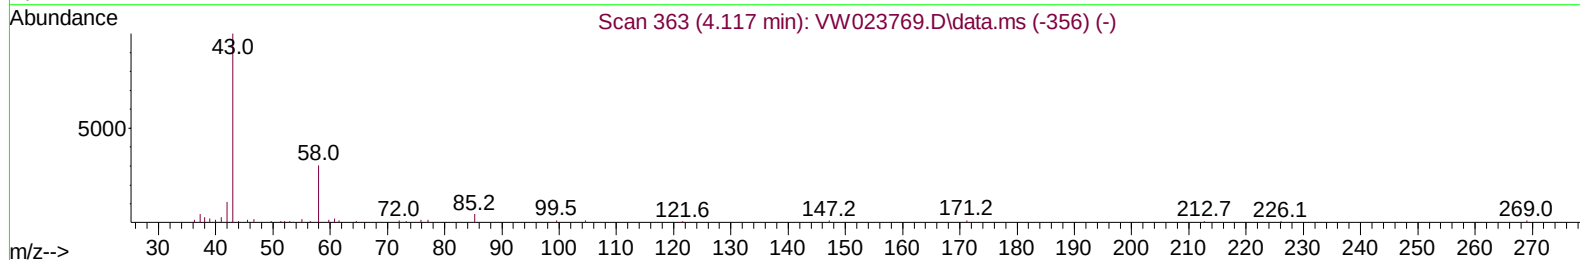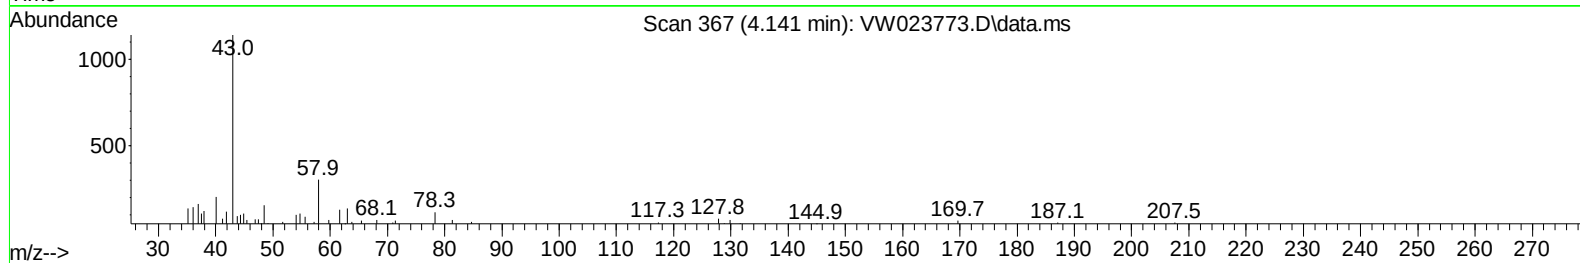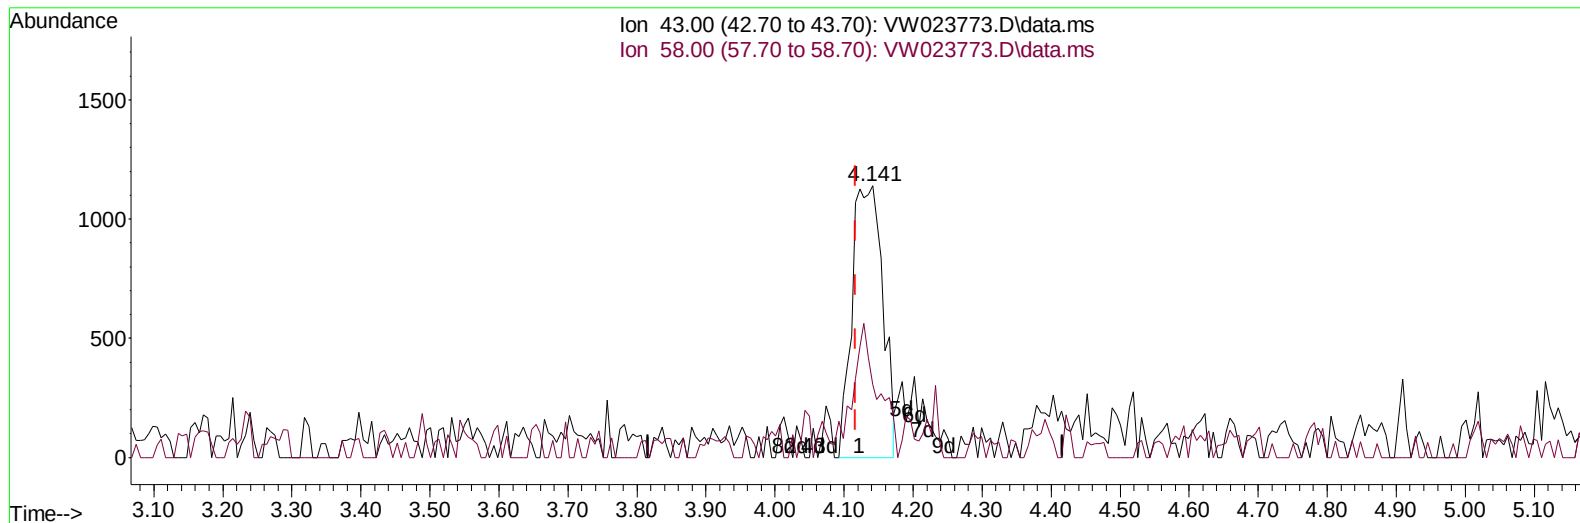

TIC: VW023773.D\data.ms

(13) Acetone (T)

4.141min (+ 0.024) 53.13 ug/L m

response 3526

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	25.18
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023773.D
 Acq On : 16 Jul 2022 03:09
 Operator : SY/VA
 Sample : N3700-18RE
 Misc : 6.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B59RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

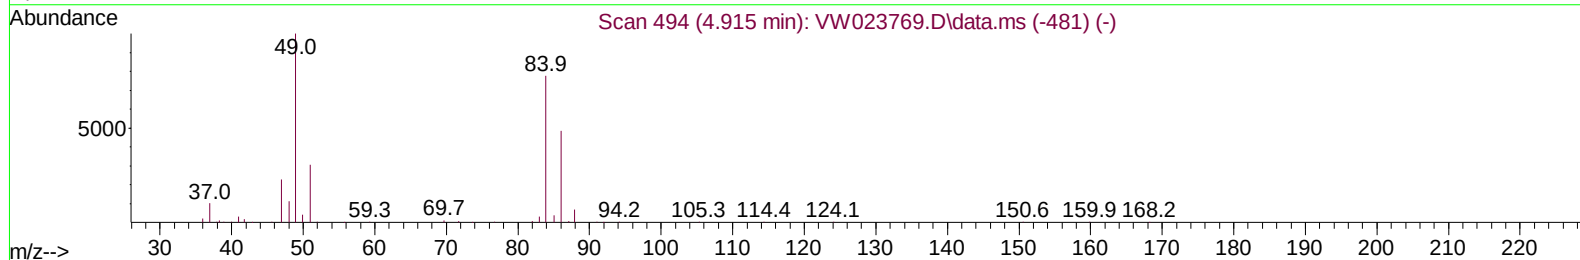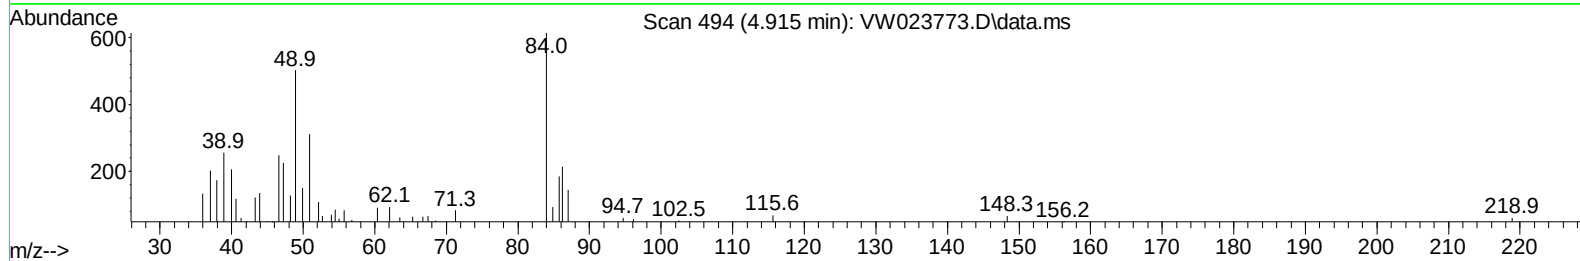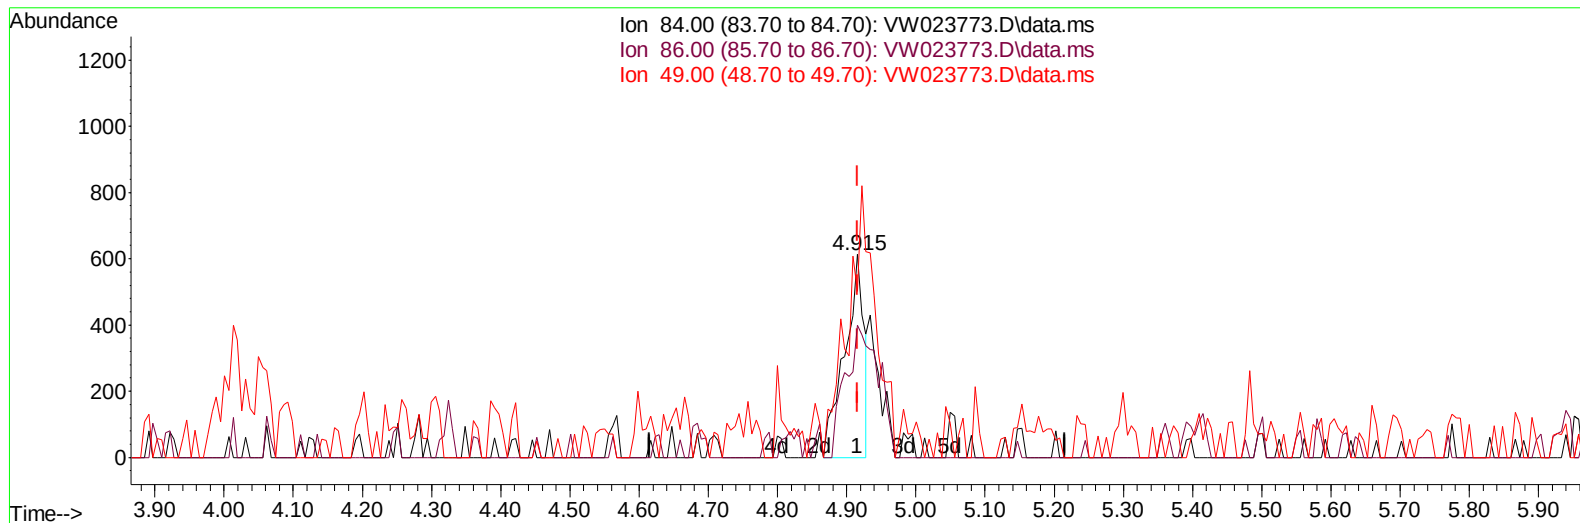

TIC: VW023773.D\data.ms

(16) Methylene chloride (T)

4.915min (-0.000) 3.21 ug/L

response 1188

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	65.25
49.00	122.00	81.89#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023773.D
Acq On : 16 Jul 2022 03:09
Operator : SY/VA
Sample : N3700-18RE
Misc : 6.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B59RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 16 01:30:01 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

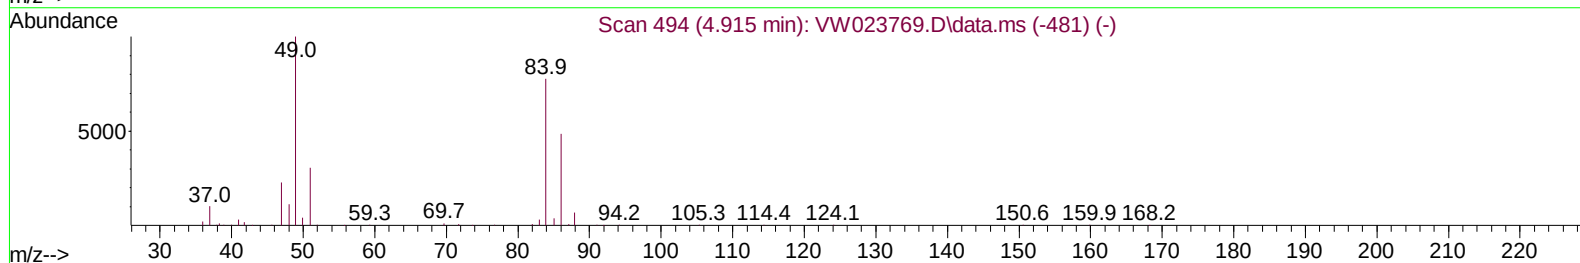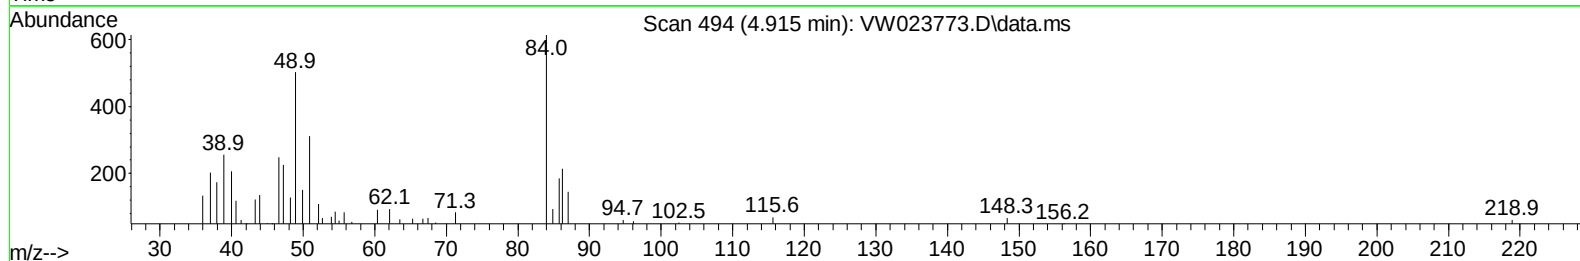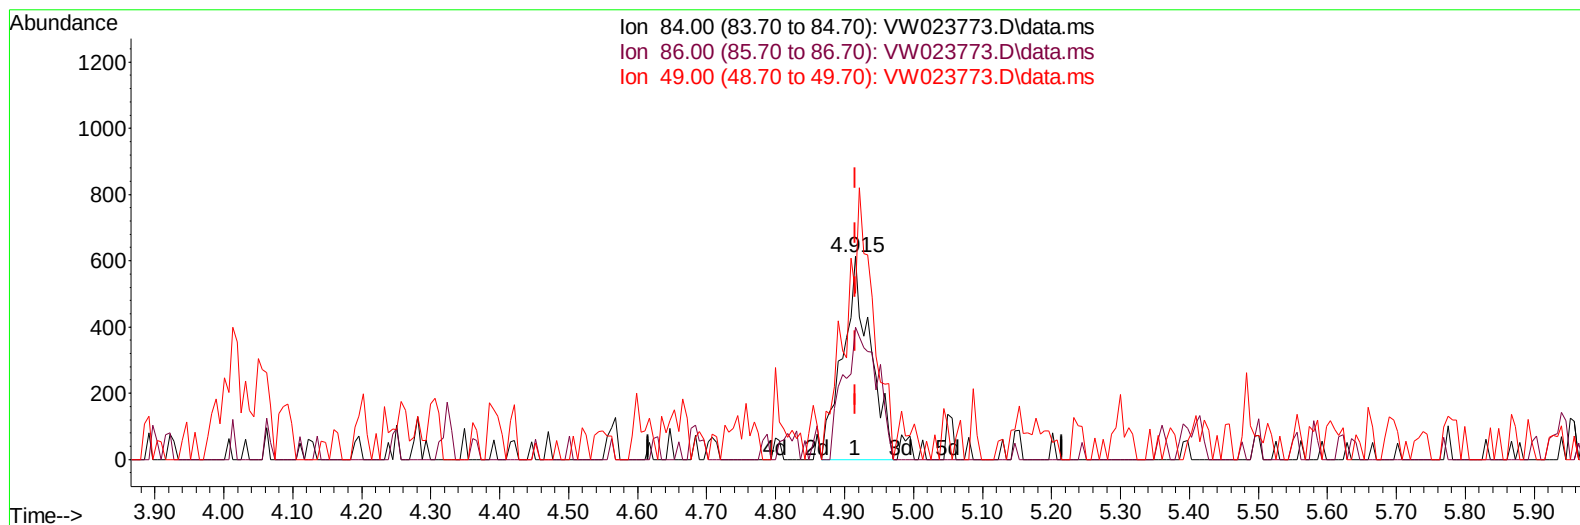

TIC: VW023773.D\data.ms

(16) Methylene chloride (T)

4.915min (-0.000) 4.60 ug/L m

response 1704

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	35.07#
49.00	122.00	81.89#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023773.D
 Acq On : 16 Jul 2022 03:09
 Operator : SY/VA
 Sample : N3700-18RE
 Misc : 6.57g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B59RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

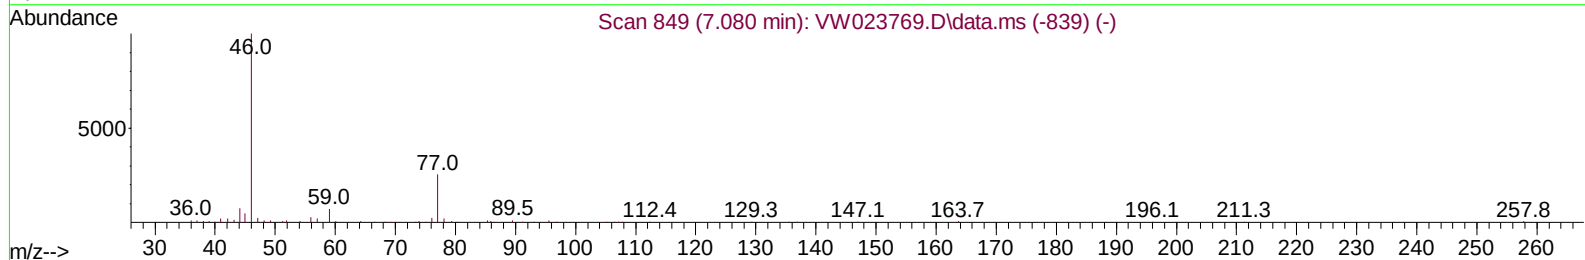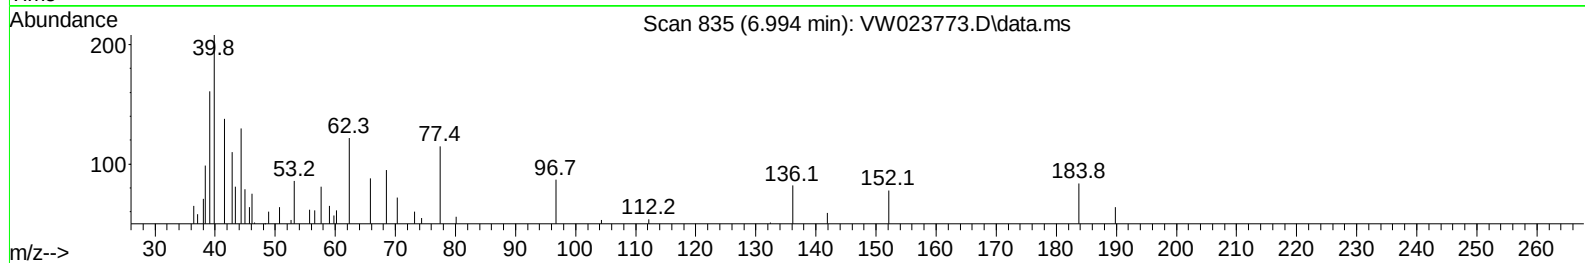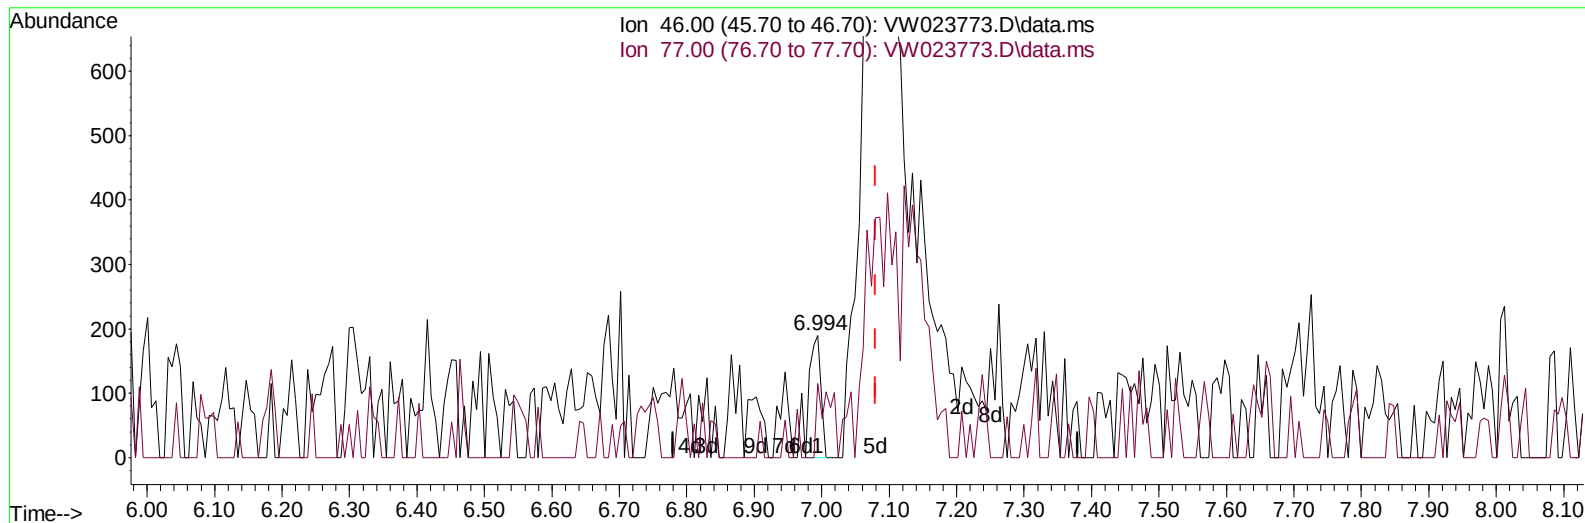

TIC: VW023773.D\data.ms

(21) 2-Butanone-d5 (S)

6.994min (-0.085) 2.26 ug/L

response 212

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	30.19
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023773.D
 Acq On : 16 Jul 2022 03:09
 Operator : SY/VA
 Sample : N3700-18RE
 Misc : 6.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B59RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

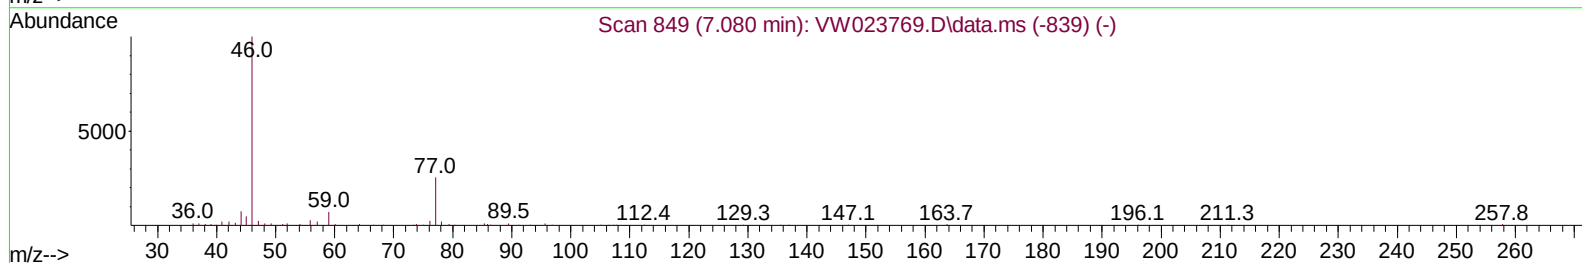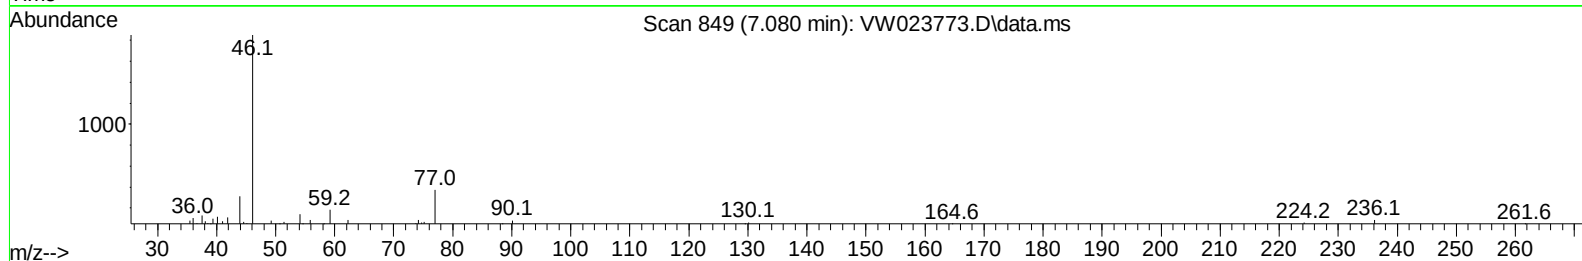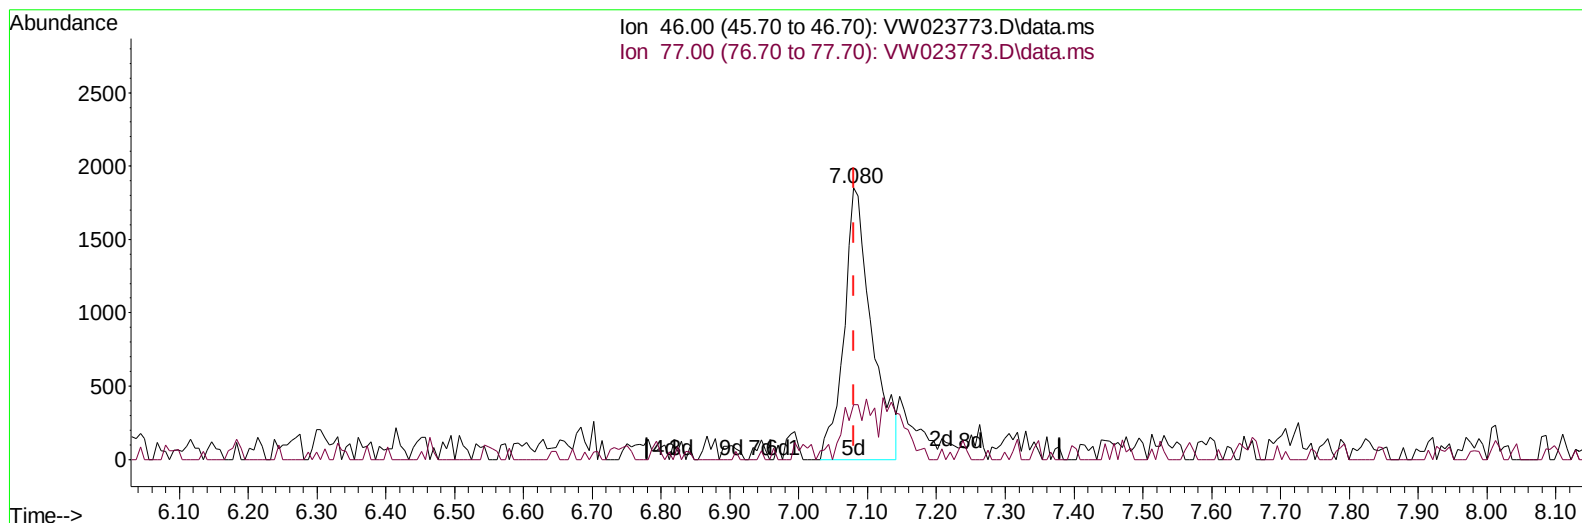

TIC: VW023773.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (-0.000) 54.92 ug/L m

response 5155

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	1.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023773.D
 Acq On : 16 Jul 2022 03:09
 Operator : SY/VA
 Sample : N3700-18RE
 Misc : 6.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B59RE

Manual IntegrationsAPPROVED

Quant Time: Jul 16 04:47:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	23694	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	23398	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	7200	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	15052	24.873	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	99.480%	
7) Chloroethane-d5	2.873	69	13912	34.460	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	137.840%	
11) 1,1-Dichloroethene-d2	4.013	63	10137	20.571	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	82.280%	
21) 2-Butanone-d5	7.080	46	5155m	54.918	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	109.840%	
24) Chloroform-d	7.647	84	18030	26.136	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	104.560%	
26) 1,2-Dichloroethane-d4	8.299	65	9892	23.446	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	93.800%	
32) Benzene-d6	8.275	84	28954	23.805	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	95.200%	
36) 1,2-Dichloropropane-d6	9.274	67	9764	26.650	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	106.600%	
41) Toluene-d8	10.323	98	22798	18.479	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	73.920%	
43) trans-1,3-Dichloroprop...	10.585	79	2664	15.512	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	62.040%	
47) 2-Hexanone-d5	10.927	63	2363	30.672	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	61.340%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	8640	21.339	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	85.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	6362	24.752	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	99.000%	
Target Compounds						
					Qvalue	
13) Acetone	4.141	43	3526m	53.130	ug/L	
14) Carbon disulfide	4.385	76	4828	6.535	ug/L #	91
16) Methylene chloride	4.915	84	1704m	4.599	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023773.D
Acq On : 16 Jul 2022 03:09
Operator : SY/VA
Sample : N3700-18RE
Misc : 6.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B59RE

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 16 04:47:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 16 01:30:01 2022
Response via : Initial Calibration

