




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023786.D
 Acq On : 16 Jul 2022 08:26
 Operator : SY/VA
 Sample : N3701-19
 Misc : 6.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B92

Manual IntegrationsAPPROVED

Quant Time: Jul 18 01:31:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

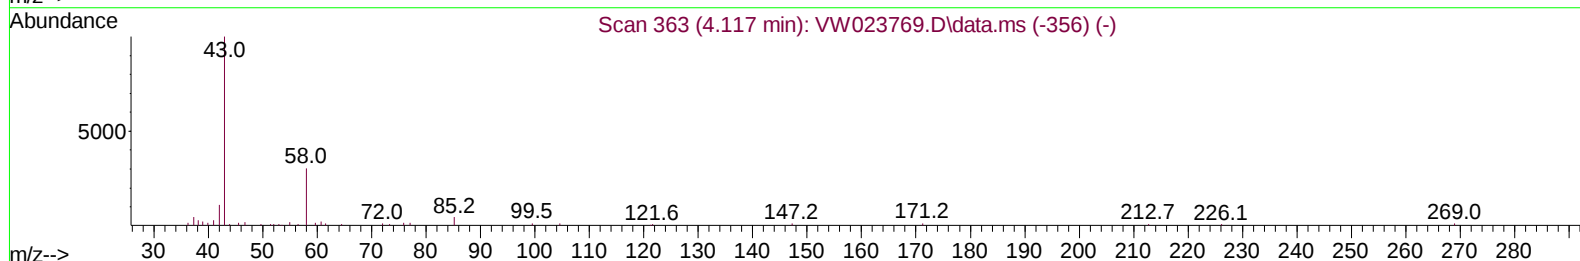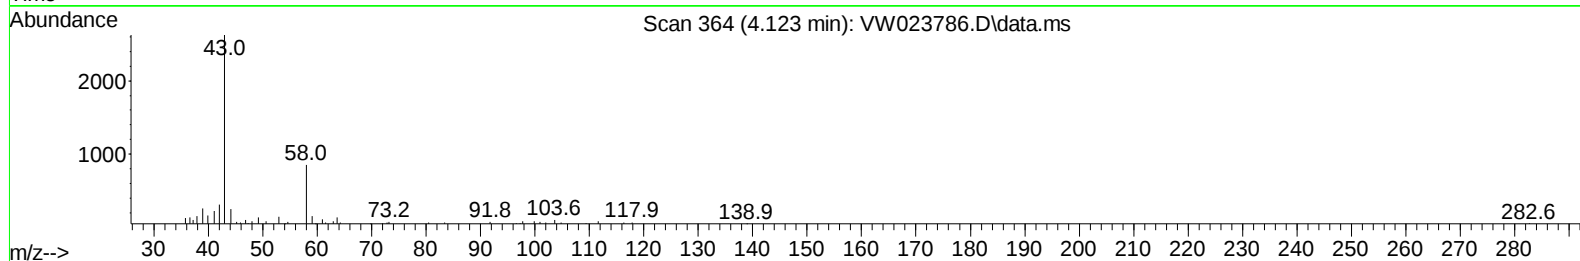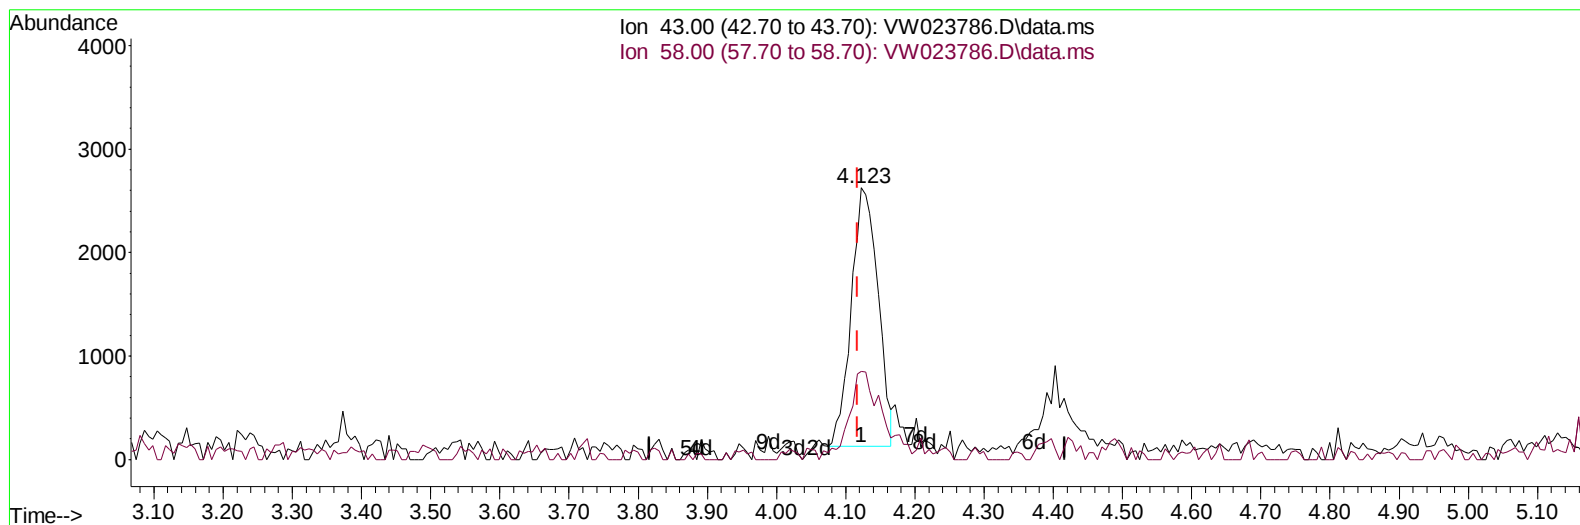

TIC: VW023786.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 13.62 ug/L

response 6692

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	27.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023786.D
 Acq On : 16 Jul 2022 08:26
 Operator : SY/VA
 Sample : N3701-19
 Misc : 6.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B92

Manual IntegrationsAPPROVED

Quant Time: Jul 18 01:31:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

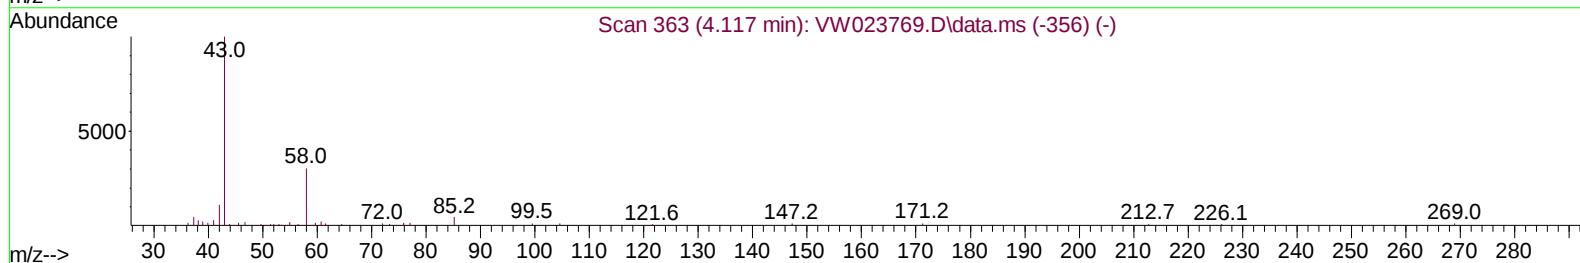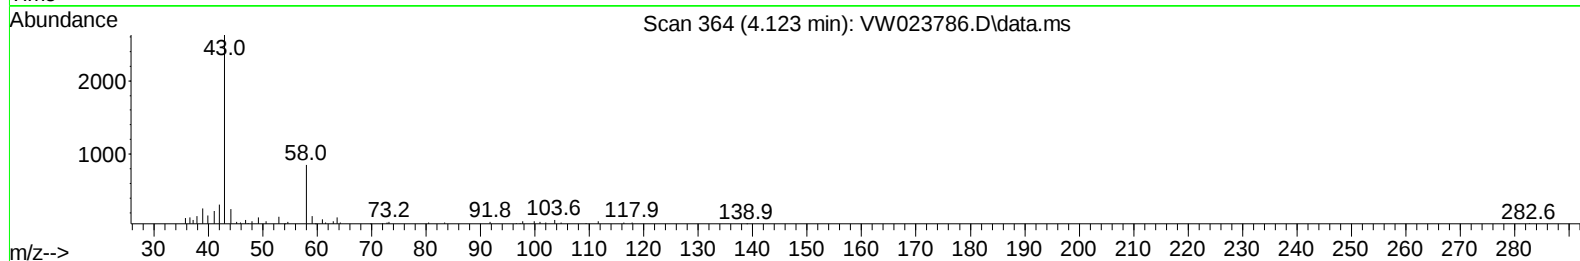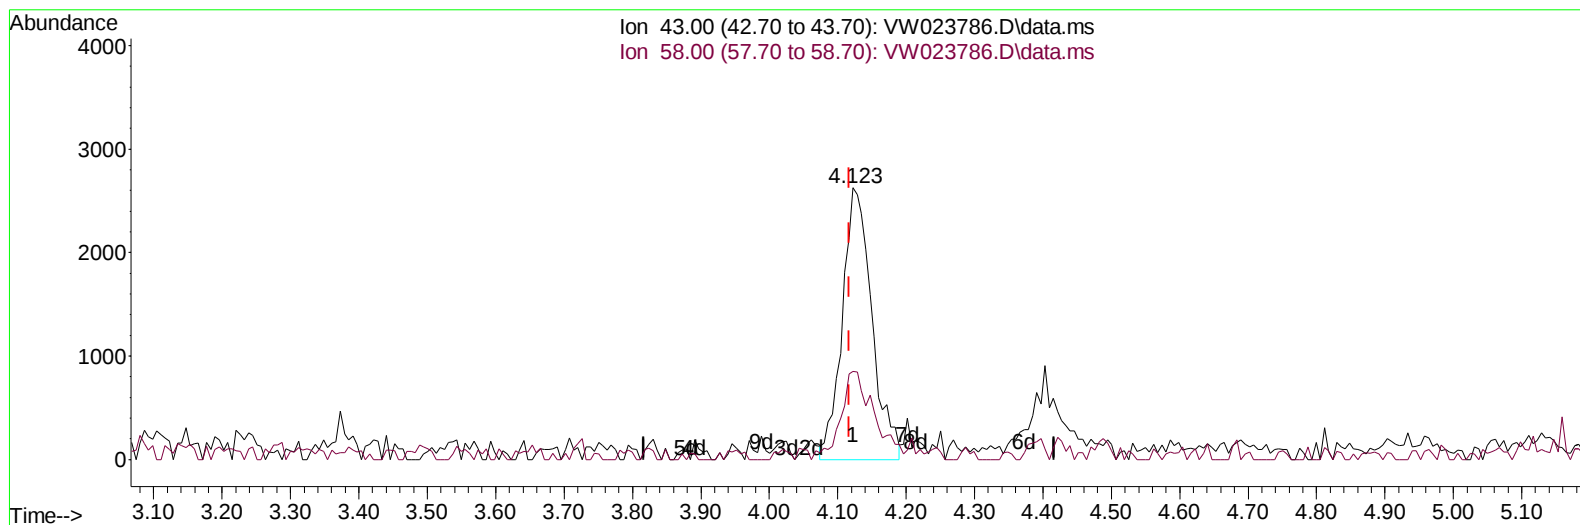

TIC: VW023786.D\data.ms

(13) Acetone (T)

4.123min (+ 0.006) 15.99 ug/L m

response 7855

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	23.48
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023786.D
 Acq On : 16 Jul 2022 08:26
 Operator : SY/VA
 Sample : N3701-19
 Misc : 6.17g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B92

Manual IntegrationsAPPROVED

Quant Time: Jul 18 01:31:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	175397	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	167564	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	62276	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	60686	13.547	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	54.200%	
7) Chloroethane-d5	2.879	69	55836	18.683	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.720%	
11) 1,1-Dichloroethene-d2	4.013	63	36481	10.001	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	40.000%#	
21) 2-Butanone-d5	7.079	46	31147	44.825	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.640%	
24) Chloroform-d	7.646	84	109496	21.442	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	85.760%	
26) 1,2-Dichloroethane-d4	8.305	65	70139	22.457	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	89.840%	
32) Benzene-d6	8.274	84	197012	22.618	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	90.480%	
36) 1,2-Dichloropropane-d6	9.274	67	64976	24.764	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	99.040%	
41) Toluene-d8	10.323	98	170485	19.296	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	77.200%	
43) trans-1,3-Dichloroprop...	10.579	79	17562	14.280	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	57.120%	
47) 2-Hexanone-d5	10.920	63	24173	43.814	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	87.620%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	62065	21.405	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	85.600%	
66) 1,2-Dichlorobenzene-d4	13.853	152	51596	23.209	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.840%	
Target Compounds					Qvalue	
13) Acetone	4.123	43	7855m	15.989	ug/L	
14) Carbon disulfide	4.379	76	18319	3.349	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023786.D
Acq On : 16 Jul 2022 08:26
Operator : SY/VA
Sample : N3701-19
Misc : 6.17g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B92

Manual IntegrationsAPPROVED

Quant Time: Jul 18 01:31:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 16 01:30:01 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

