




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023795.D
 Acq On : 16 Jul 2022 13:40
 Operator : SY/VA
 Sample : VW0715SBL03
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK550

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

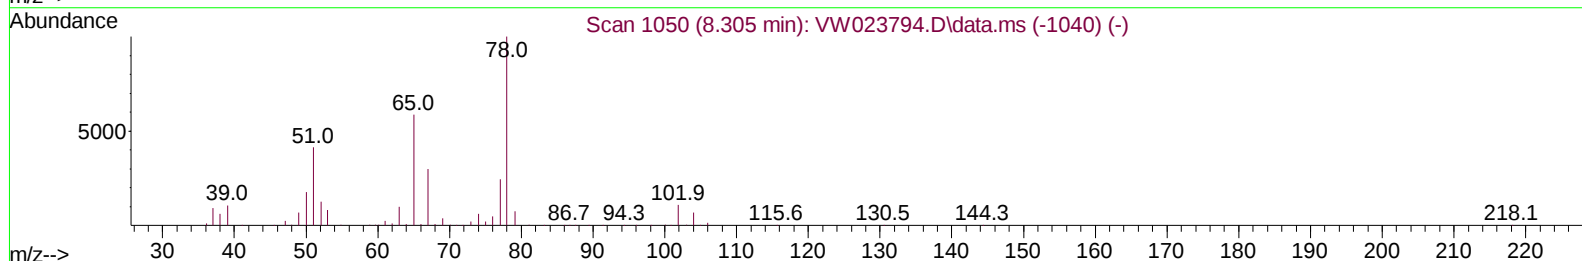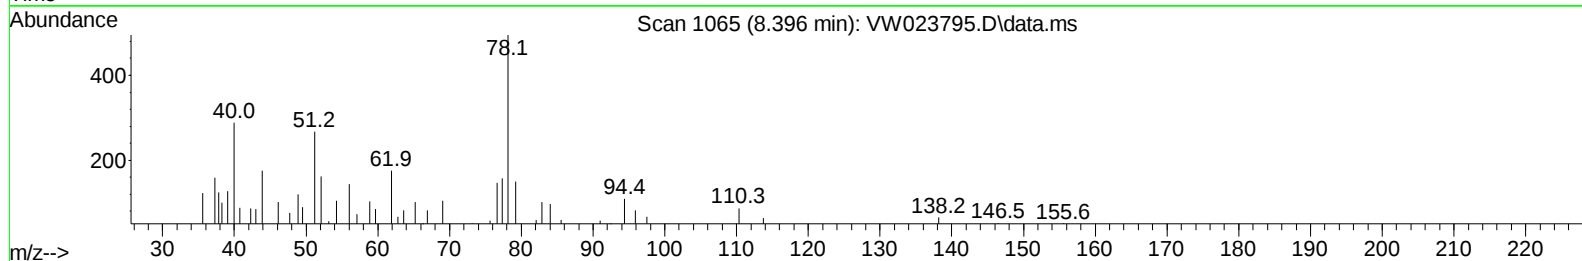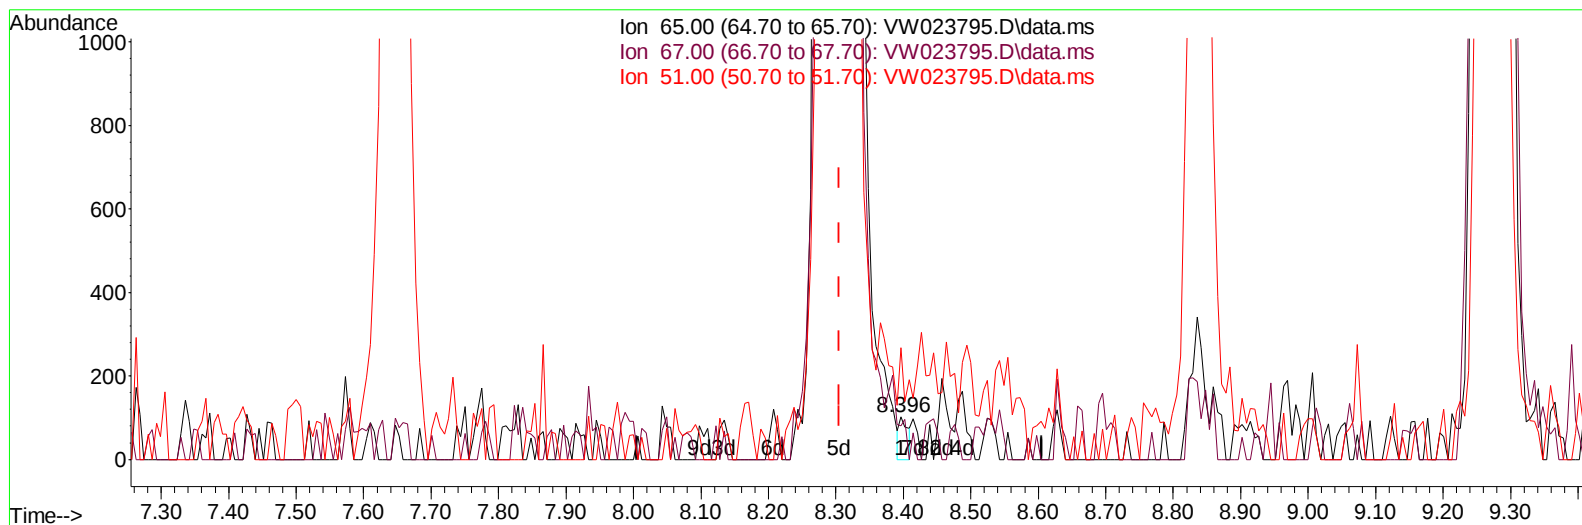

TIC: VW023795.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.396min (+ 0.091) 0.03 ug/L

response 93

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	37.63
51.00	92.20	97.85
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023795.D
 Acq On : 16 Jul 2022 13:40
 Operator : SY/VA
 Sample : VW0715SBL03
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK550

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

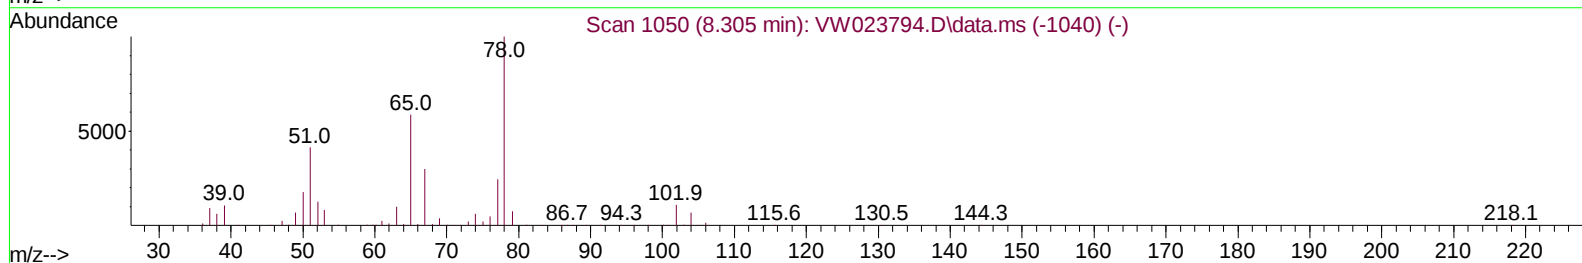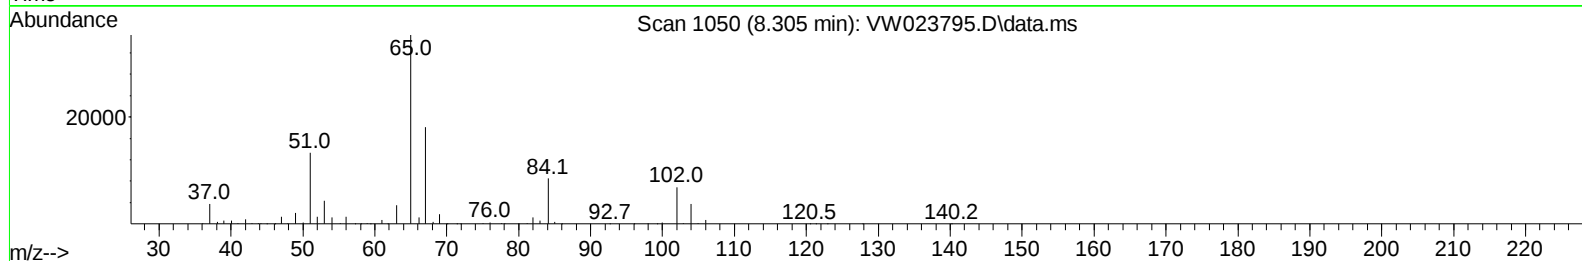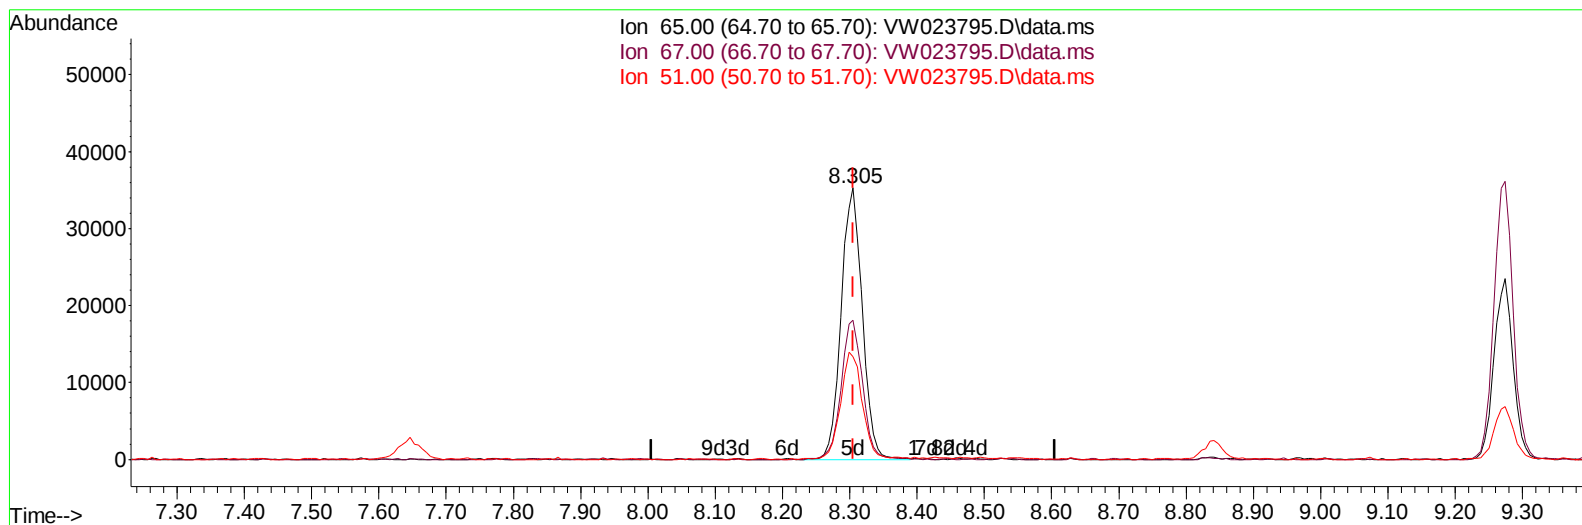

TIC: VW023795.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 23.80 ug/L m

response 76490

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.05#
51.00	92.20	0.12#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023795.D
 Acq On : 16 Jul 2022 13:40
 Operator : SY/VA
 Sample : VW0715SBL03
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK550

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	180517	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	177586	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	80545	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	131503	28.522	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	114.080%	
7) Chloroethane-d5	2.873	69	77209	25.102	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	100.400%	
11) 1,1-Dichloroethene-d2	4.007	63	57381	15.284	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	61.120%	
21) 2-Butanone-d5	7.073	46	32902	46.007	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	92.020%	
24) Chloroform-d	7.647	84	125347	23.850	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.400%	
26) 1,2-Dichloroethane-d4	8.305	65	76490m	23.796	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	95.200%	
32) Benzene-d6	8.268	84	236308	25.598	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	102.400%	
36) 1,2-Dichloropropane-d6	9.274	67	71759	25.806	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	103.240%	
41) Toluene-d8	10.323	98	221997	23.708	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	94.840%	
43) trans-1,3-Dichloroprop...	10.573	79	30402	23.325	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	93.280%	
47) 2-Hexanone-d5	10.920	63	26033	44.522	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.040%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	66510	21.643	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	86.560%	
66) 1,2-Dichlorobenzene-d4	13.853	152	74250	25.824	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	103.280%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023795.D
Acq On : 16 Jul 2022 13:40
Operator : SY/VA
Sample : VW0715SBL03
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK550

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jul 18 02:05:50 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

