




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023796.D
 Acq On : 16 Jul 2022 14:29
 Operator : SY/VA
 Sample : N3702-10
 Misc : 5.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C64

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 18 02:07:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

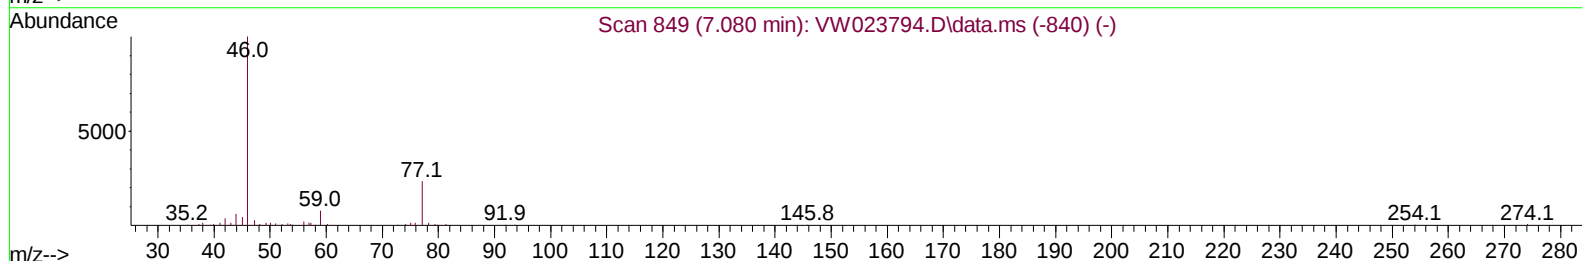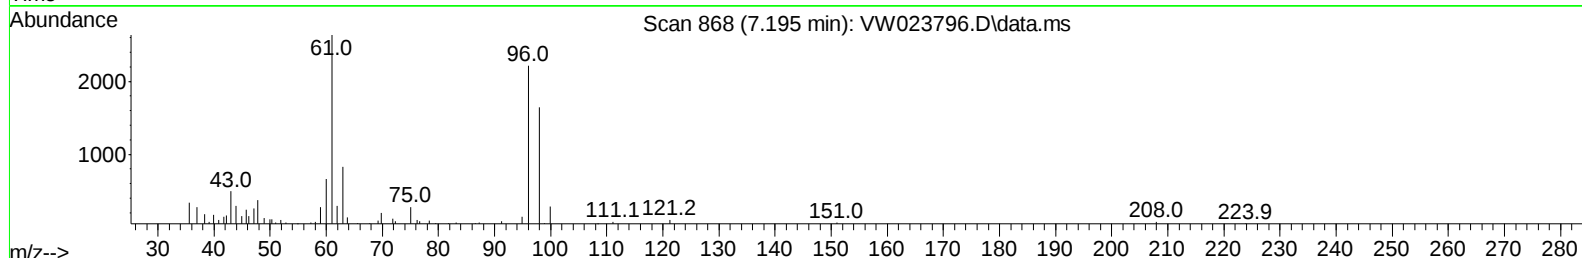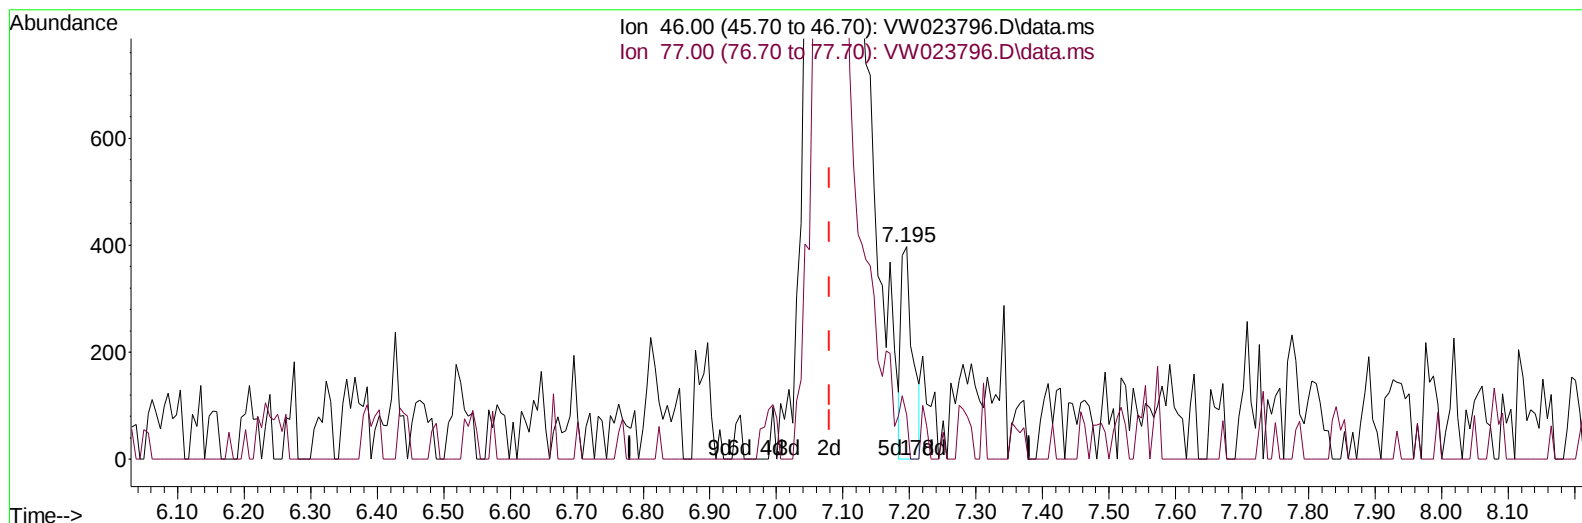

TIC: VW023796.D\data.ms

(21) 2-Butanone-d5 (S)

7.195min (+ 0.116) 0.61 ug/L

response 478

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	21.76
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023796.D
 Acq On : 16 Jul 2022 14:29
 Operator : SY/VA
 Sample : N3702-10
 Misc : 5.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C64

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 18 02:07:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

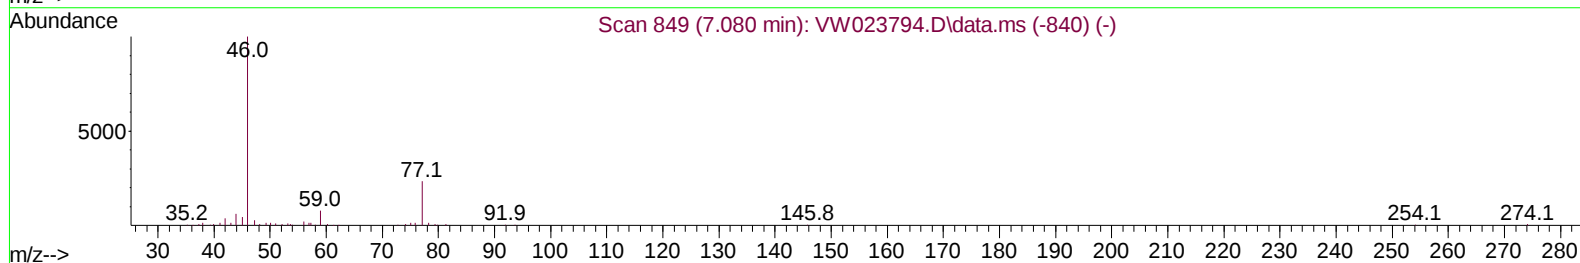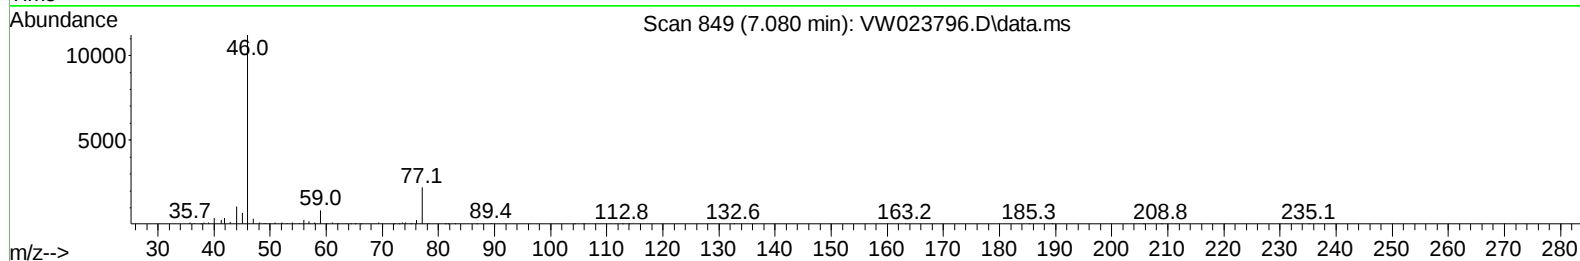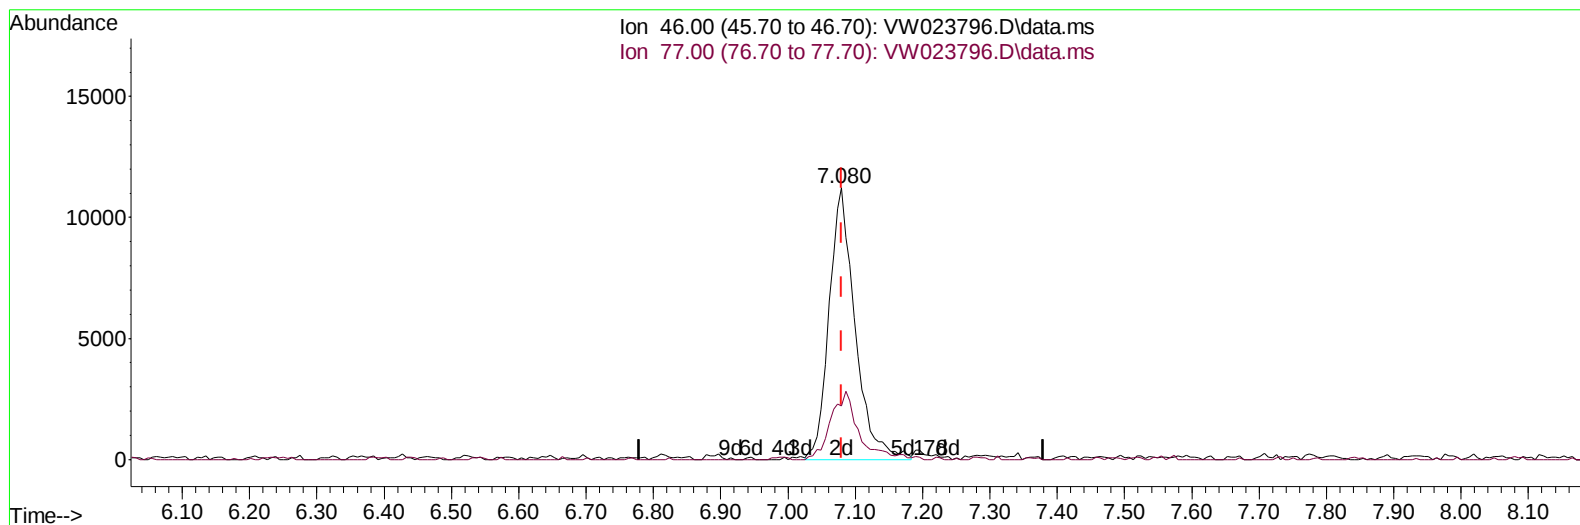

TIC: VW023796.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (-0.000) 38.52 ug/L m

response 30107

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	0.35#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023796.D
 Acq On : 16 Jul 2022 14:29
 Operator : SY/VA
 Sample : N3702-10
 Misc : 5.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C64

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

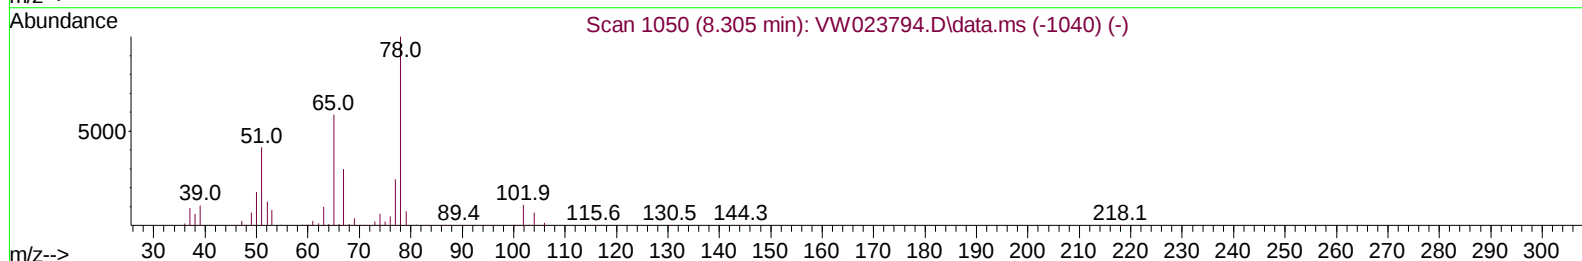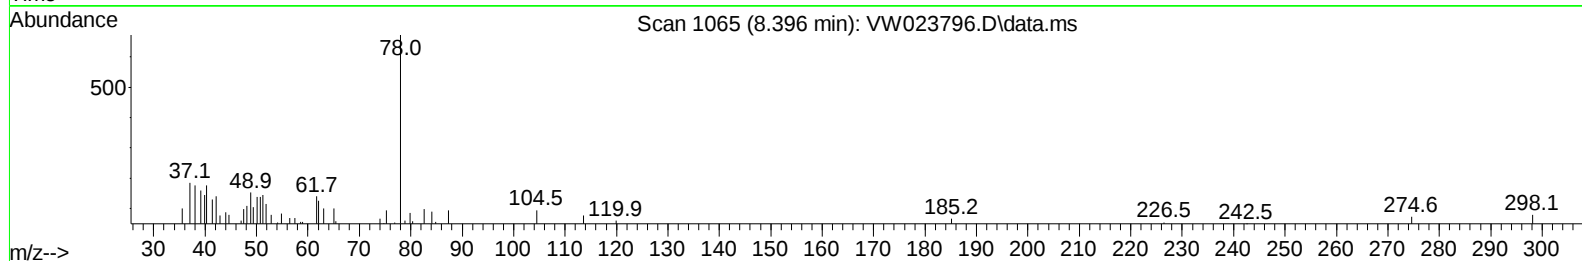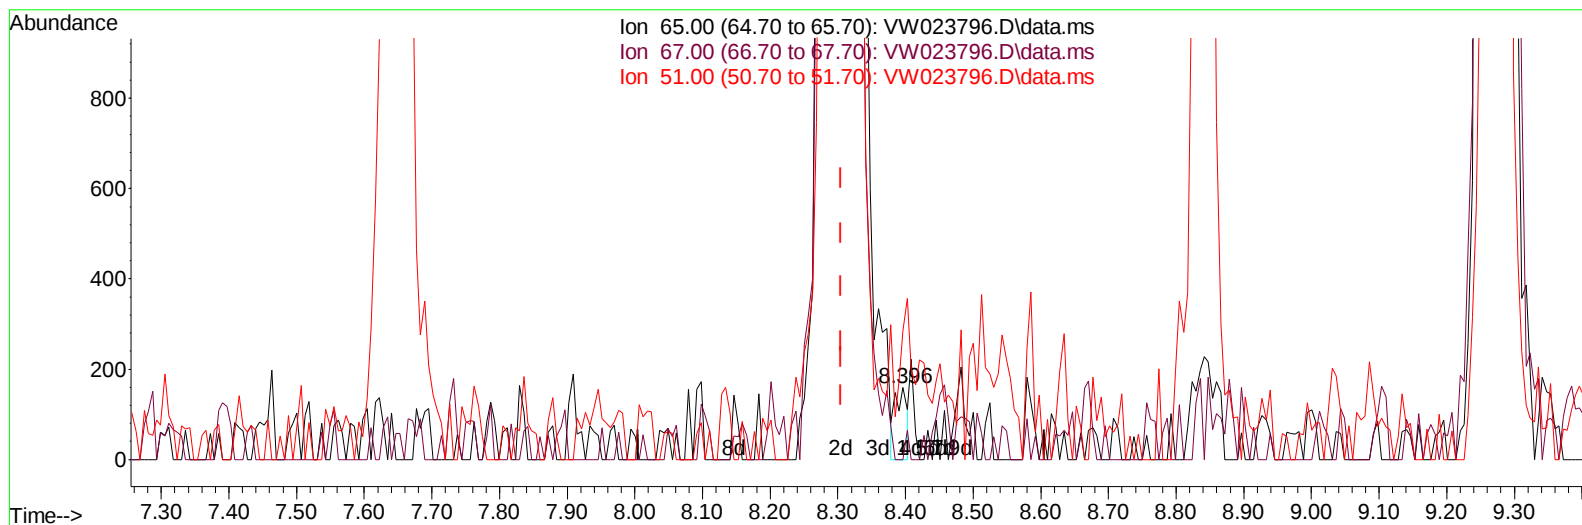

TIC: VW023796.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.396min (+ 0.091) 0.05 ug/L

response 192

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	43.23
51.00	92.20	75.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023796.D
 Acq On : 16 Jul 2022 14:29
 Operator : SY/VA
 Sample : N3702-10
 Misc : 5.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C64

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

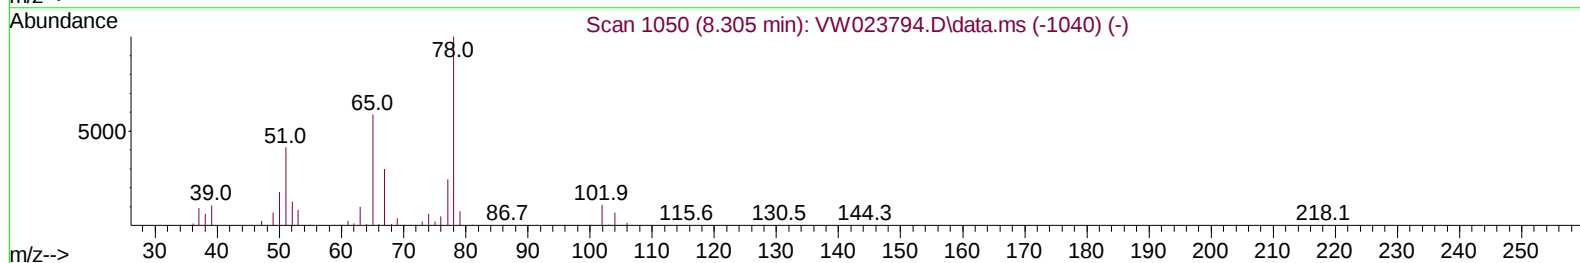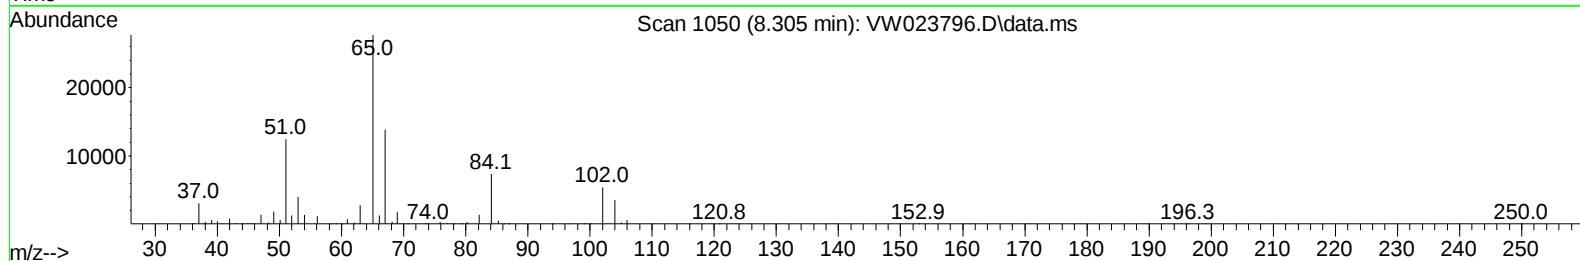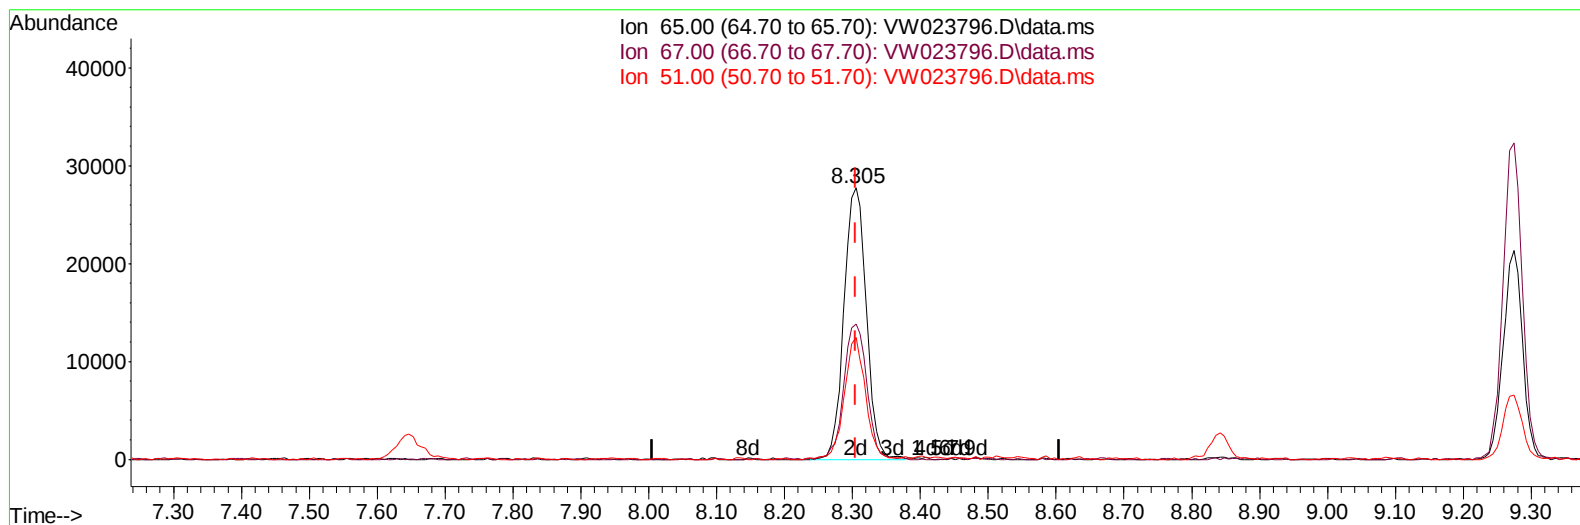

TIC: VW023796.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 18.15 ug/L m

response 63758

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.13#
51.00	92.20	0.23#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023796.D
 Acq On : 16 Jul 2022 14:29
 Operator : SY/VA
 Sample : N3702-10
 Misc : 5.64g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C64

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	197289	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	191177	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	83641	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	82679	16.408	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	65.640%	
7) Chloroethane-d5	2.879	69	60284	17.933	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.720%	
11) 1,1-Dichloroethene-d2	4.013	63	41530	10.121	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	40.480%#	
21) 2-Butanone-d5	7.080	46	30107m	38.520	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	77.040%	
24) Chloroform-d	7.647	84	108885	18.956	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	75.840%	
26) 1,2-Dichloroethane-d4	8.305	65	63758m	18.149	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	72.600%	
32) Benzene-d6	8.275	84	192074	19.327	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	77.320%	
36) 1,2-Dichloropropane-d6	9.274	67	64319	21.486	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	85.960%	
41) Toluene-d8	10.323	98	179016	17.759	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	71.040%	
43) trans-1,3-Dichloroprop...	10.579	79	23643	16.850	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	67.400%	
47) 2-Hexanone-d5	10.920	63	24652	39.163	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	78.320%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	61499	18.590	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	74.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	67860	22.728	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	90.920%	
Target Compounds						
					Qvalue	
5) vinyl chloride	2.355	62	62798	11.139	ug/L	98
13) Acetone	4.129	43	9497	17.186	ug/L	63
20) cis-1,2-Dichloroethene	7.165	96	21103	7.507	ug/L #	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023796.D
Acq On : 16 Jul 2022 14:29
Operator : SY/VA
Sample : N3702-10
Misc : 5.64g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C64

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jul 18 02:05:50 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

