




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023797.D
 Acq On : 16 Jul 2022 14:53
 Operator : SY/VA
 Sample : N3702-11
 Misc : 6.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C65

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

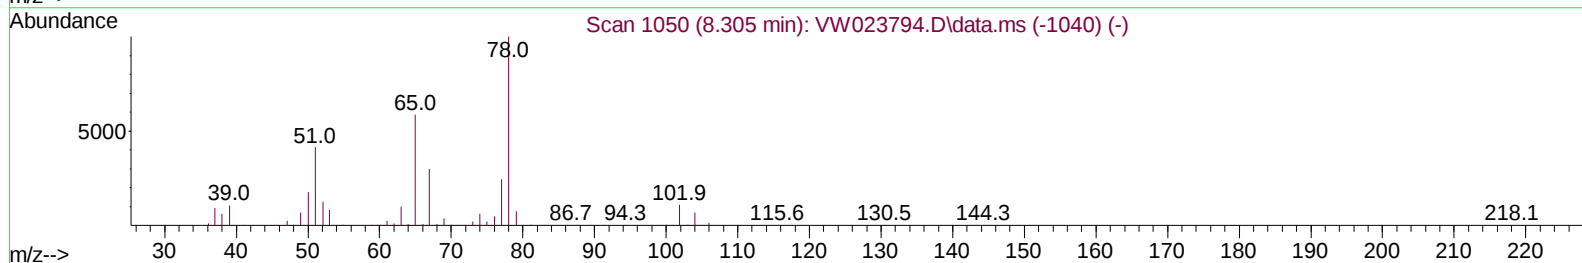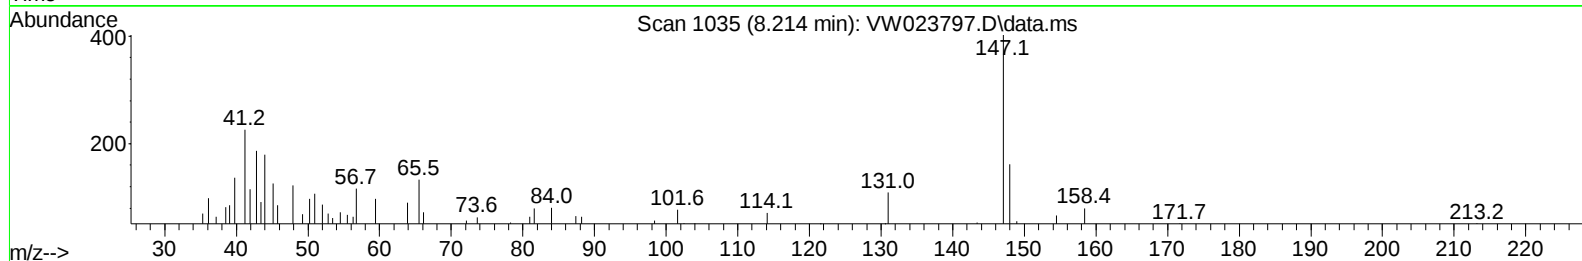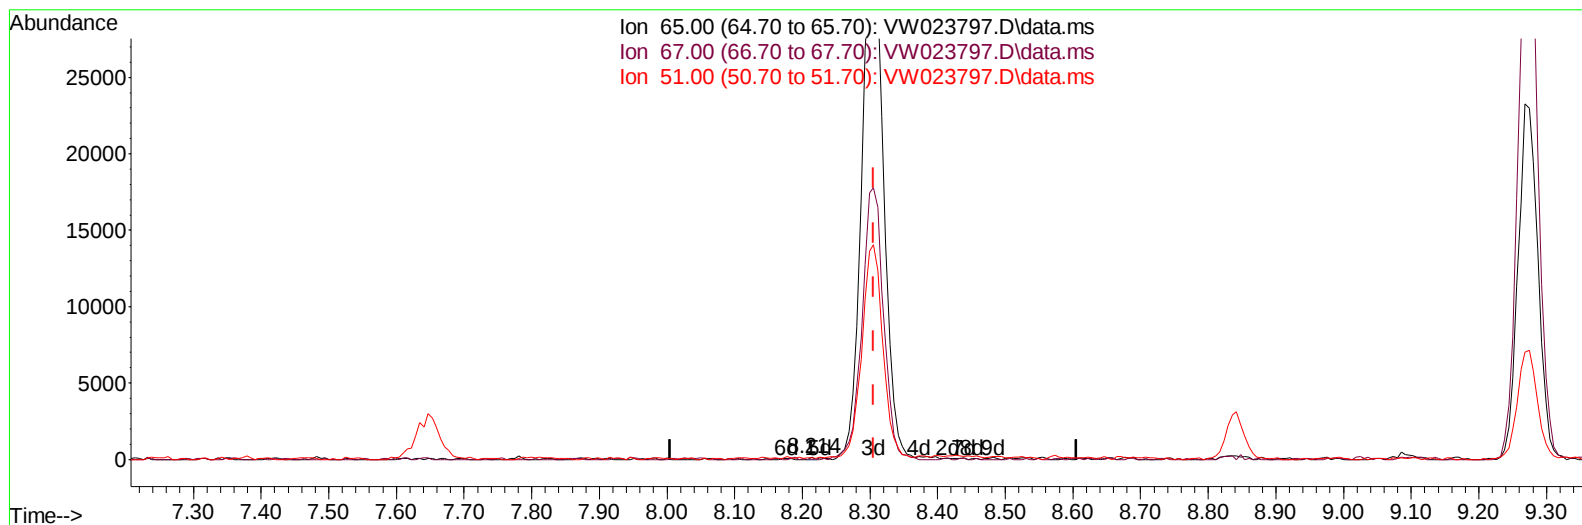

TIC: VW023797.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.214min (-0.091) 0.01 ug/L

response 49

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	40.82
51.00	92.20	83.67
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023797.D
 Acq On : 16 Jul 2022 14:53
 Operator : SY/VA
 Sample : N3702-11
 Misc : 6.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C65

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

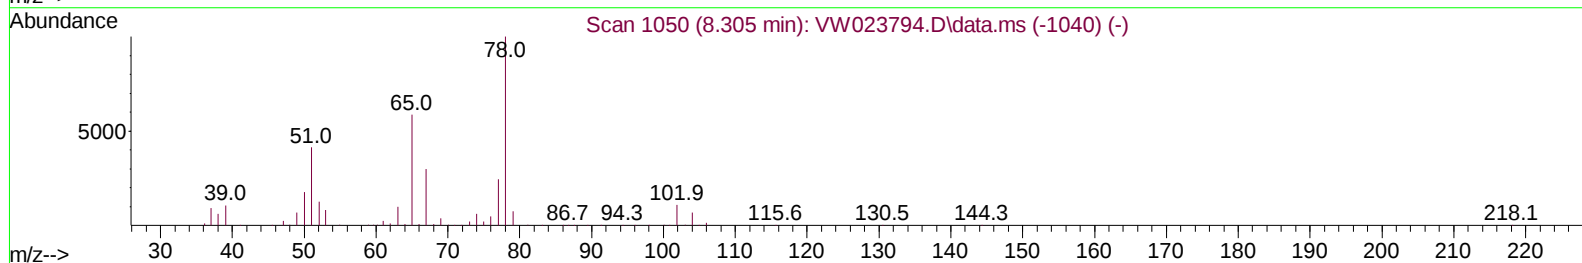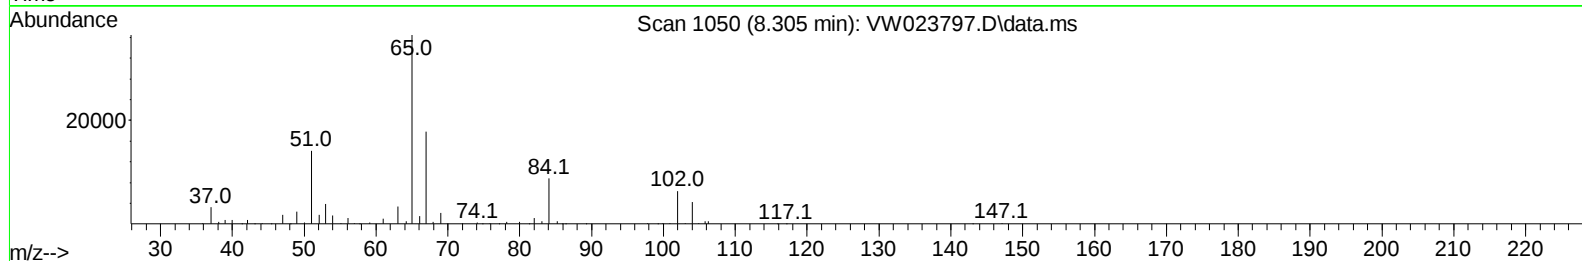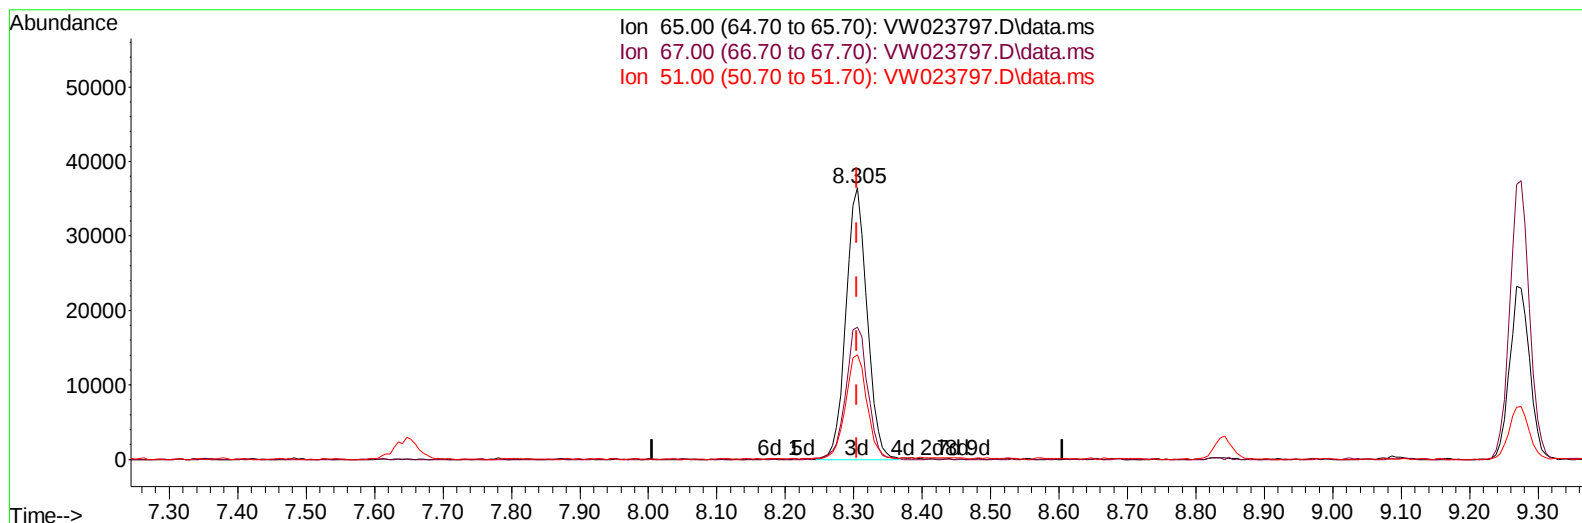

TIC: VW023797.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 19.64 ug/L m

response 77476

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.03#
51.00	92.20	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023797.D
 Acq On : 16 Jul 2022 14:53
 Operator : SY/VA
 Sample : N3702-11
 Misc : 6.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C65

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:07:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:05:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	221536	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	210792	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	87717	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	83207	14.706	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	58.840%	
7) Chloroethane-d5	2.873	69	67656	17.924	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.680%	
11) 1,1-Dichloroethene-d2	4.007	63	50490	10.958	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	43.840%#	
21) 2-Butanone-d5	7.074	46	40713	46.389	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	92.780%	
24) Chloroform-d	7.647	84	129705	20.109	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	80.440%	
26) 1,2-Dichloroethane-d4	8.305	65	77476m	19.640	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	78.560%	
32) Benzene-d6	8.269	84	221456	20.210	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	80.840%	
36) 1,2-Dichloropropane-d6	9.275	67	75159	22.771	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	91.080%	
41) Toluene-d8	10.323	98	204996	18.444	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	73.760%	
43) trans-1,3-Dichloroprop...	10.573	79	28669	18.530	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	74.120%	
47) 2-Hexanone-d5	10.921	63	32772	47.218	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	94.440%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	73440	20.134	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	80.520%	
66) 1,2-Dichlorobenzene-d4	13.847	152	69722	22.266	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	89.080%	
Target Compounds						
					Qvalue	
13) Acetone	4.123	43	8473	13.655	ug/L	93
20) cis-1,2-Dichloroethene	7.165	96	16960	5.373	ug/L #	97
34) Trichloroethene	9.086	95	36121	11.419	ug/L	90
46) Tetrachloroethene	10.860	164	28385	11.605	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023797.D
Acq On : 16 Jul 2022 14:53
Operator : SY/VA
Sample : N3702-11
Misc : 6.30g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C65

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 18 02:07:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jul 18 02:05:50 2022
Response via : Initial Calibration

