

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023827.D
 Acq On : 17 Jul 2022 08:16
 Operator : SY/VA
 Sample : N3721-10
 Misc : 5.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 F5C30

Manual IntegrationsAPPROVED

Quant Time: Jul 18 03:04:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:58:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

07/18/2022
 Supervised By :Mahesh
 Dadoda

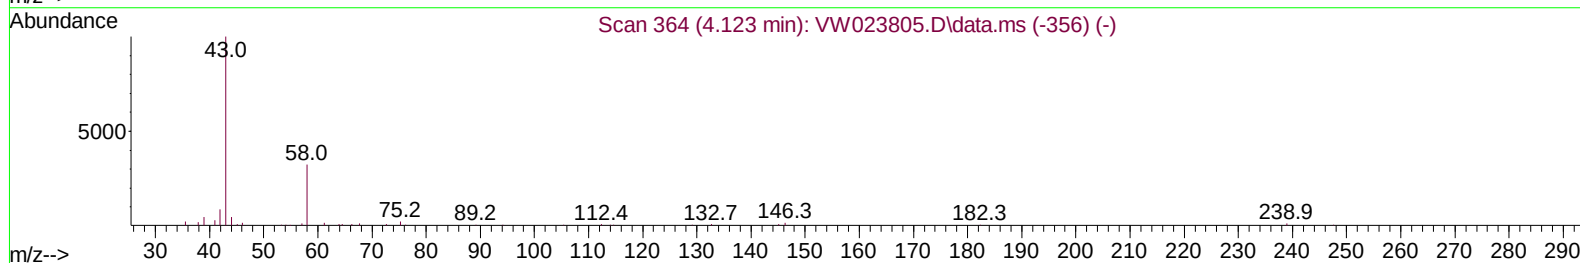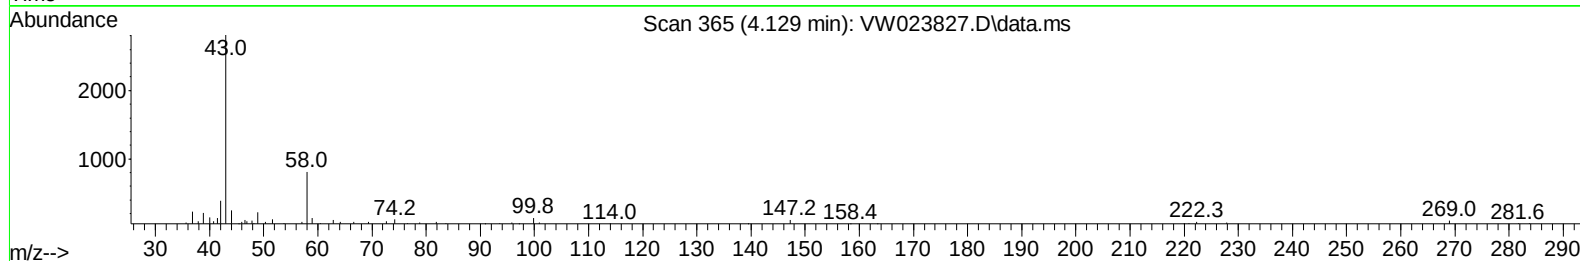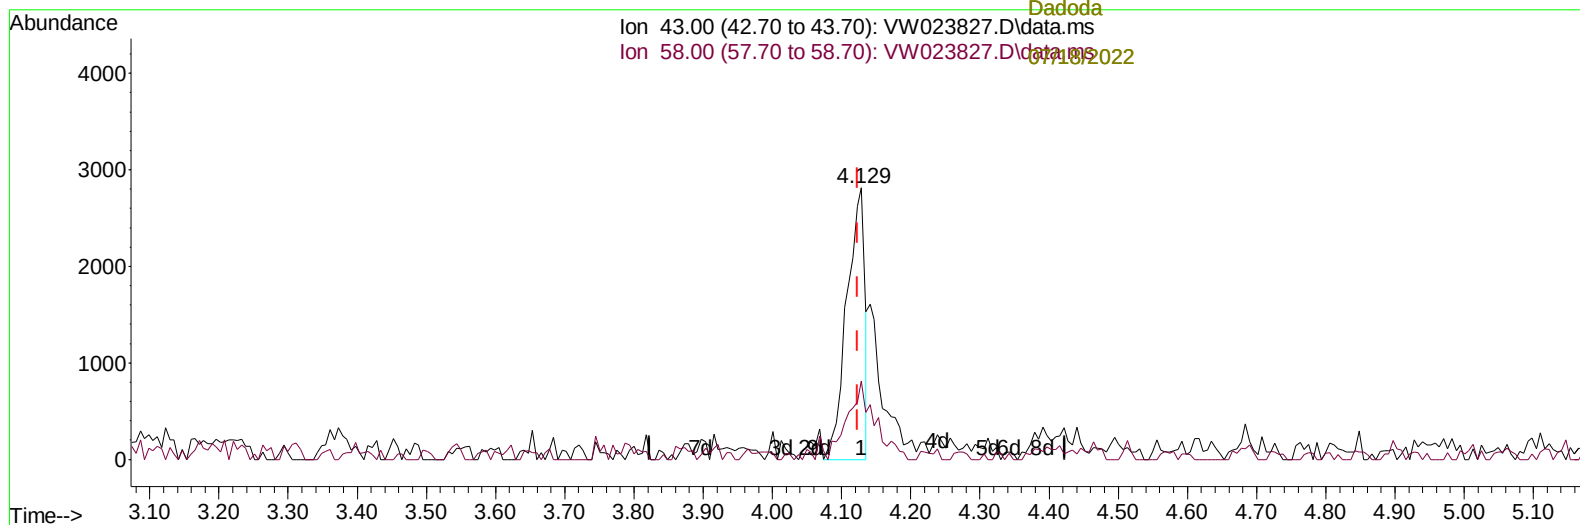

TIC: VW023827.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 11.46 ug/L

response 5102

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	40.14
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023827.D
 Acq On : 17 Jul 2022 08:16
 Operator : SY/VA
 Sample : N3721-10
 Misc : 5.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 F5C30

Manual IntegrationsAPPROVED

Quant Time: Jul 18 03:04:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:58:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

07/18/2022
 Supervised By :Mahesh
 Dadoda
 07/18/2022

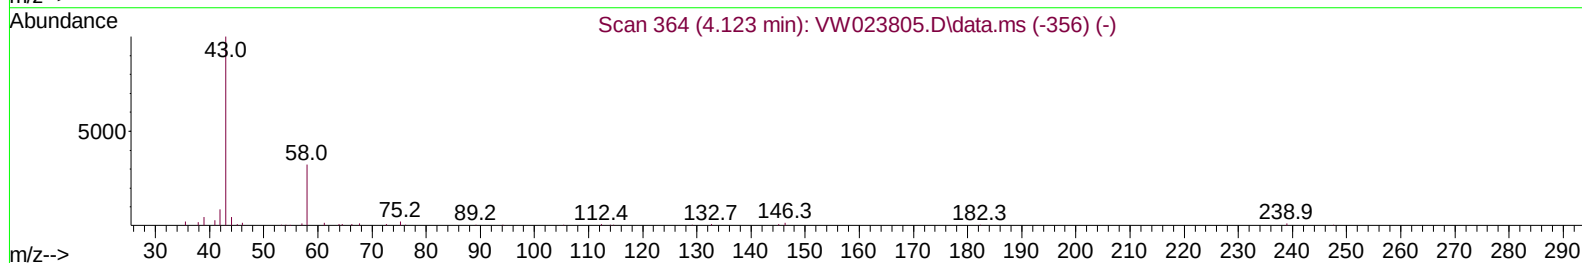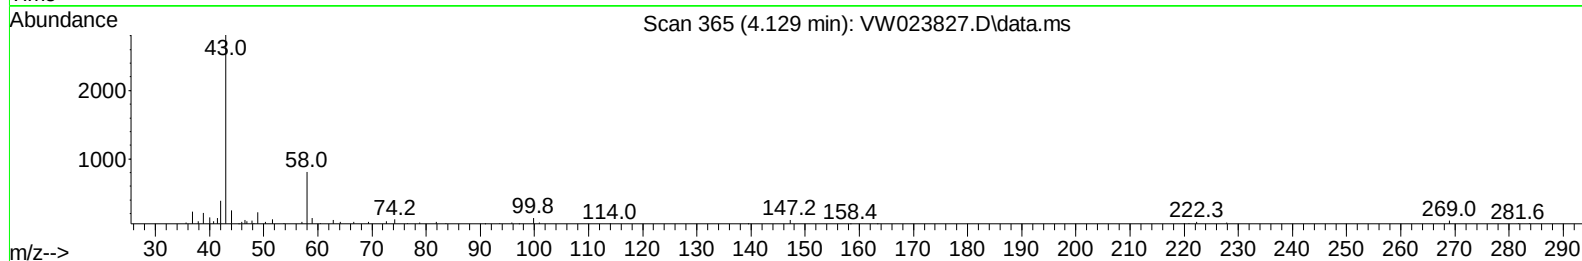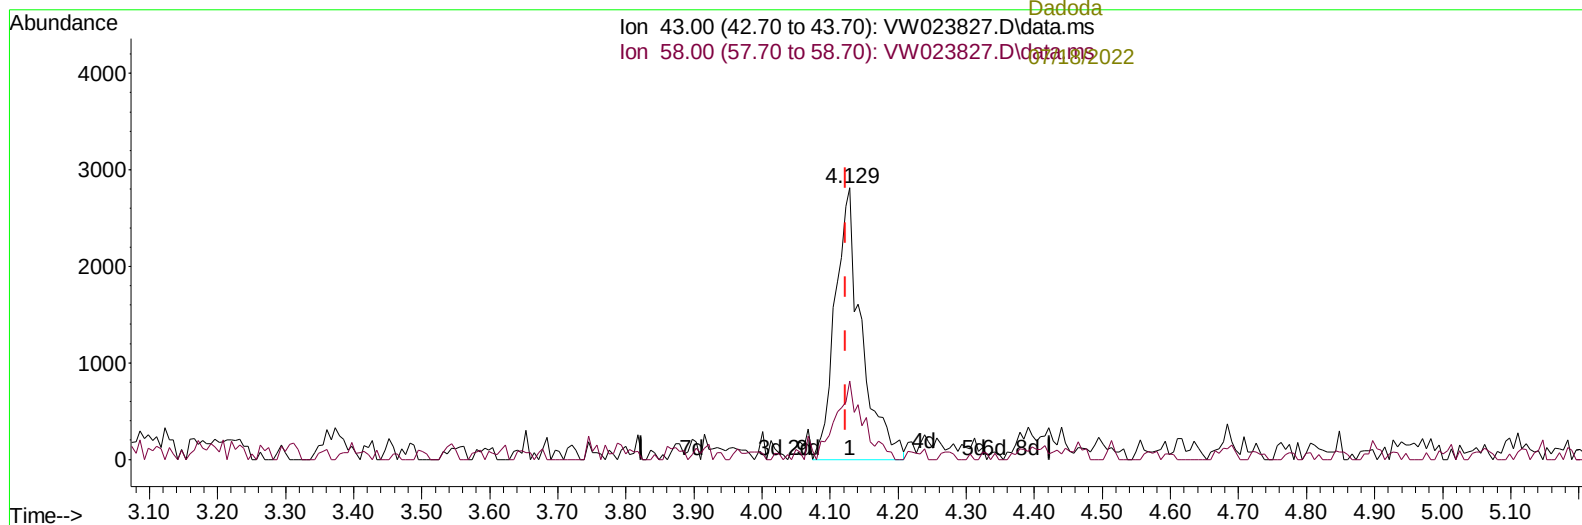

TIC: VW023827.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 16.98 ug/L m

response 7556

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	27.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023827.D
 Acq On : 17 Jul 2022 08:16
 Operator : SY/VA
 Sample : N3721-10
 Misc : 5.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C30

Manual IntegrationsAPPROVED

Quant Time: Jul 18 03:04:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:58:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

07/18/2022
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----07/18/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	158897	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	149582	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	55282	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	68286	16.826	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.320%	
7) Chloroethane-d5	2.879	69	60669	22.409	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	89.640%	
11) 1,1-Dichloroethene-d2	4.013	63	36261	10.972	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	43.880%#	
21) 2-Butanone-d5	7.080	46	22823	36.256	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	72.520%	
24) Chloroform-d	7.647	84	91982	19.883	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	79.520%	
26) 1,2-Dichloroethane-d4	8.305	65	49838	17.614	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	70.440%	
32) Benzene-d6	8.274	84	157027	20.194	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	80.760%	
36) 1,2-Dichloropropane-d6	9.274	67	53076	22.661	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	90.640%	
41) Toluene-d8	10.323	98	144724	18.349	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	73.400%	
43) trans-1,3-Dichloroprop...	10.573	79	13139	11.968	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	47.880%	
47) 2-Hexanone-d5	10.920	63	17313	35.152	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	70.300%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	43154	16.672	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	66.680%	
66) 1,2-Dichlorobenzene-d4	13.853	152	44456	22.527	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	90.120%	
Target Compounds						
5) vinyl chloride	2.355	62	54526	12.008	ug/L	95
13) Acetone	4.129	43	7556m	16.977	ug/L	
14) Carbon disulfide	4.379	76	13175	2.659	ug/L #	92
20) cis-1,2-Dichloroethene	7.171	96	42054	18.575	ug/L #	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023827.D
Acq On : 17 Jul 2022 08:16
Operator : SY/VA
Sample : N3721-10
Misc : 5.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C30

Manual IntegrationsAPPROVED

Quant Time: Jul 18 03:04:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jul 18 02:58:45 2022
Response via : Initial Calibration

Reviewed By :Krupa
Patel

07/18/2022
Supervised By :Mahesh
Dadoda

07/18/2022

