

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023762.D
 Acq On : 15 Jul 2022 22:16
 Operator : SY/VA
 Sample : N3698-17
 Misc : 5.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C04

Quant Time: Jul 15 22:41:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	202734	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	188914	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	75761	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	97081	18.749	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.000%
7) Chloroethane-d5	2.873	69	75950	21.987	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.960%
11) 1,1-Dichloroethene-d2	4.007	63	49029	11.628	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.520%
21) 2-Butanone-d5	7.080	46	30926	38.505	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.020%
24) Chloroform-d	7.647	84	123278	20.886	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.560%
26) 1,2-Dichloroethane-d4	8.305	65	69649	19.293	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	77.160%
32) Benzene-d6	8.269	84	224050	22.815	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.240%
36) 1,2-Dichloropropane-d6	9.274	67	68438	23.136	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.560%
41) Toluene-d8	10.323	98	205138	20.594	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.360%
43) trans-1,3-Dichloroprop...	10.573	79	22544	16.259	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.040%
47) 2-Hexanone-d5	10.927	63	22857	36.746	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.500%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	60878	18.623	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	74.480%
66) 1,2-Dichlorobenzene-d4	13.853	152	61898	22.887	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.560%
Target Compounds						
13) Acetone	4.117	43	10173	17.915	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023762.D
Acq On : 15 Jul 2022 22:16
Operator : SY/VA
Sample : N3698-17
Misc : 5.35g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C04

Quant Time: Jul 15 22:41:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 06:03:21 2022
Response via : Initial Calibration

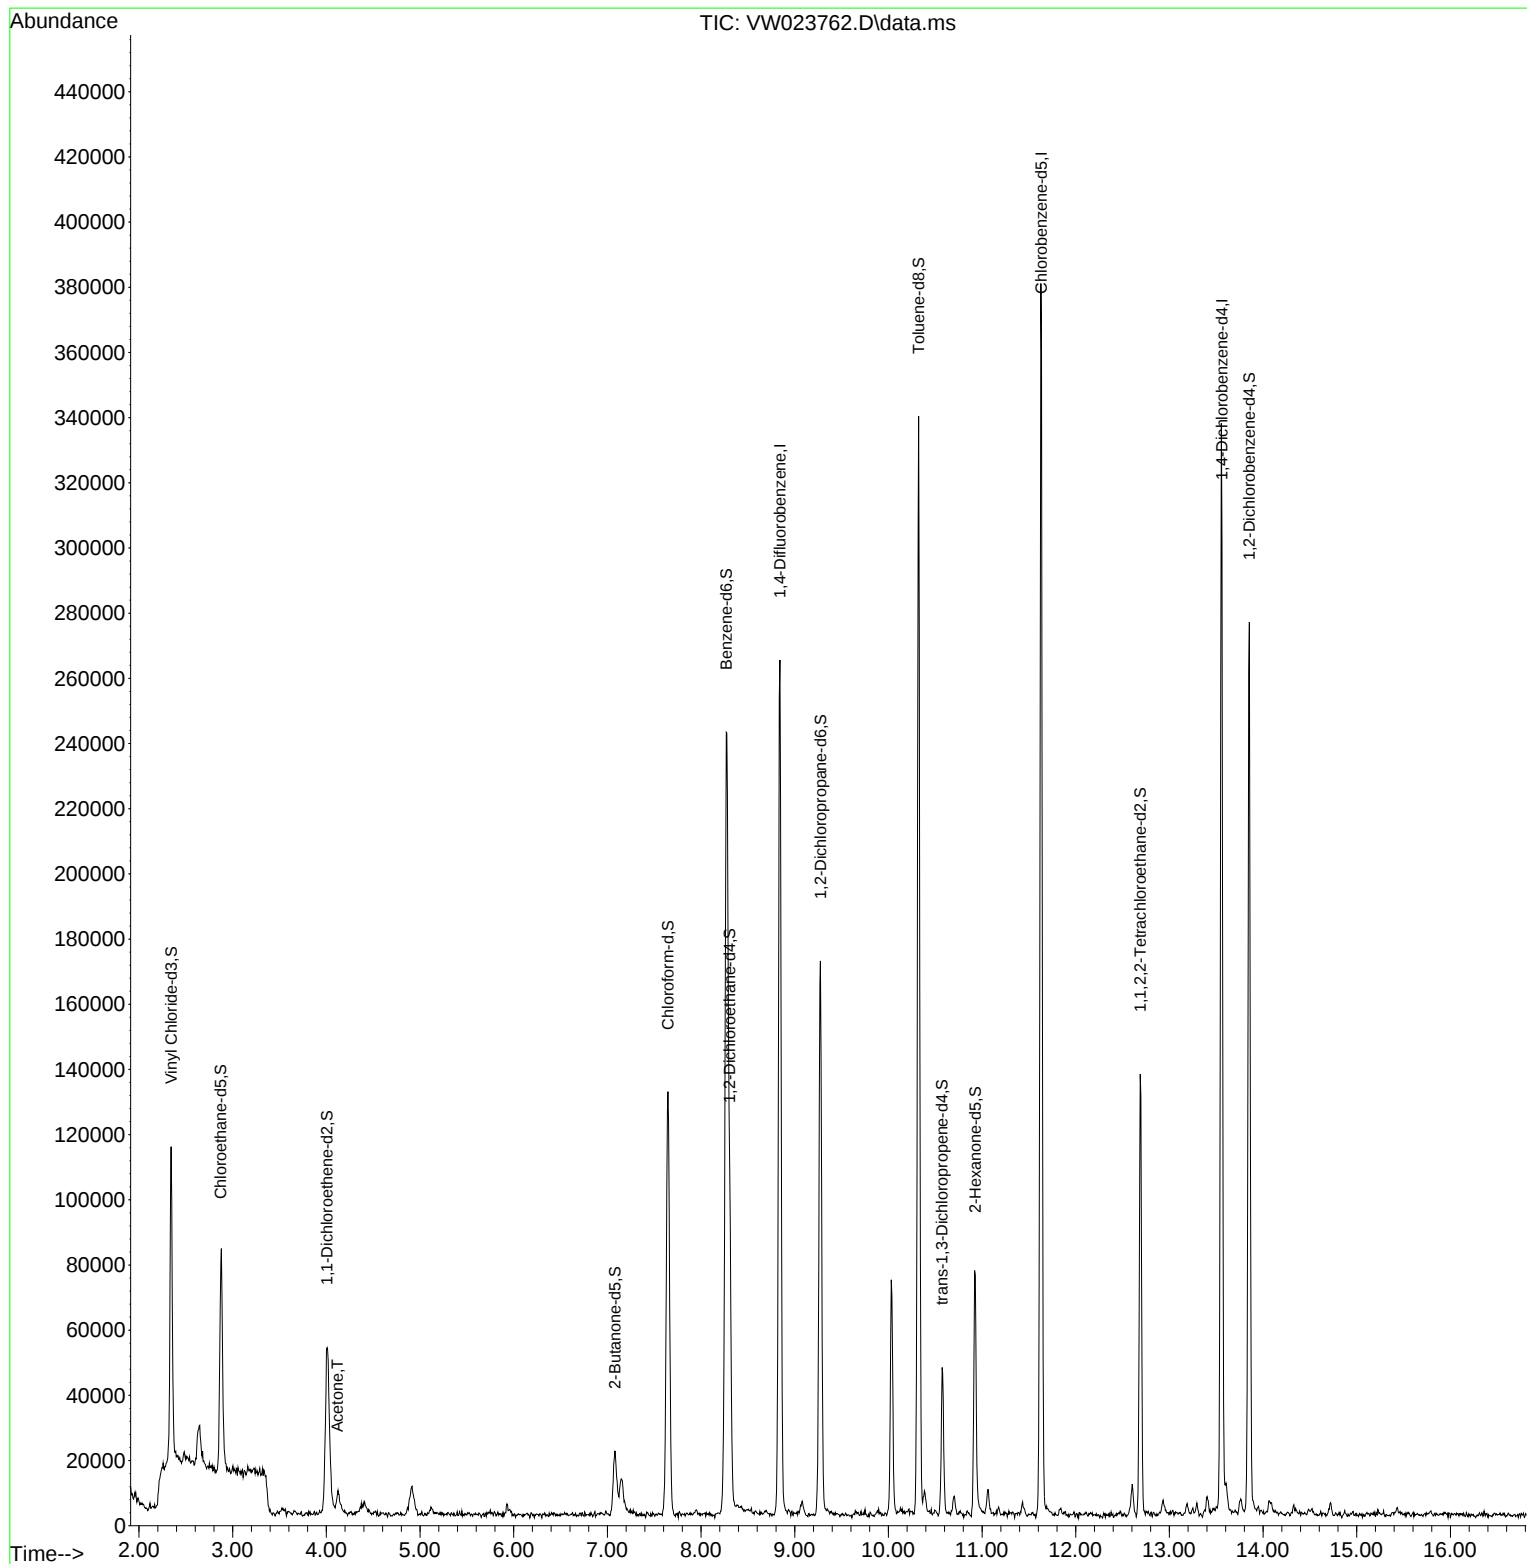

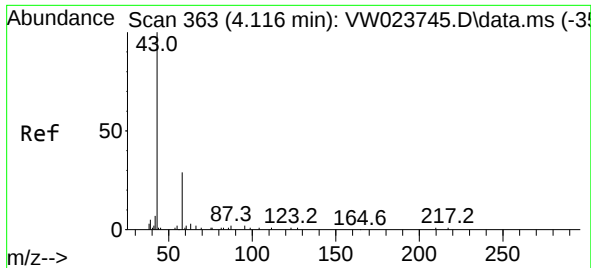

#13
 Acetone
 Concen: 17.915 ug/L
 RT: 4.117 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: VW023762.D
 Acq: 15 Jul 2022 22:16

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C04

Tgt Ion: 43 Resp: 10173
 Ion Ratio Lower Upper
 43 100
 58 24.4 0.0 64.2

