

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023765.D
 Acq On : 15 Jul 2022 23:29
 Operator : SY/VA
 Sample : N3698-20
 Misc : 4.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C07

Quant Time: Jul 16 00:16:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	198179	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	182211	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	68586	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	89180	17.619	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.480%
7) Chloroethane-d5	2.873	69	69892	20.698	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.800%
11) 1,1-Dichloroethene-d2	4.013	63	46381	11.253	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	45.000%
21) 2-Butanone-d5	7.080	46	30813	39.246	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.500%
24) Chloroform-d	7.647	84	119310	20.678	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.720%
26) 1,2-Dichloroethane-d4	8.299	65	69997	19.835	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.360%
32) Benzene-d6	8.268	84	214718	22.669	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.680%
36) 1,2-Dichloropropane-d6	9.274	67	67988	23.829	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.320%
41) Toluene-d8	10.323	98	191545	19.937	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.760%
43) trans-1,3-Dichloroprop...	10.579	79	21034	15.728	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	62.920%
47) 2-Hexanone-d5	10.920	63	22959	38.268	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.540%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	57412	18.208	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	72.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	53550	21.872	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.480%
Target Compounds						
13) Acetone	4.123	43	8838	15.922	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023765.D
Acq On : 15 Jul 2022 23:29
Operator : SY/VA
Sample : N3698-20
Misc : 4.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C07

Quant Time: Jul 16 00:16:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

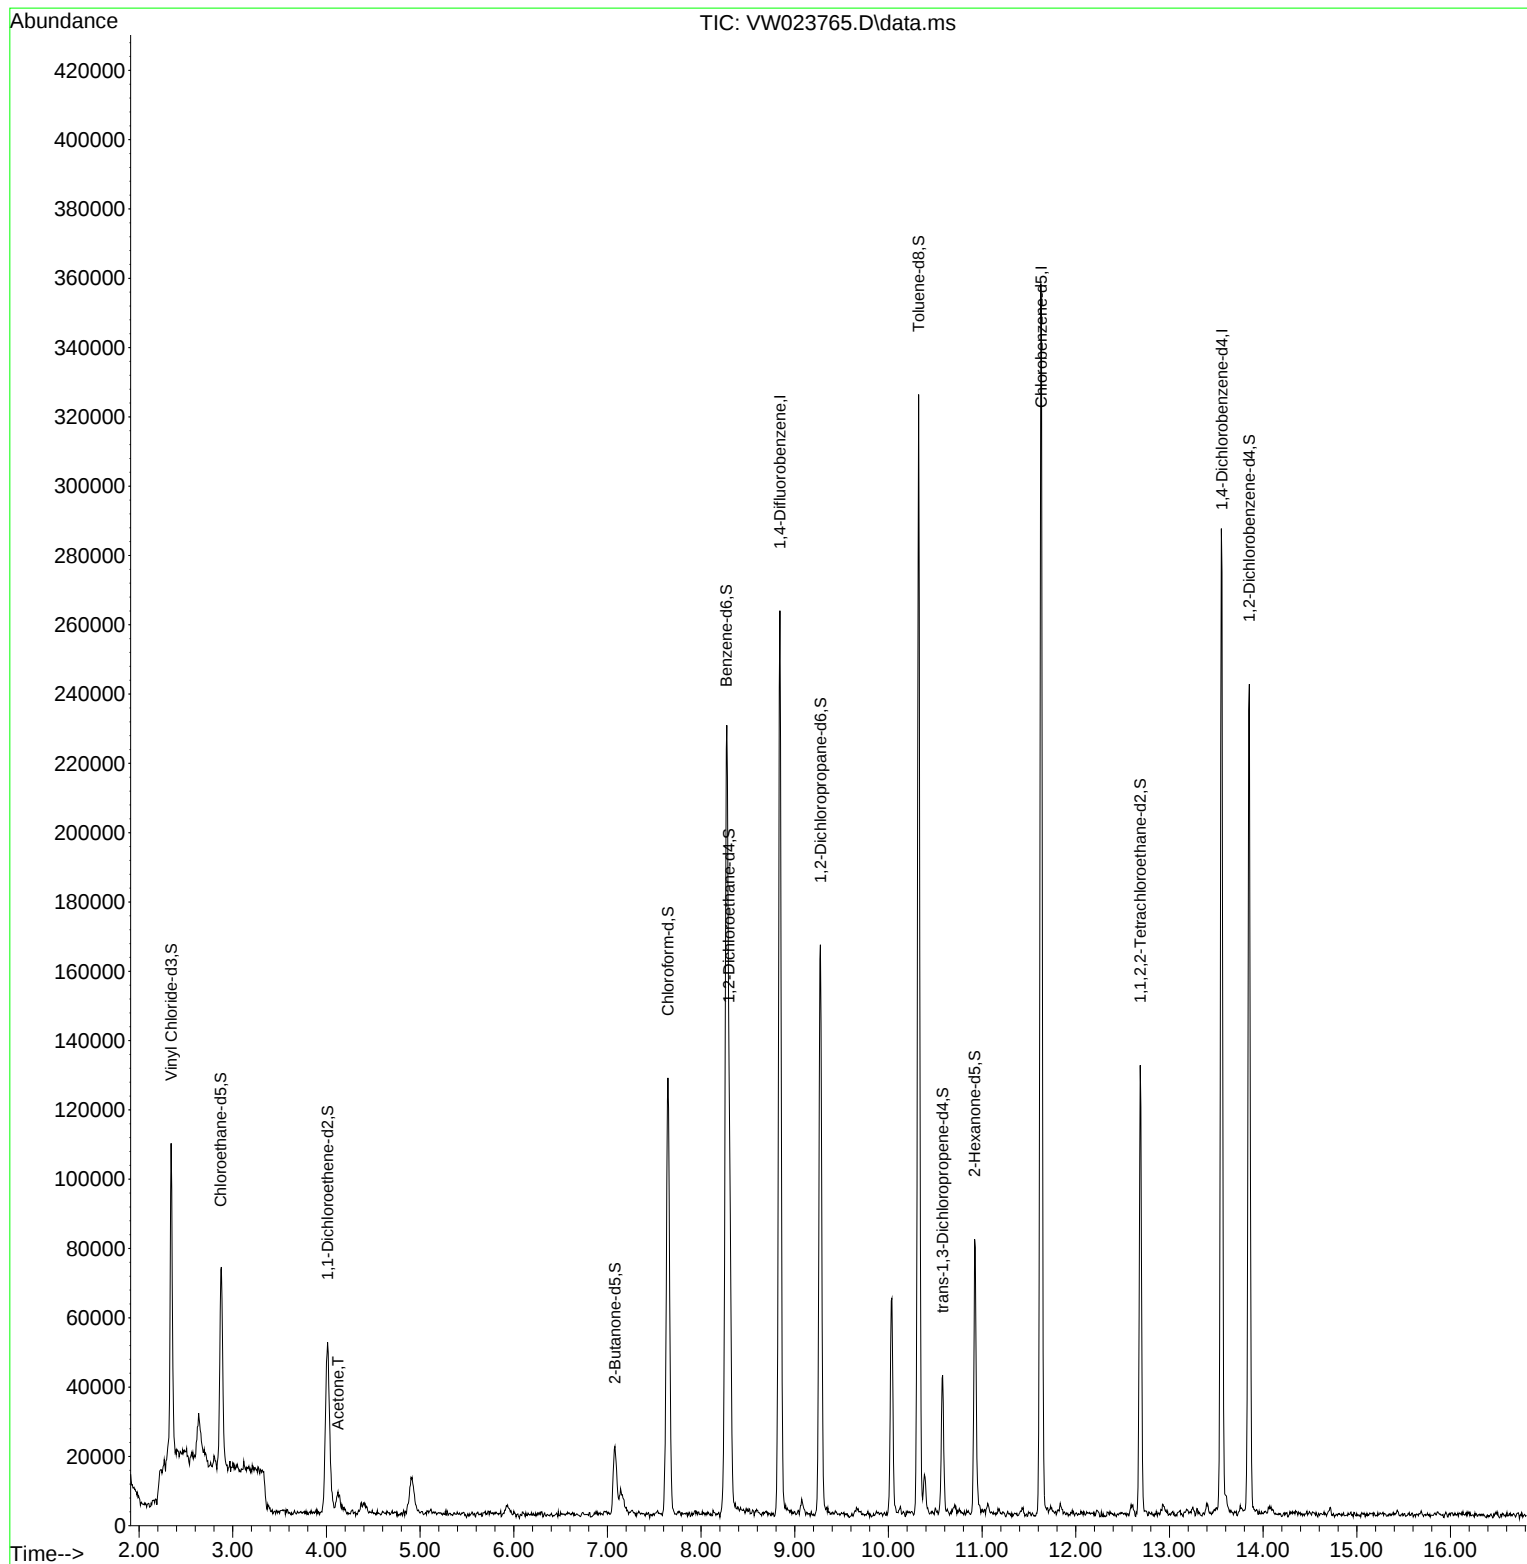

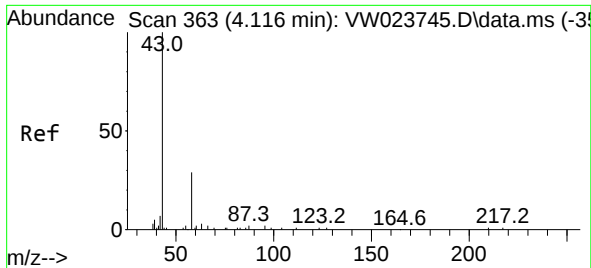

#13
 Acetone
 Concen: 15.922 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW023765.D
 Acq: 15 Jul 2022 23:29

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C07

Tgt Ion: 43 Resp: 8838
 Ion Ratio Lower Upper
 43 100
 58 25.1 0.0 64.2

