

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023766.D
 Acq On : 15 Jul 2022 23:54
 Operator : SY/VA
 Sample : N3700-06RE
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C13RE

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 16 00:32:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 22:15:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	12460	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	13054	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	4404	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	6432	20.211	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.840%		
7) Chloroethane-d5	2.873	69	6480	30.522	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	122.080%		
11) 1,1-Dichloroethene-d2	4.019	63	4409	17.014	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	68.040%		
21) 2-Butanone-d5	7.098	46	4509m	91.345	ug/L	0.02
Spiked Amount 50.000	Range 20 - 135		Recovery =	182.700%#		
24) Chloroform-d	7.647	84	10649	29.355	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	117.400%		
26) 1,2-Dichloroethane-d4	8.305	65	7569m	34.114	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	136.440%#		
32) Benzene-d6	8.275	84	16158	23.811	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	95.240%		
36) 1,2-Dichloropropane-d6	9.274	67	5980	29.256	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	117.040%		
41) Toluene-d8	10.317	98	11349	16.488	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	65.960%		
43) trans-1,3-Dichloroprop...	10.585	79	1932	20.165	ug/L	0.01
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.640%		
47) 2-Hexanone-d5	10.921	63	1970	45.833	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	91.660%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	7149	31.648	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	126.600%#		
66) 1,2-Dichlorobenzene-d4	13.847	152	3920	24.934	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.720%		
Target Compounds						Qvalue
13) Acetone	4.141	43	2001m	57.336	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023766.D
Acq On : 15 Jul 2022 23:54
Operator : SY/VA
Sample : N3700-06RE
Misc : 6.41g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F5C13RE

Quant Time: Jul 16 00:32:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 22:15:34 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

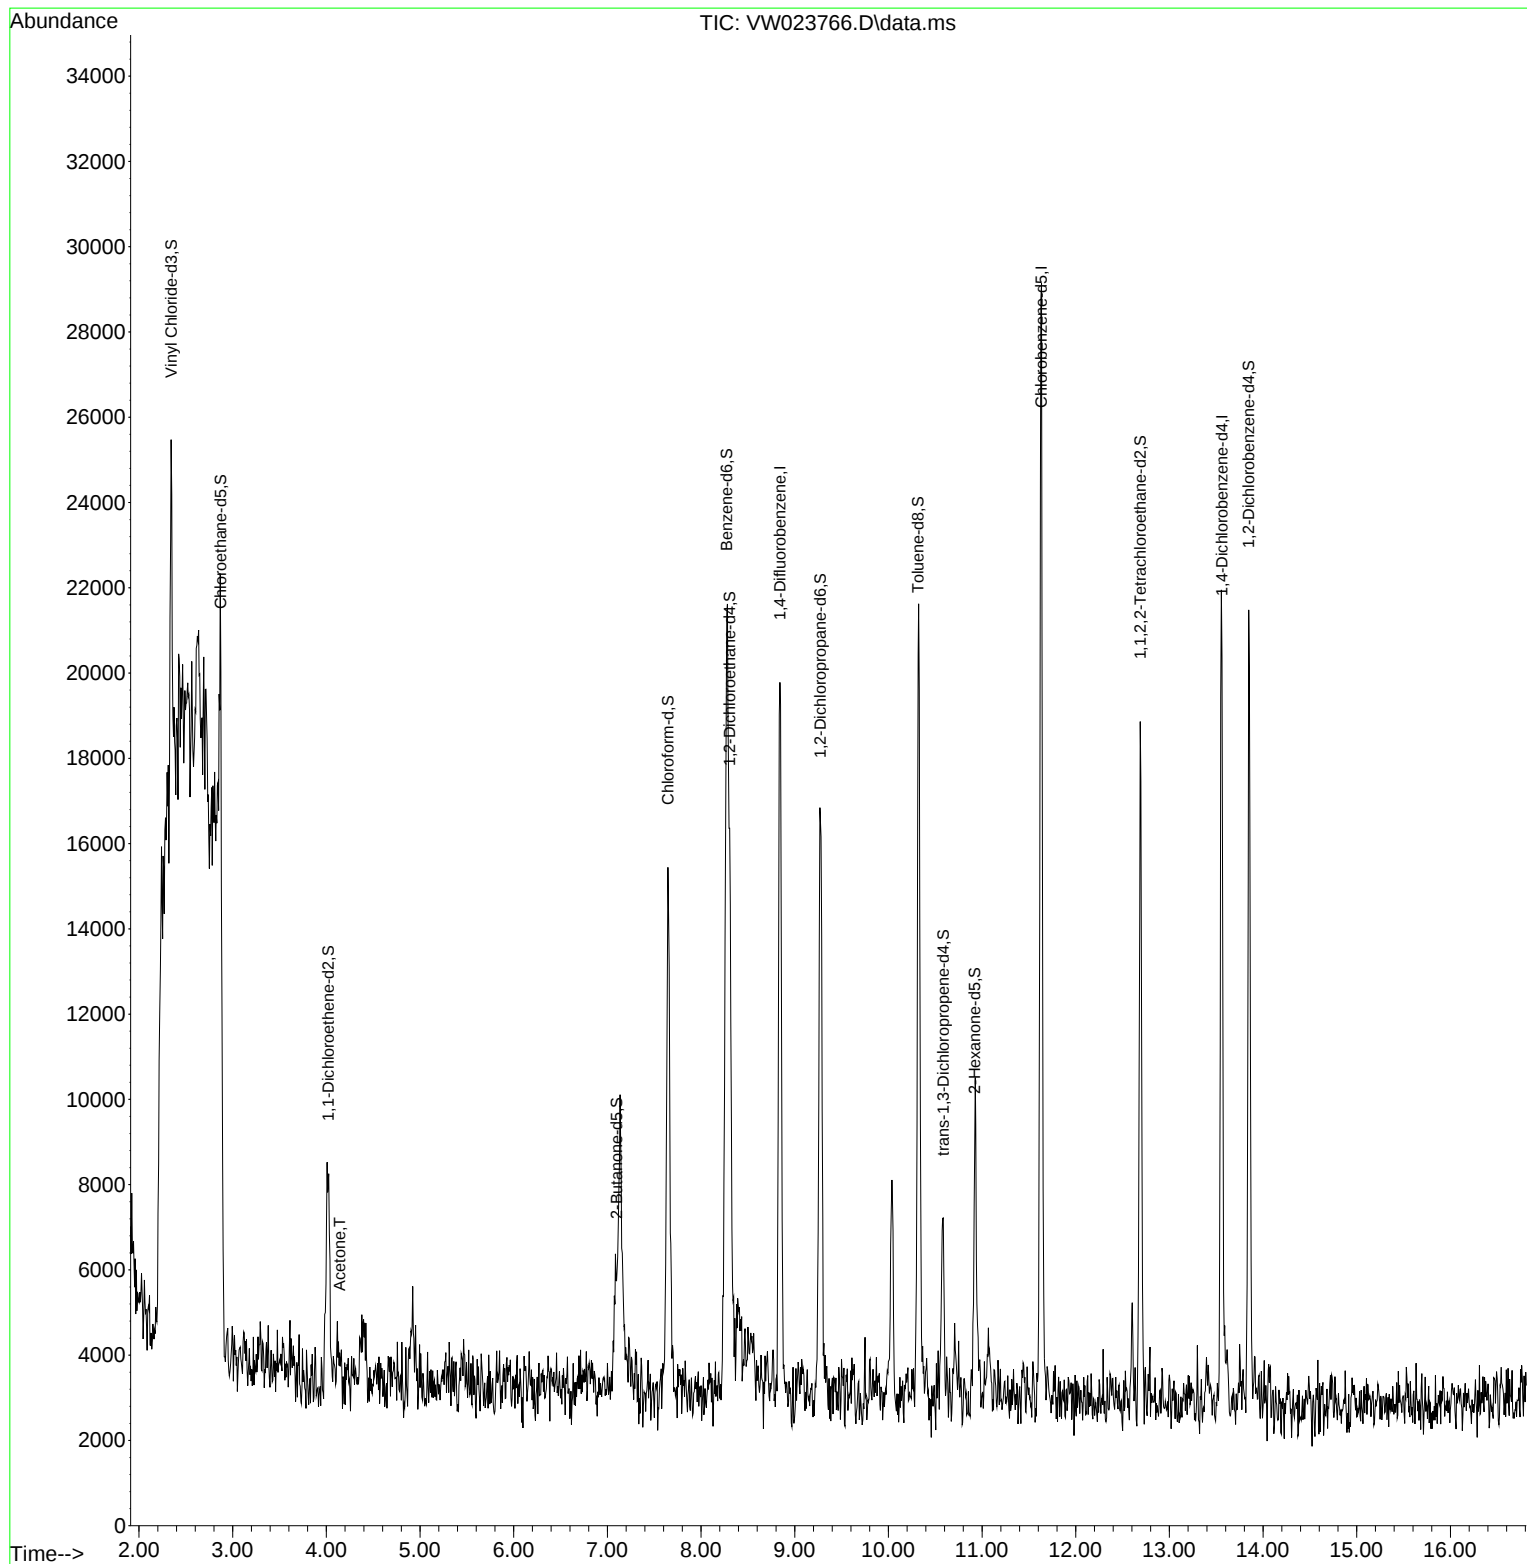

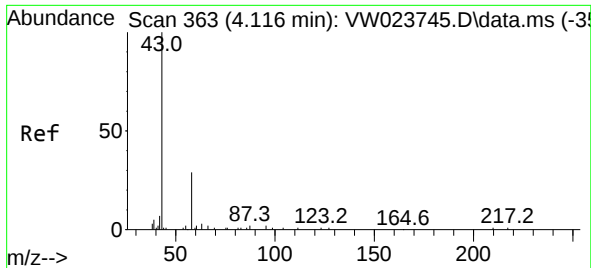

#13
 Acetone
 Concen: 57.336 ug/L m
 RT: 4.141 min Scan# 30
 Delta R.T. 0.025 min
 Lab File: VW023766.D
 Acq: 15 Jul 2022 23:54

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C13RE

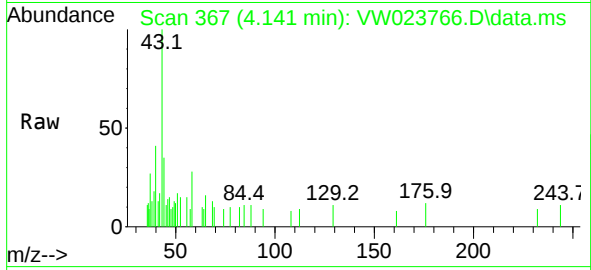

Tgt Ion: 43 Resp: 200
 Ion Ratio Lower Upper
 43 100
 58 26.8 0.0 64.2

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

