

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023792.D
 Acq On : 16 Jul 2022 10:52
 Operator : SY/VA
 Sample : N3702-05
 Misc : 5.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B98

Quant Time: Jul 18 01:51:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 16 01:30:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	209003	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	198879	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	86226	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	81822	15.328	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.320%
7) Chloroethane-d5	2.879	69	67774	19.031	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.120%
11) 1,1-Dichloroethene-d2	4.013	63	44704	10.284	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	41.120%#
21) 2-Butanone-d5	7.074	46	38448	46.435	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.860%
24) Chloroform-d	7.653	84	118710	19.508	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.040%
26) 1,2-Dichloroethane-d4	8.305	65	69372	18.640	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	74.560%
32) Benzene-d6	8.275	84	202915	19.627	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.520%
36) 1,2-Dichloropropane-d6	9.274	67	67308	21.614	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.440%
41) Toluene-d8	10.323	98	193542	18.456	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.840%
43) trans-1,3-Dichloroprop...	10.579	79	26832	18.382	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.520%
47) 2-Hexanone-d5	10.927	63	30636	46.784	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.560%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	69444	20.179	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.720%
66) 1,2-Dichlorobenzene-d4	13.853	152	67355	21.882	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.520%
Target Compounds					Qvalue	
13) Acetone	4.123	43	11265	19.243	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023792.D
Acq On : 16 Jul 2022 10:52
Operator : SY/VA
Sample : N3702-05
Misc : 5.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B98

Quant Time: Jul 18 01:51:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 16 01:30:01 2022
Response via : Initial Calibration

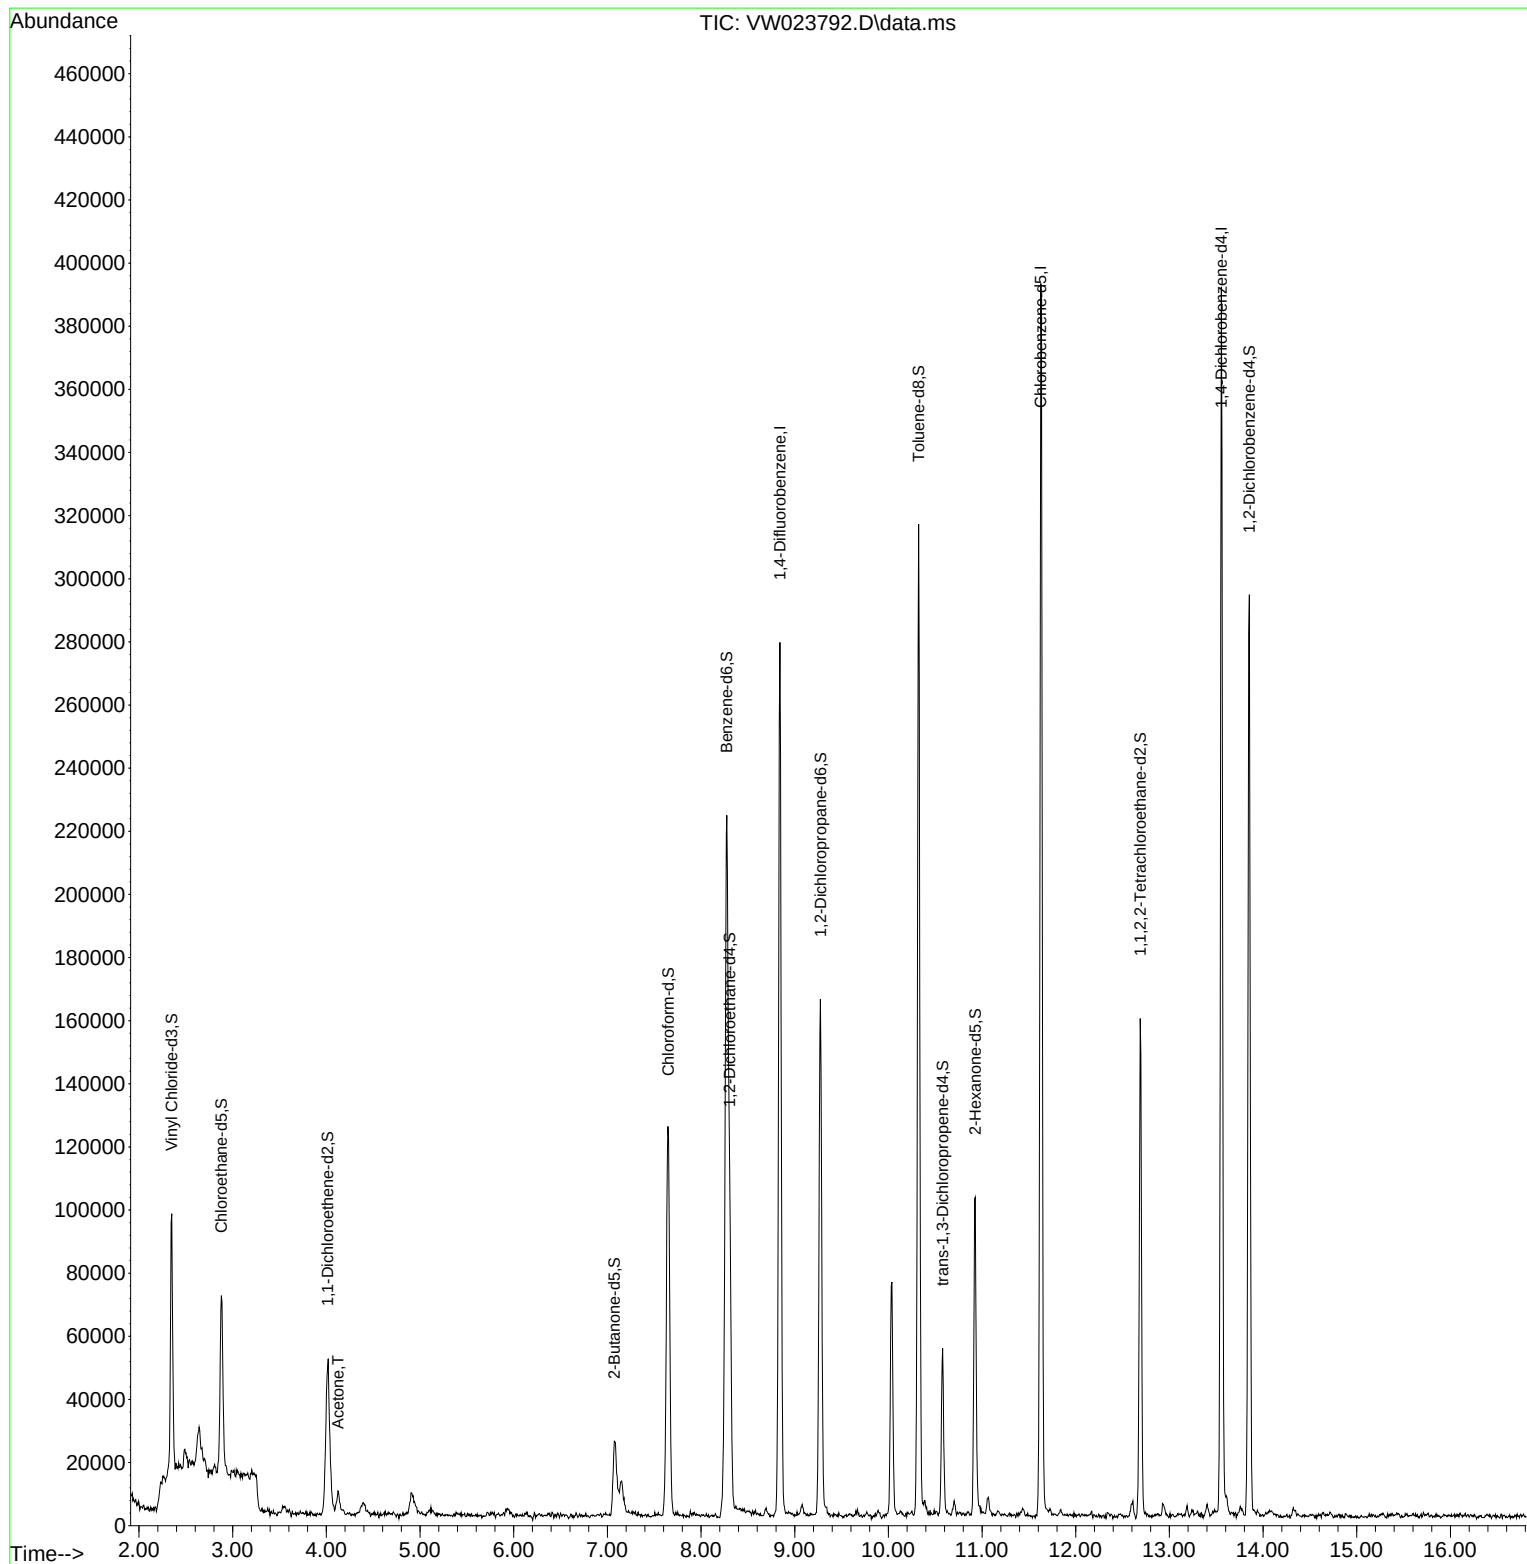

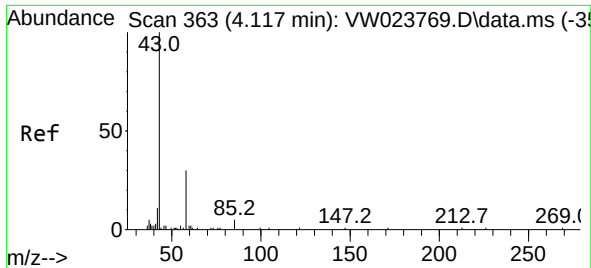

#13

Acetone

Concen: 19.243 ug/L

RT: 4.123 min Scan# 30

Delta R.T. 0.006 min

Lab File: VW023792.D


Acq: 16 Jul 2022 10:52

Instrument :

MSVOA_W

ClientSampleId :

F5B98

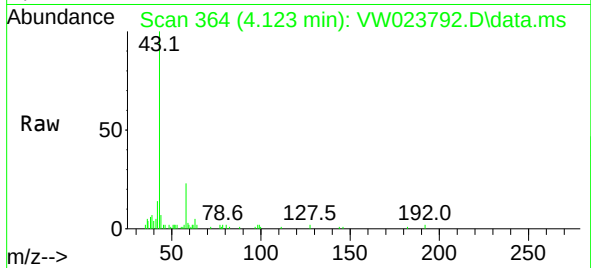

Tgt Ion: 43 Resp: 11265

Ion Ratio Lower Upper

43 100

58 27.2 0.0 64.2

