

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
 Data File : VW023819.D
 Acq On : 17 Jul 2022 05:01
 Operator : SY/VA
 Sample : N3722-01
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C34

Quant Time: Jul 18 03:02:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 18 02:58:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	159562	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	143382	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	50974	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	72264	17.732	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.920%
7) Chloroethane-d5	2.873	69	58172	21.397	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.600%
11) 1,1-Dichloroethene-d2	4.013	63	37533	11.310	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	45.240%
21) 2-Butanone-d5	7.080	46	29936	47.357	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.720%
24) Chloroform-d	7.647	84	94586	20.360	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.440%
26) 1,2-Dichloroethane-d4	8.305	65	54819	19.294	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	77.160%
32) Benzene-d6	8.275	84	158098	21.211	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.840%
36) 1,2-Dichloropropane-d6	9.268	67	54646	24.340	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.360%
41) Toluene-d8	10.323	98	140874	18.634	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.520%
43) trans-1,3-Dichloroprop...	10.573	79	16755	15.921	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	63.680%
47) 2-Hexanone-d5	10.927	63	22845	48.390	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.780%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	51572	20.786	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	41259	22.674	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.680%
Target Compounds					Qvalue	
13) Acetone	4.129	43	8535	19.097	ug/L	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071522\
Data File : VW023819.D
Acq On : 17 Jul 2022 05:01
Operator : SY/VA
Sample : N3722-01
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C34

Quant Time: Jul 18 03:02:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jul 18 02:58:45 2022
Response via : Initial Calibration

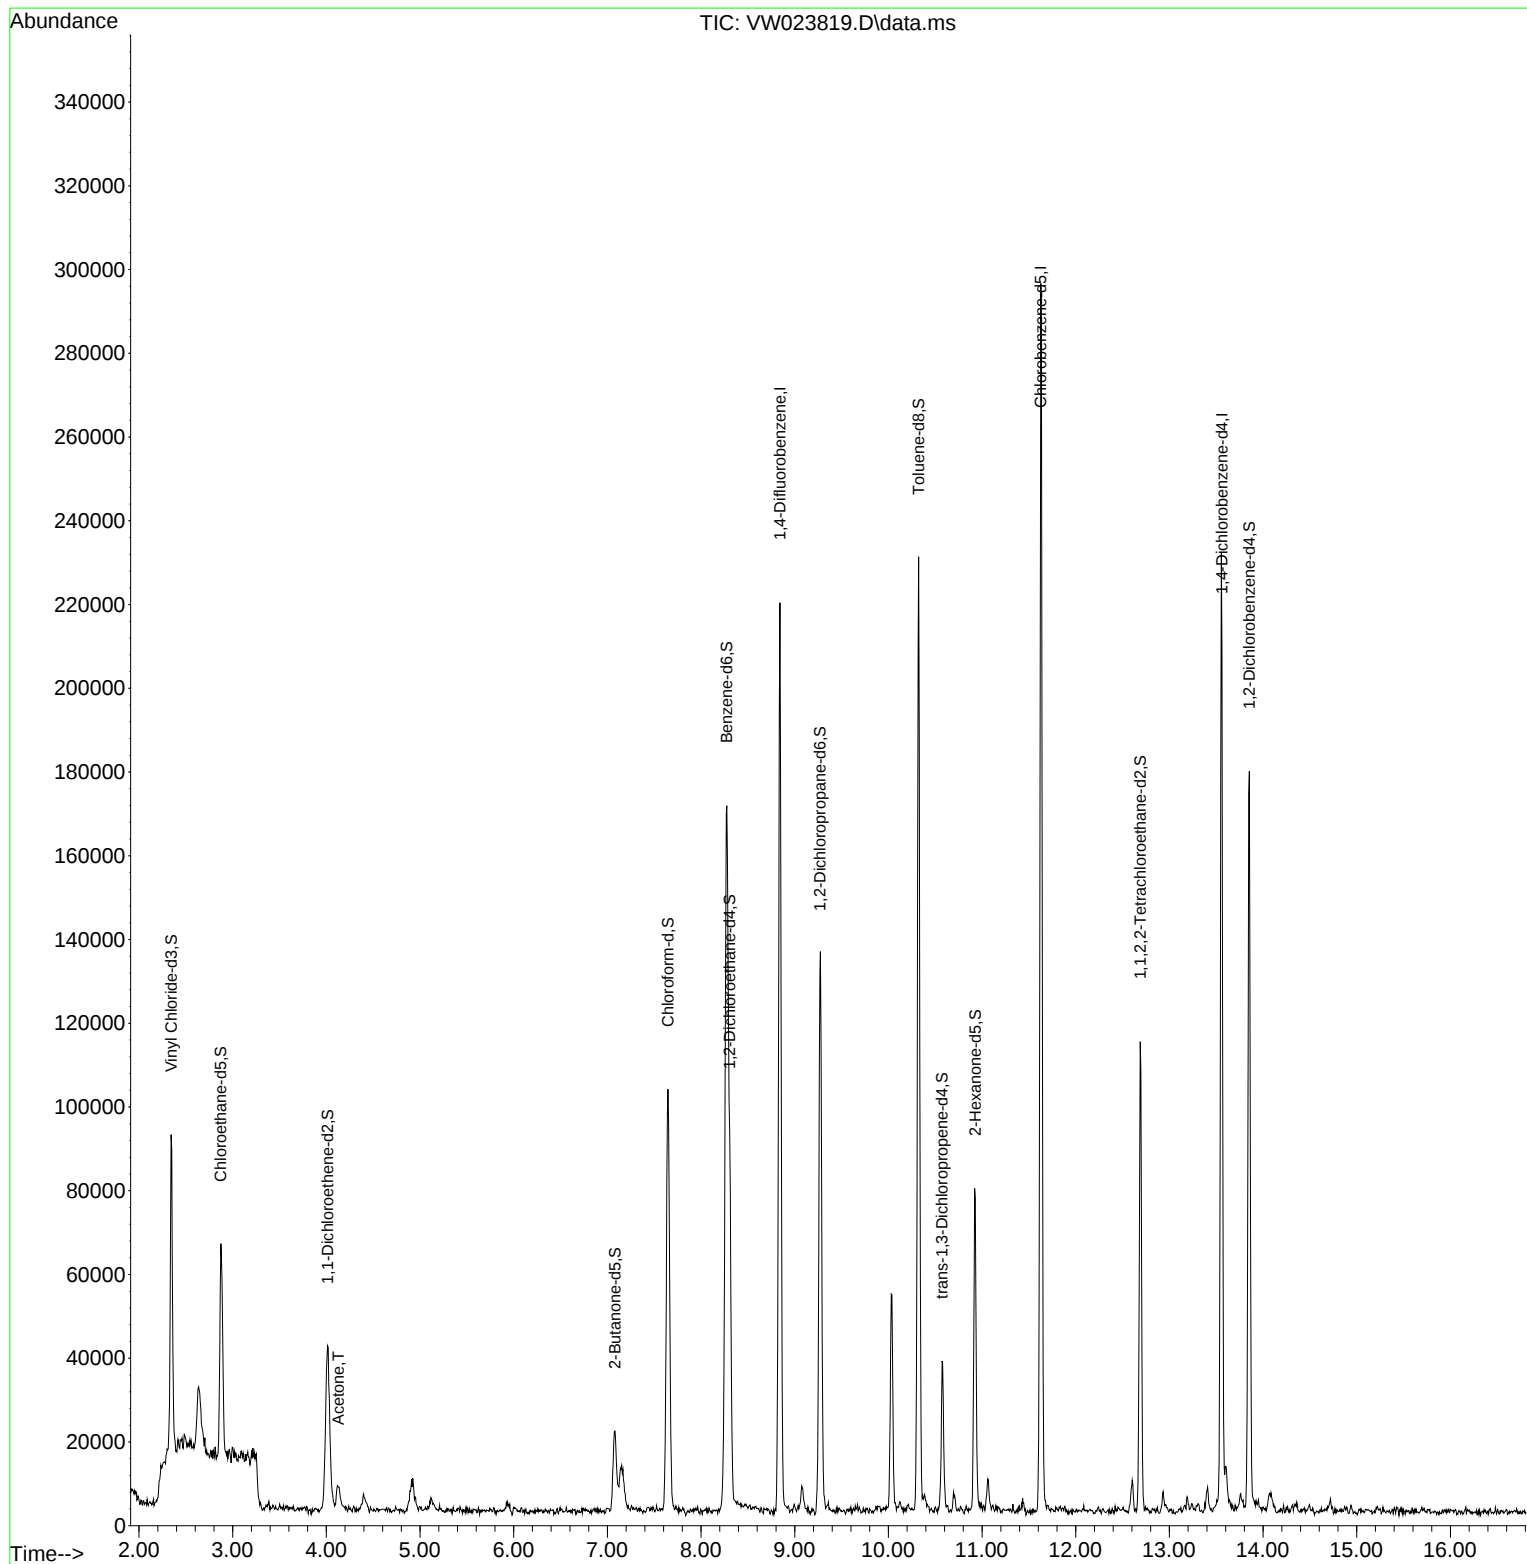

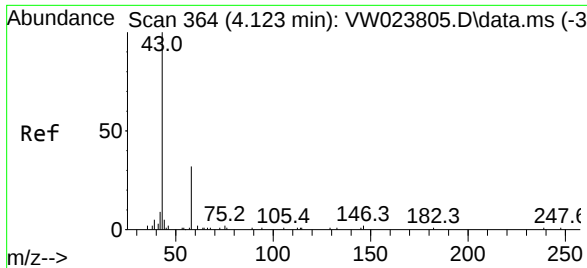

#13
 Acetone
 Concen: 19.097 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW023819.D
 Acq: 17 Jul 2022 05:01

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C34

Tgt Ion: 43 Resp: 8535
 Ion Ratio Lower Upper
 43 100
 58 17.8 0.0 64.2

