


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071620\
 Data File : VW015858.D
 Acq On : 16 Jul 2020 10:44
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070720S.M
 Title : SW846 8260
 Last Update : Wed Jul 08 08:28:05 2020

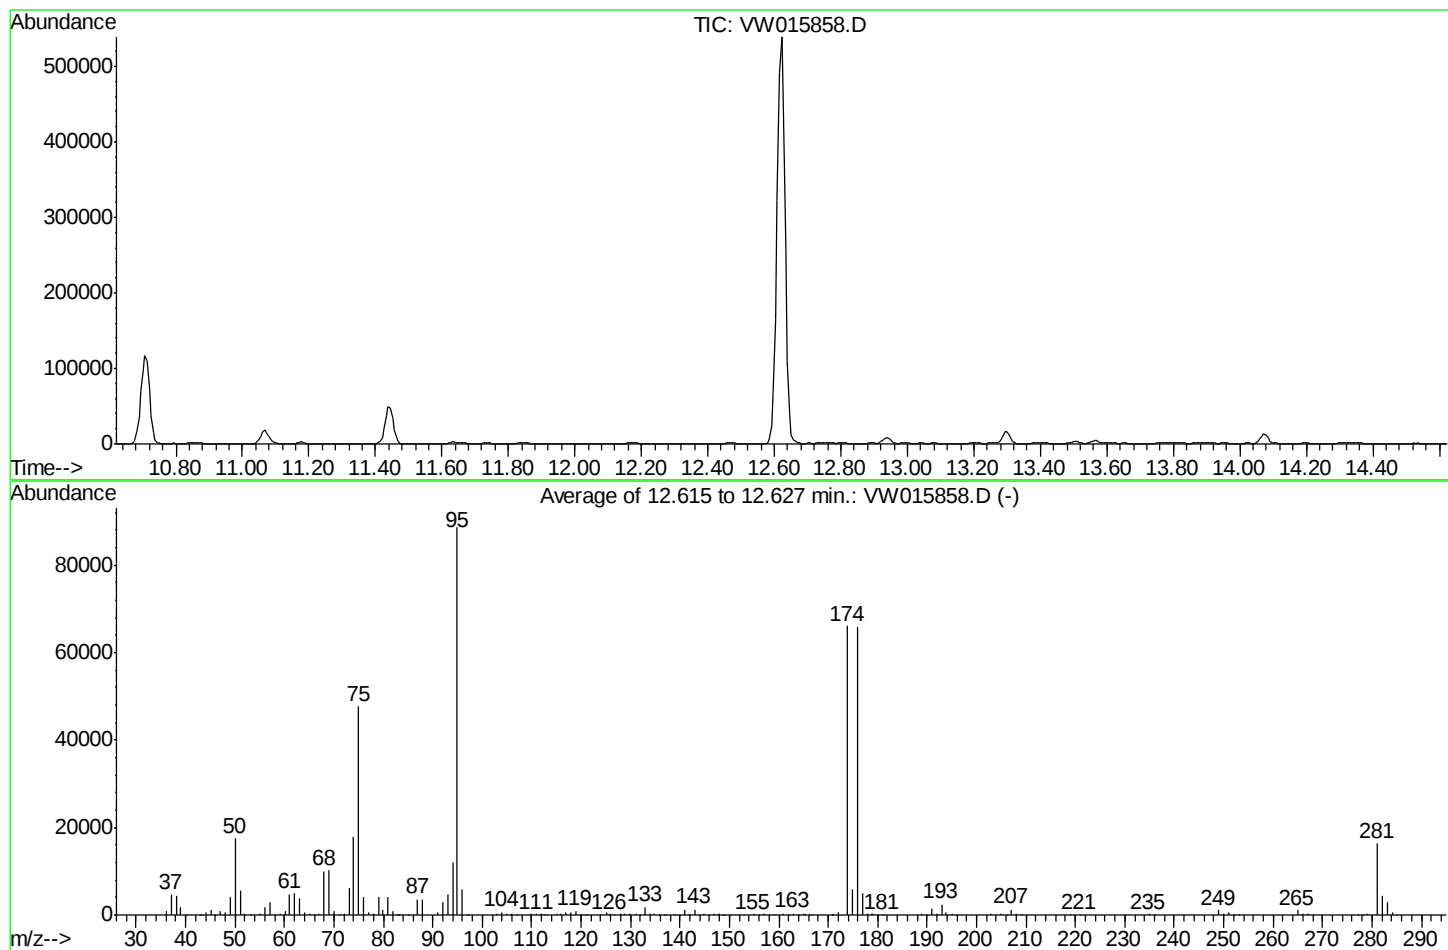

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	17495	PASS
75	95	30	60	53.8	47669	PASS
95	95	100	100	100.0	88637	PASS
96	95	5	9	6.7	5960	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.6	66130	PASS
175	174	5	9	8.7	5727	PASS
176	174	95	101	99.7	65944	PASS
177	176	5	9	7.4	4882	PASS