


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071718\
Data File : VW004000.D
Acq On : 17 Jul 2018 22:41
Operator : VA/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W071618S.M
Title : SW846 8260
Last Update : Mon Jul 16 15:06:12 2018

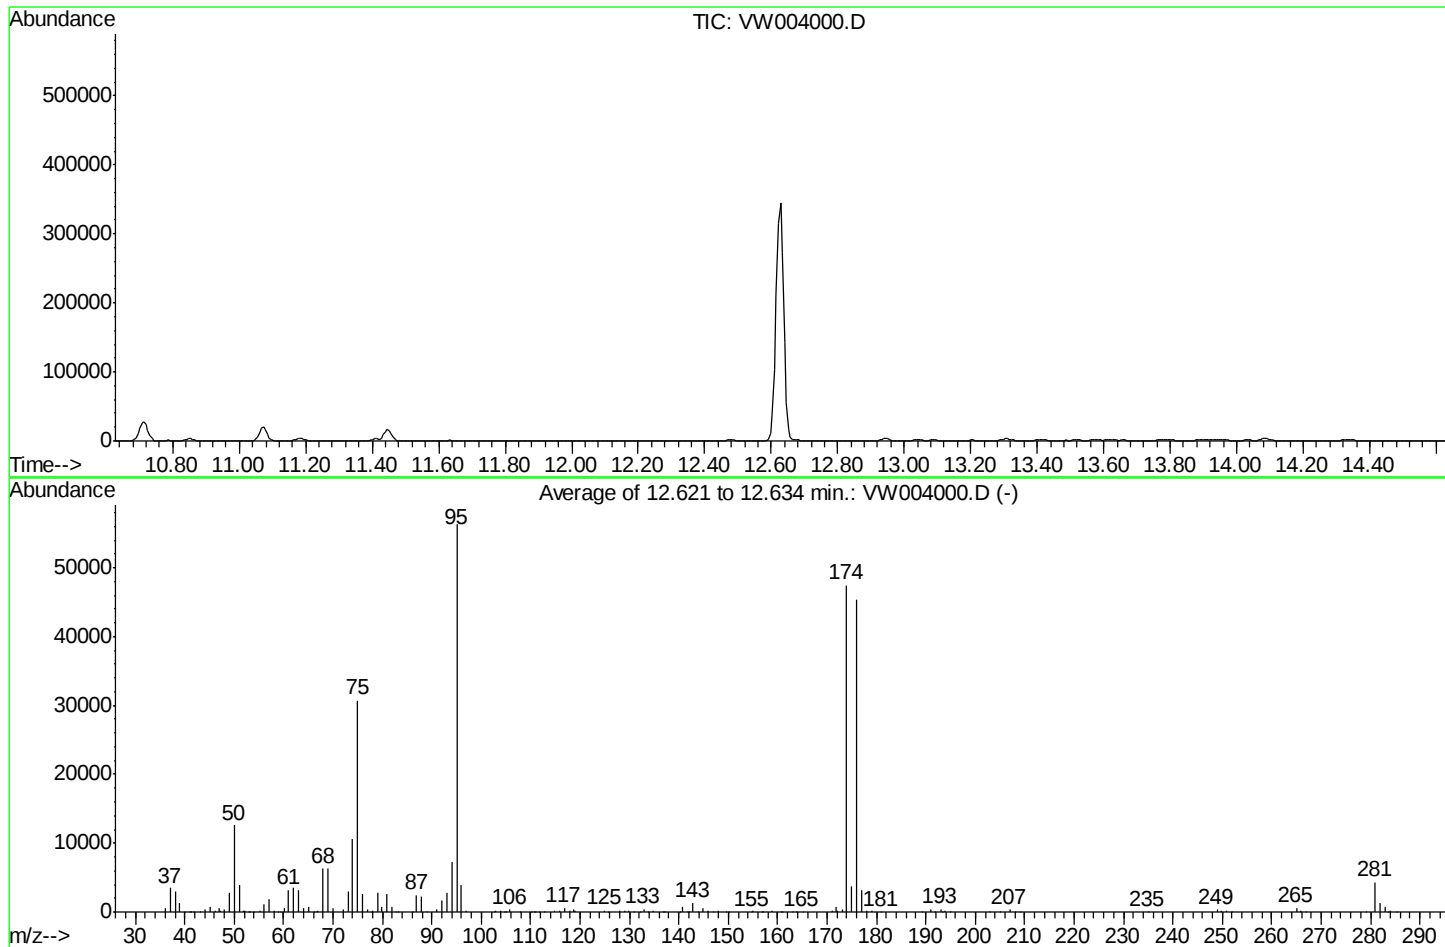

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	12570	PASS
75	95	30	60	54.5	30709	PASS
95	95	100	100	100.0	56328	PASS
96	95	5	9	7.1	3975	PASS
173	174	0.00	2	0.7	347	PASS
174	95	50	100	84.3	47480	PASS
175	174	5	9	7.9	3760	PASS
176	174	95	101	95.5	45333	PASS
177	176	5	9	7.0	3165	PASS