


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071819\
Data File : VW011329.D
Acq On : 18 Jul 2019 08:52
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5.0ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070819S.M
Title : SW846 8260
Last Update : Thu Jul 11 08:14:17 2019

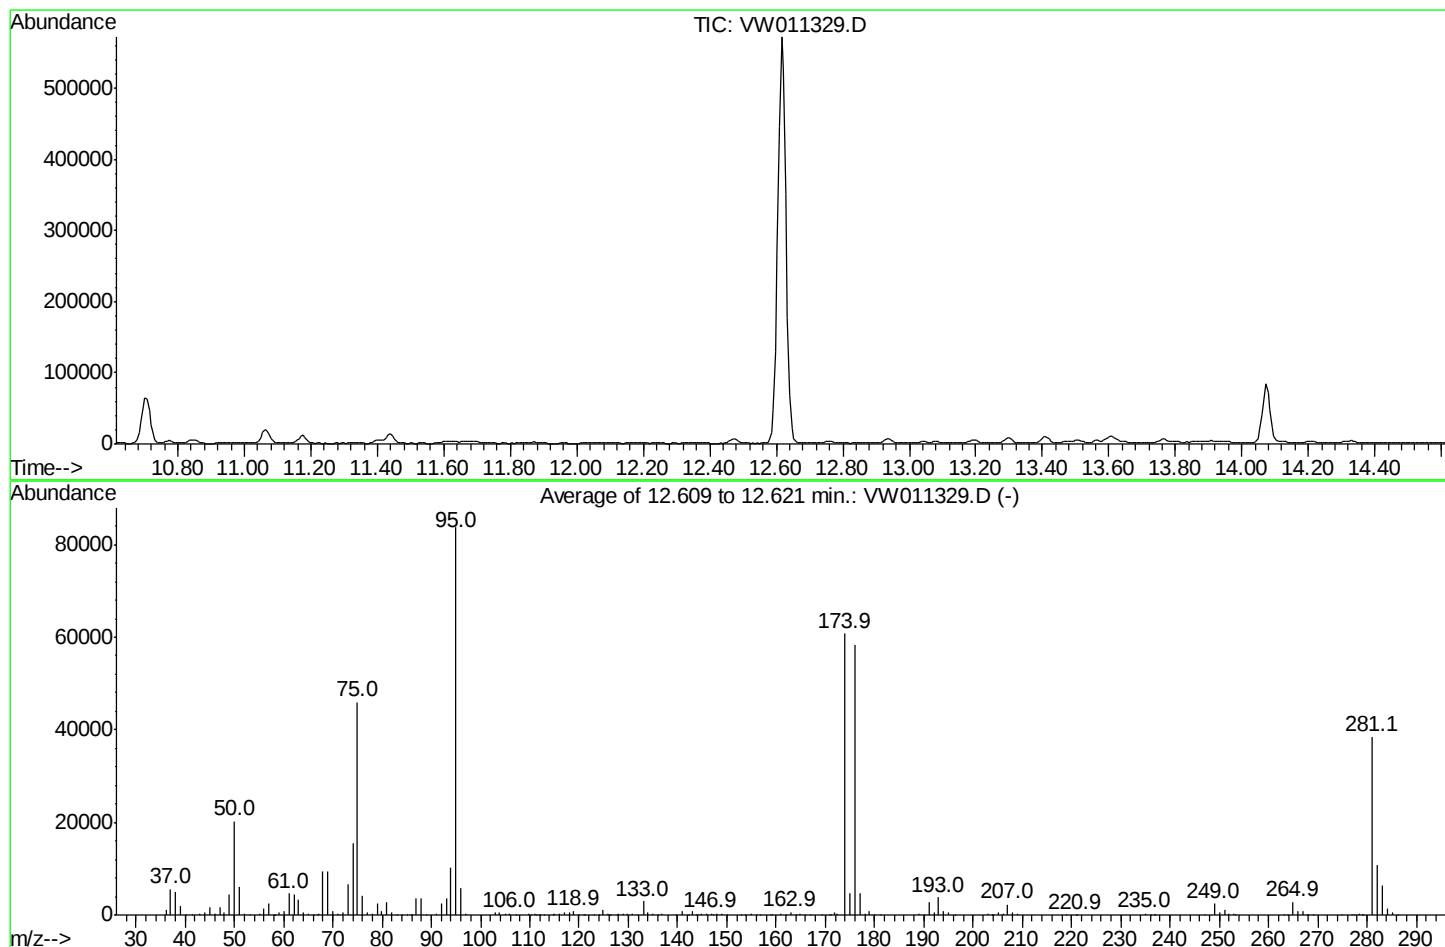

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	20224	PASS
75	95	30	60	54.9	45981	PASS
95	95	100	100	100.0	83733	PASS
96	95	5	9	6.9	5756	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.5	60704	PASS
175	174	5	9	7.9	4819	PASS
176	174	95	101	96.3	58448	PASS
177	176	5	9	8.2	4799	PASS