

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
 Data File : VW023831.D
 Acq On : 18 Jul 2022 10:35
 Operator : SY/VA
 Sample : VW0718SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK552

Quant Time: Jul 19 01:06:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 19 01:05:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.835	114	182329	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	179121	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	81648	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	152223	32.688	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	130.760%
7) Chloroethane-d5	2.873	69	93999	30.257	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	121.040%
11) 1,1-Dichloroethene-d2	4.141	63	183	0.048	ug/L	0.12
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.200%#
21) 2-Butanone-d5	7.000	46	163	0.226	ug/L	-0.07
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.460%#
24) Chloroform-d	7.647	84	115427	21.744	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.960%
26) 1,2-Dichloroethane-d4	8.305	65	69345	21.359	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.440%
32) Benzene-d6	8.268	84	230304	24.734	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.920%
36) 1,2-Dichloropropane-d6	9.268	67	69134	24.649	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.600%
41) Toluene-d8	10.323	98	213690	22.625	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.520%
43) trans-1,3-Dichloroprop...	10.573	79	28939	22.012	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.040%
47) 2-Hexanone-d5	10.920	63	25725	43.618	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.240%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	63180	20.383	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.520%
66) 1,2-Dichlorobenzene-d4	13.853	152	74050	25.406	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.640%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	3059	0.795	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
Data File : VW023831.D
Acq On : 18 Jul 2022 10:35
Operator : SY/VA
Sample : VW0718SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK552

Quant Time: Jul 19 01:06:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 19 01:05:58 2022
Response via : Initial Calibration

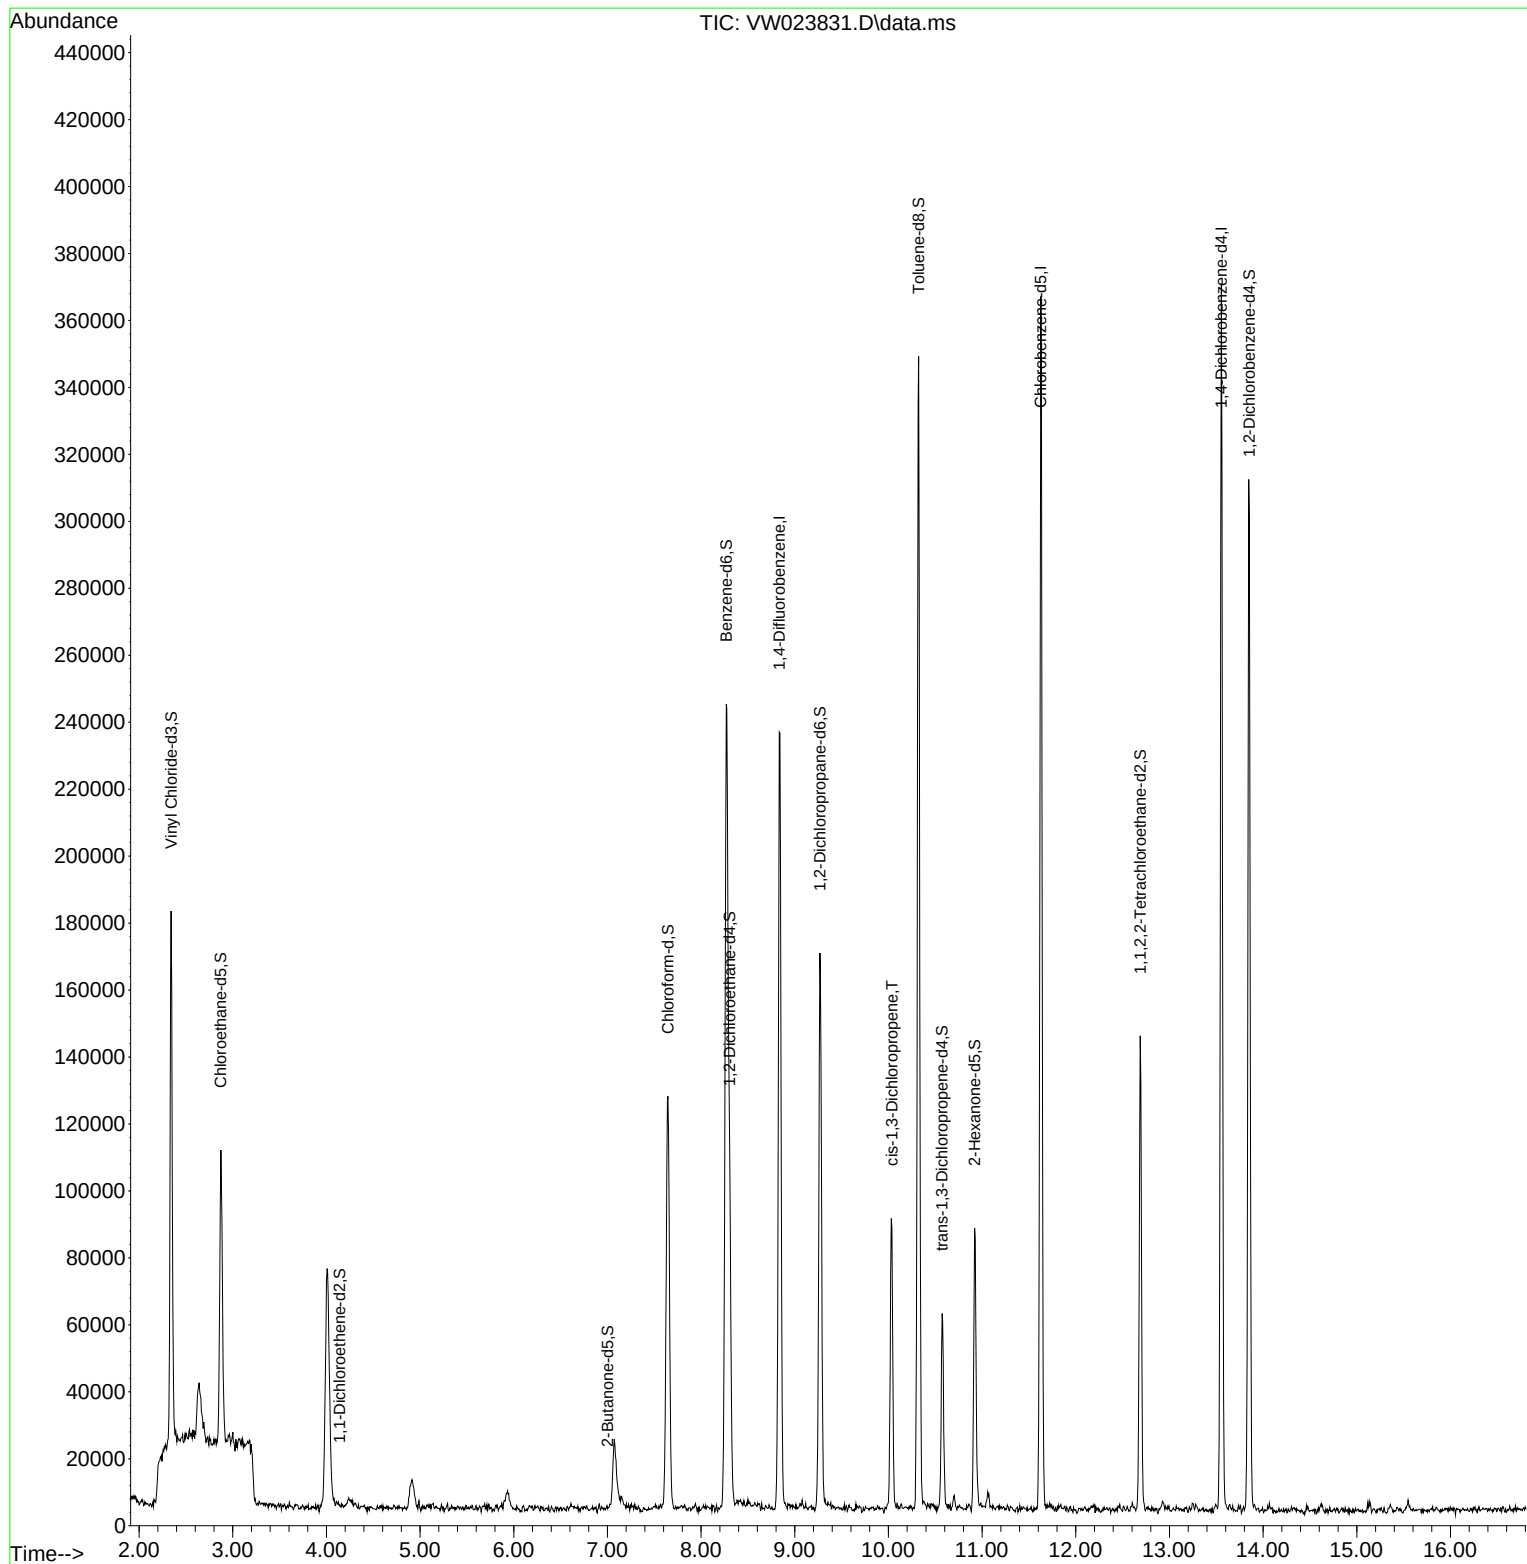

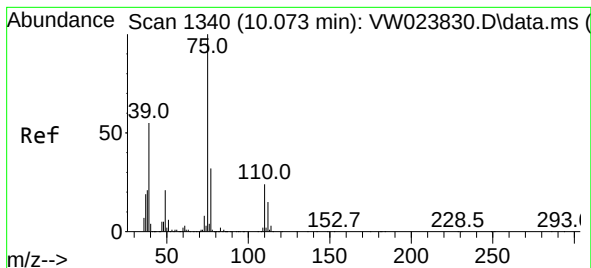

#39
 cis-1,3-Dichloropropene
 Concen: 0.795 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023831.D
 Acq: 18 Jul 2022 10:35

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK552

Tgt Ion: 75 Resp: 3059
 Ion Ratio Lower Upper
 75 100
 77 34.8 22.5 41.9

