

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
 Data File : VW023836.D
 Acq On : 18 Jul 2022 12:50
 Operator : SY/VA
 Sample : N3709-01RE
 Misc : 7.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B11RE

Quant Time: Jul 19 01:07:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 19 01:05:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	119706	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	122629	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	48685	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	55331	18.097	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.400%
7) Chloroethane-d5	2.873	69	39174	19.206	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.840%
11) 1,1-Dichloroethene-d2	4.007	63	31010	12.456	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.840%
21) 2-Butanone-d5	7.086	46	18965	39.991	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.980%
24) Chloroform-d	7.647	84	71401	20.487	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.960%
26) 1,2-Dichloroethane-d4	8.305	65	40106	18.815	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	75.280%
32) Benzene-d6	8.275	84	114168	17.910	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.640%
36) 1,2-Dichloropropane-d6	9.274	67	39191	20.410	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.640%
41) Toluene-d8	10.323	98	103882	16.066	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	64.280%
43) trans-1,3-Dichloroprop...	10.573	79	14814	16.459	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.840%
47) 2-Hexanone-d5	10.927	63	14344	35.525	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.060%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	41104	19.370	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	77.480%
66) 1,2-Dichlorobenzene-d4	13.853	152	37381	21.509	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.040%
Target Compounds						Qvalue
13) Acetone	4.129	43	2352	7.015	ug/L	49
39) cis-1,3-Dichloropropene	10.030	75	1791	0.680	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
Data File : VW023836.D
Acq On : 18 Jul 2022 12:50
Operator : SY/VA
Sample : N3709-01RE
Misc : 7.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
H0B11RE

Quant Time: Jul 19 01:07:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 19 01:05:58 2022
Response via : Initial Calibration




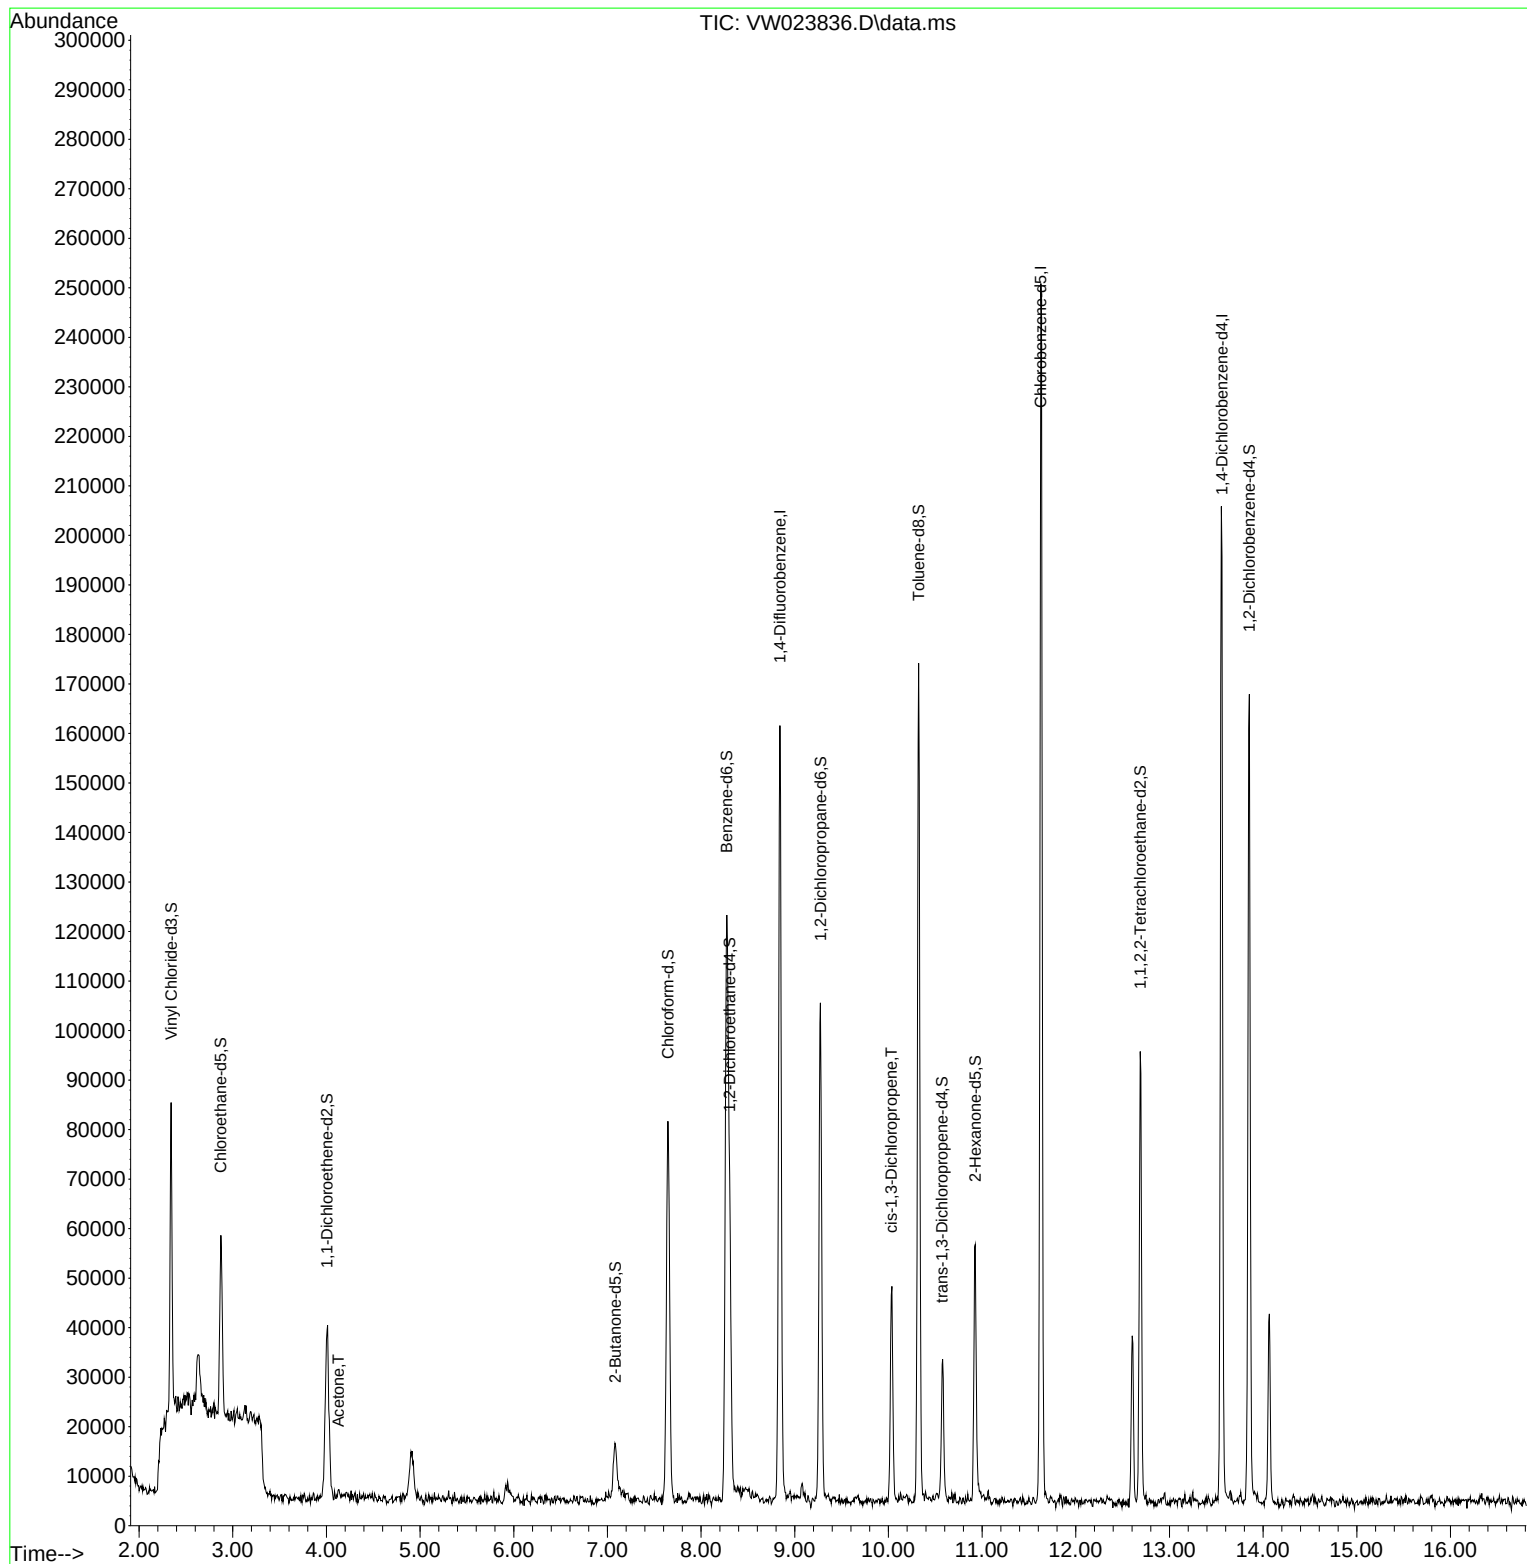


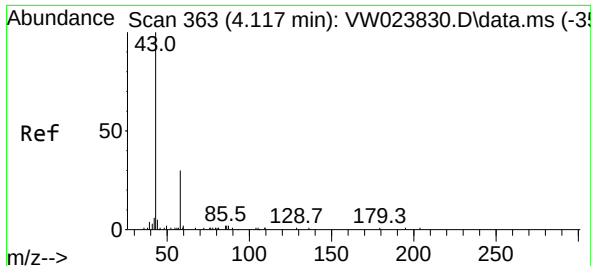

#13
Acetone
Concen: 7.015 ug/L
RT: 4.129 min Scan# 30
Delta R.T. 0.012 min
Lab File: VW023836.D
Acq: 18 Jul 2022 12:50

Instrument :
MSVOA_W
ClientSampleId :
H0B11RE

Tgt Ion: 43 Resp: 2352
Ion Ratio Lower Upper
43 100
58 3.6 0.0 64.2

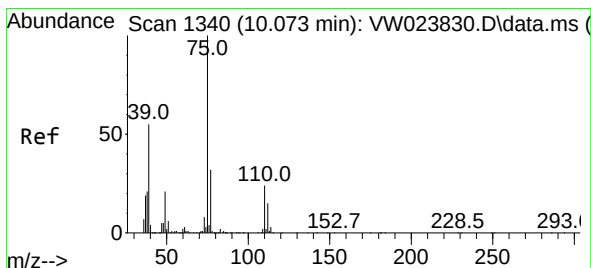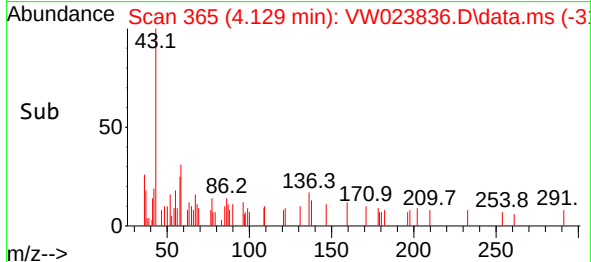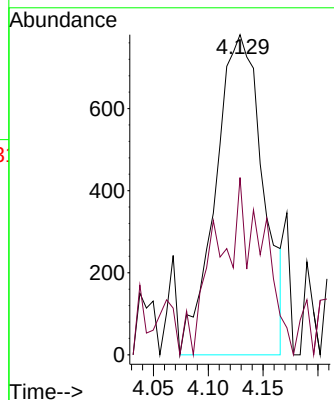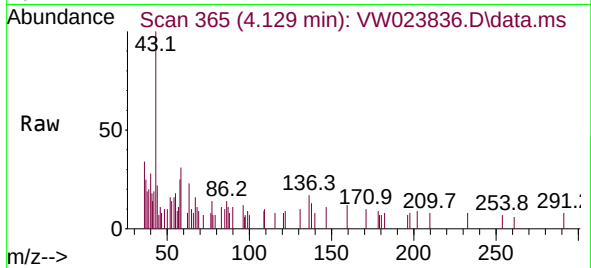

#39
cis-1,3-Dichloropropene
Concen: 0.680 ug/L
RT: 10.030 min Scan# 1333
Delta R.T. -0.043 min
Lab File: VW023836.D
Acq: 18 Jul 2022 12:50

Tgt Ion: 75 Resp: 1791
Ion Ratio Lower Upper
75 100
77 41.6 22.5 41.9

