

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
 Data File : VW023849.D
 Acq On : 18 Jul 2022 18:09
 Operator : SY/VA
 Sample : N3722-01RE
 Misc : 5.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C34

Quant Time: Jul 19 01:10:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 19 01:05:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	222309	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	216052	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93946	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	95884	16.887	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.560%
7) Chloroethane-d5	2.879	69	81301	21.463	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.840%
11) 1,1-Dichloroethene-d2	4.007	63	45987	9.946	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	39.800%#
21) 2-Butanone-d5	7.080	46	38565	43.789	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.580%
24) Chloroform-d	7.647	84	123730	19.116	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	76.480%
26) 1,2-Dichloroethane-d4	8.427	65	91	0.023	ug/L	0.12
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#
32) Benzene-d6	8.275	84	207096	18.440	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.760%
36) 1,2-Dichloropropane-d6	9.274	67	71288	21.072	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.280%
41) Toluene-d8	10.323	98	183576	16.115	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	64.440%
43) trans-1,3-Dichloroprop...	10.579	79	26499	16.711	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.840%
47) 2-Hexanone-d5	10.927	63	30615	43.036	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.080%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	71182	19.040	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	70818	21.117	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.480%
Target Compounds					Qvalue	
13) Acetone	4.135	43	7538	12.106	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
Data File : VW023849.D
Acq On : 18 Jul 2022 18:09
Operator : SY/VA
Sample : N3722-01RE
Misc : 5.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C34

Quant Time: Jul 19 01:10:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 19 01:05:58 2022
Response via : Initial Calibration

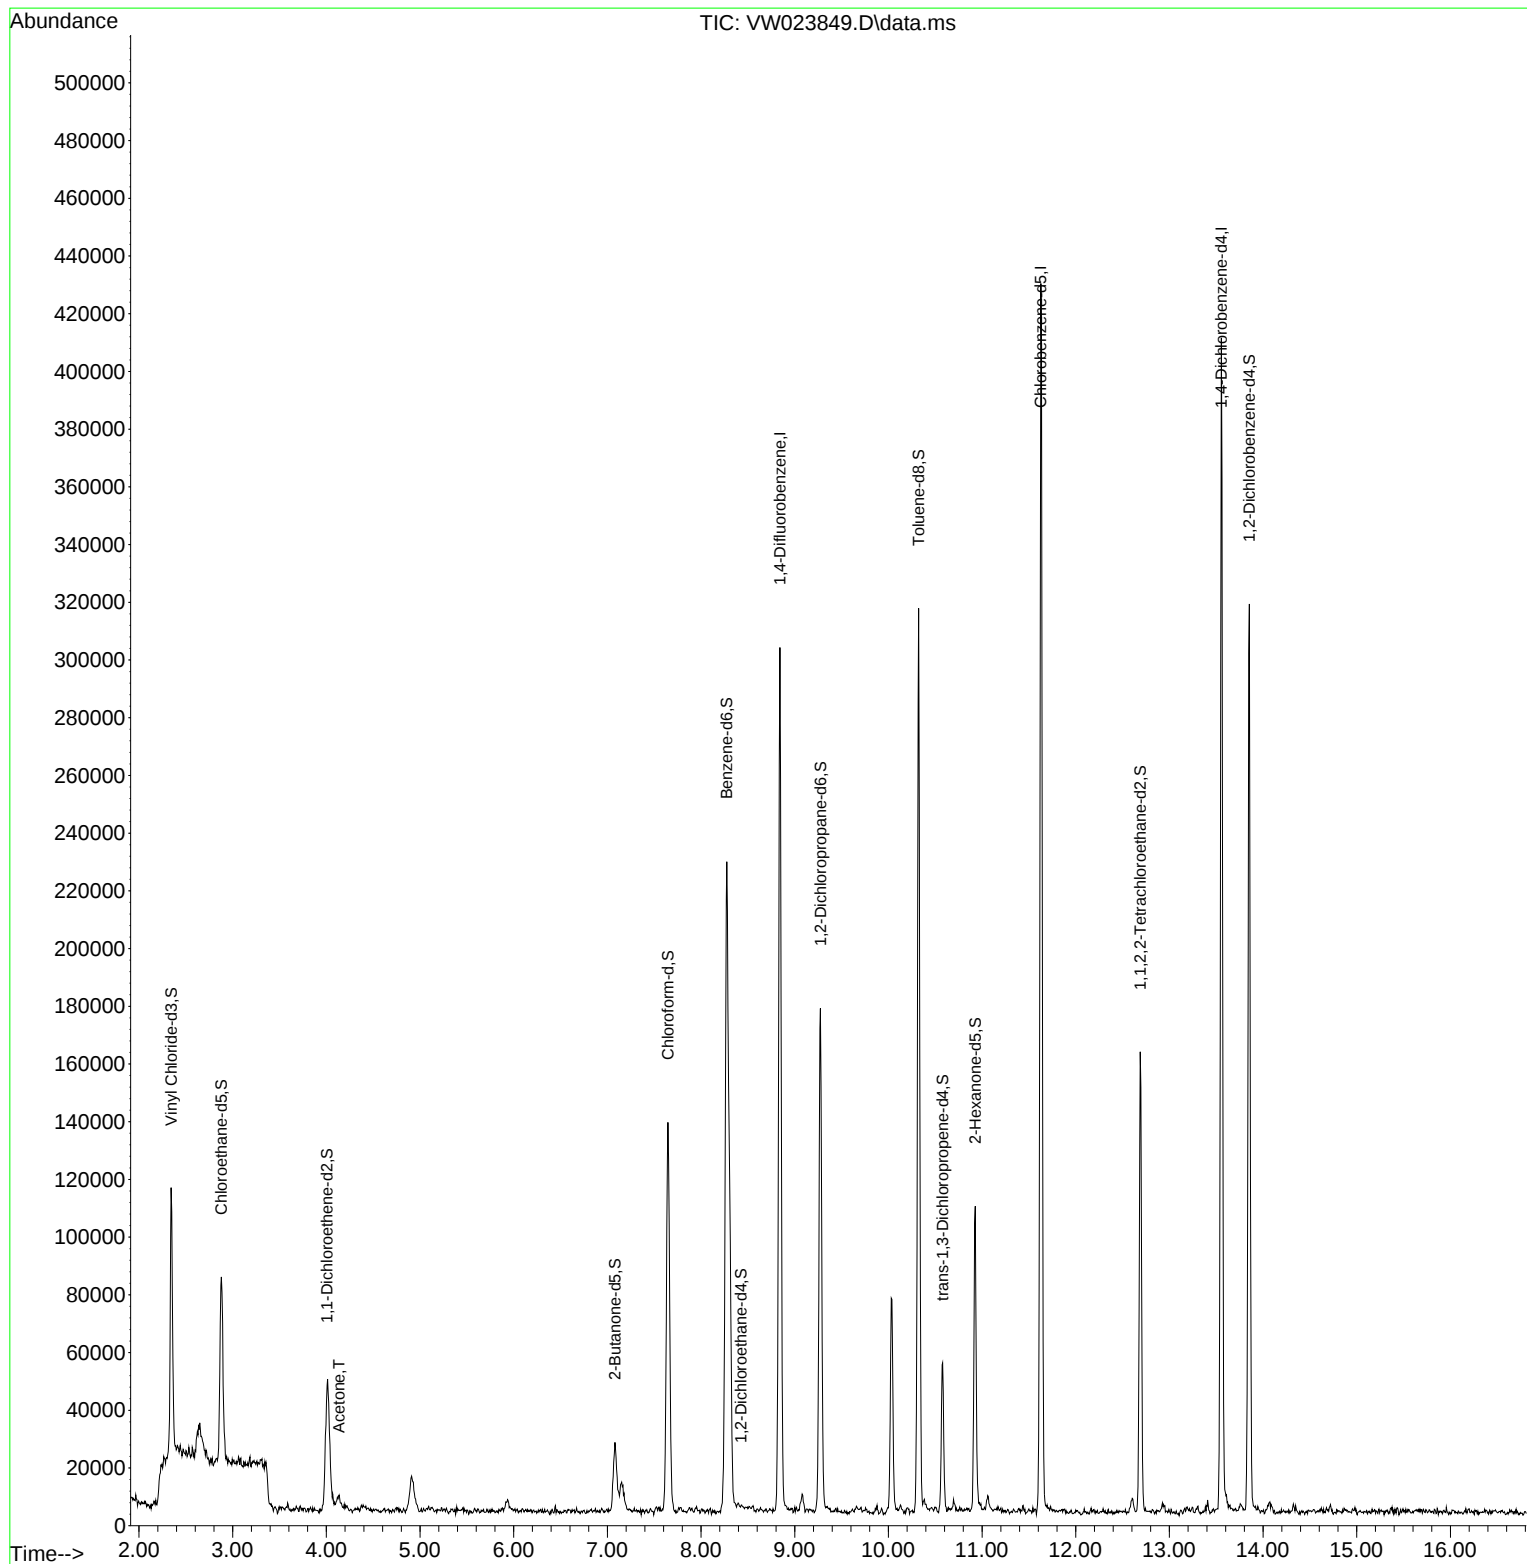

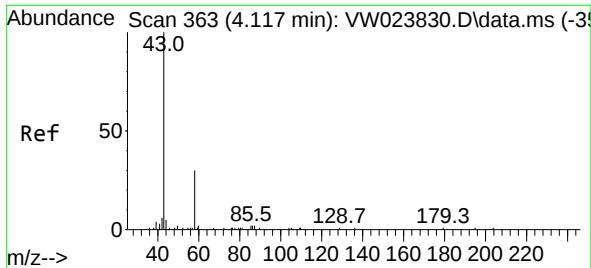

#13
 Acetone
 Concen: 12.106 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.018 min
 Lab File: VW023849.D
 Acq: 18 Jul 2022 18:09

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C34

Tgt Ion: 43 Resp: 7538
 Ion Ratio Lower Upper
 43 100
 58 25.4 0.0 64.2

