




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
 Data File : VW023847.D
 Acq On : 18 Jul 2022 17:20
 Operator : SY/VA
 Sample : N3721-16
 Misc : 6.11g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C58

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:09:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 19 01:05:58 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/19/2022
 Supervised By :Mahesh Dadoda 07/20/2022

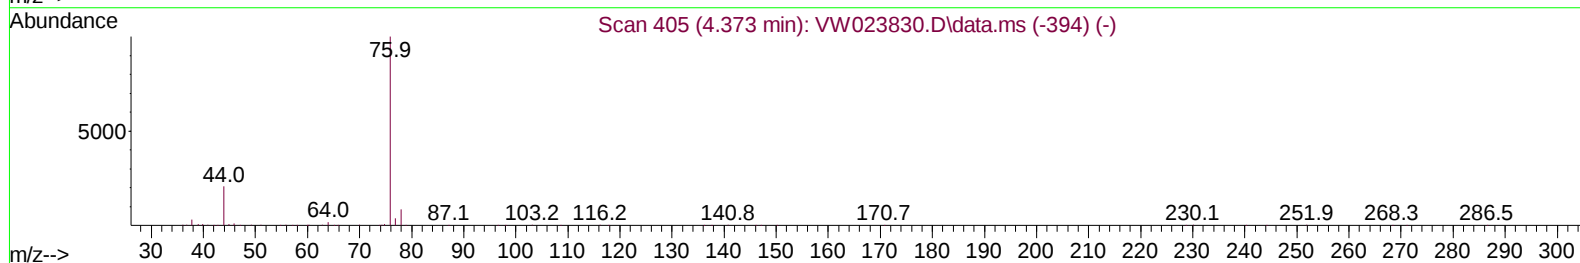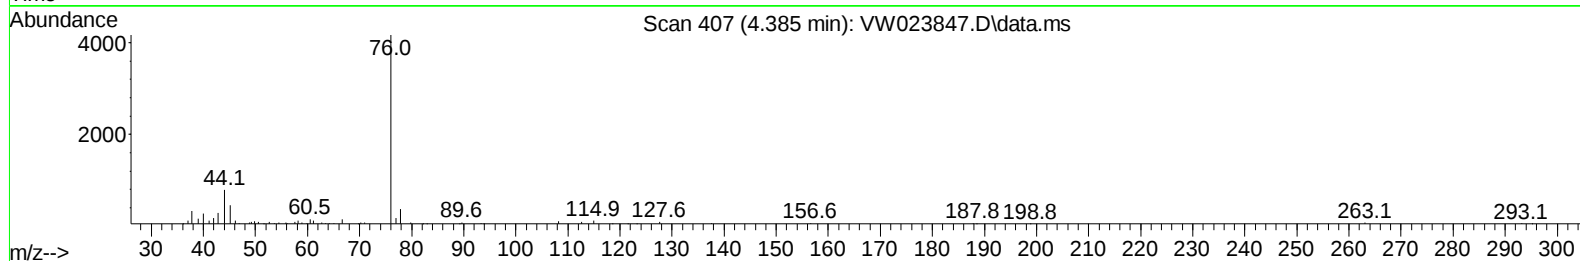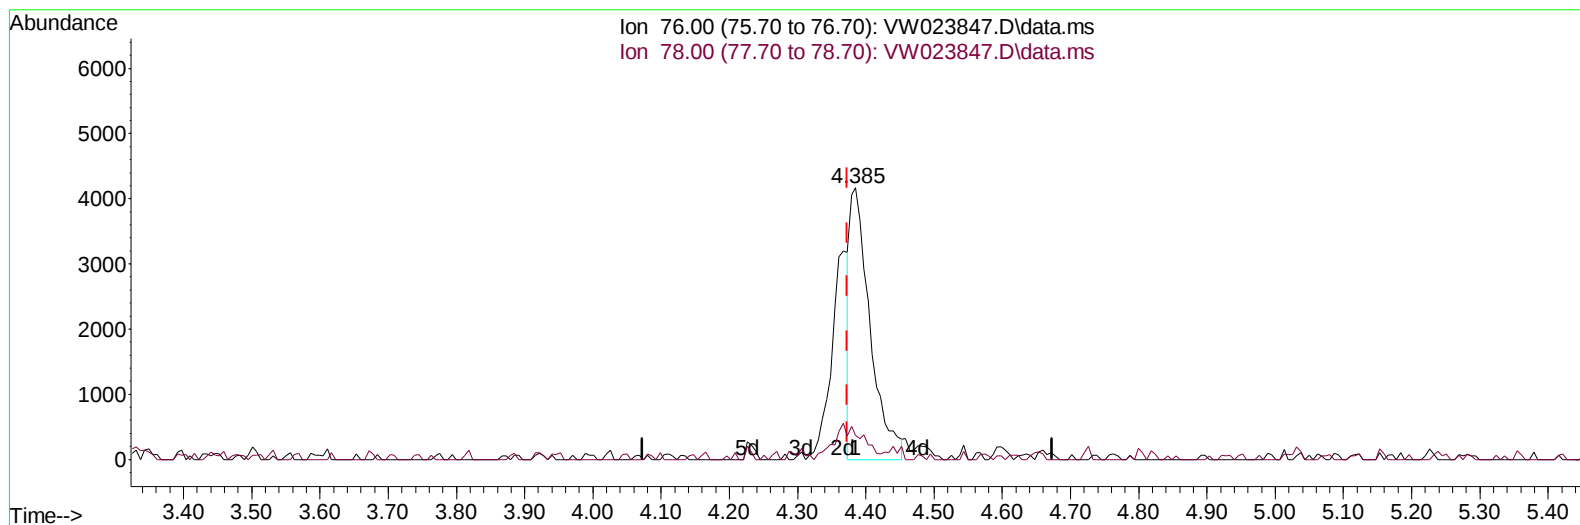

TIC: VW023847.D\data.ms

(14) Carbon disulfide (T)

4.385min (+ 0.012) 1.28 ug/L

response 8421

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.00	8.81
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
 Data File : VW023847.D
 Acq On : 18 Jul 2022 17:20
 Operator : SY/VA
 Sample : N3721-16
 Misc : 6.11g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C58

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:09:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 19 01:05:58 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/19/2022
 Supervised By :Mahesh Dadoda 07/20/2022

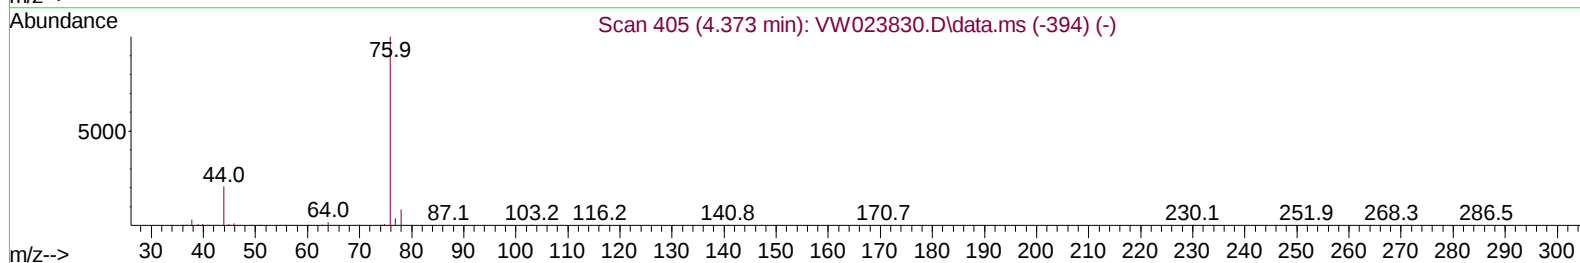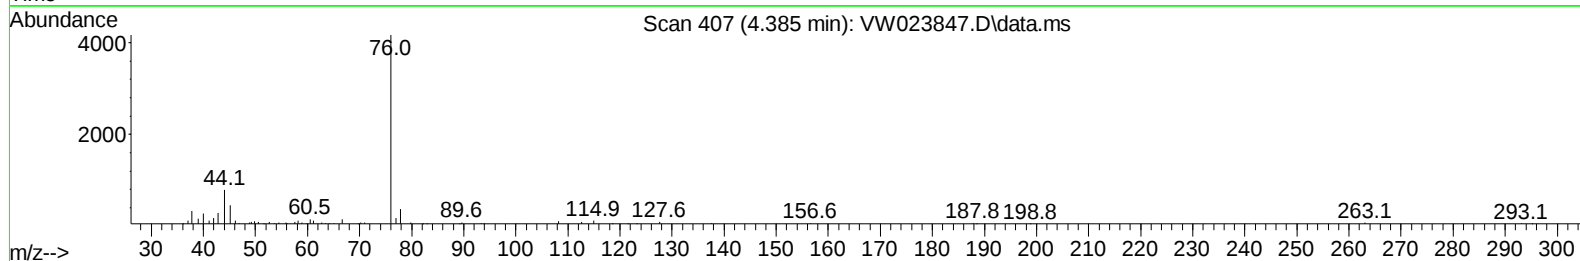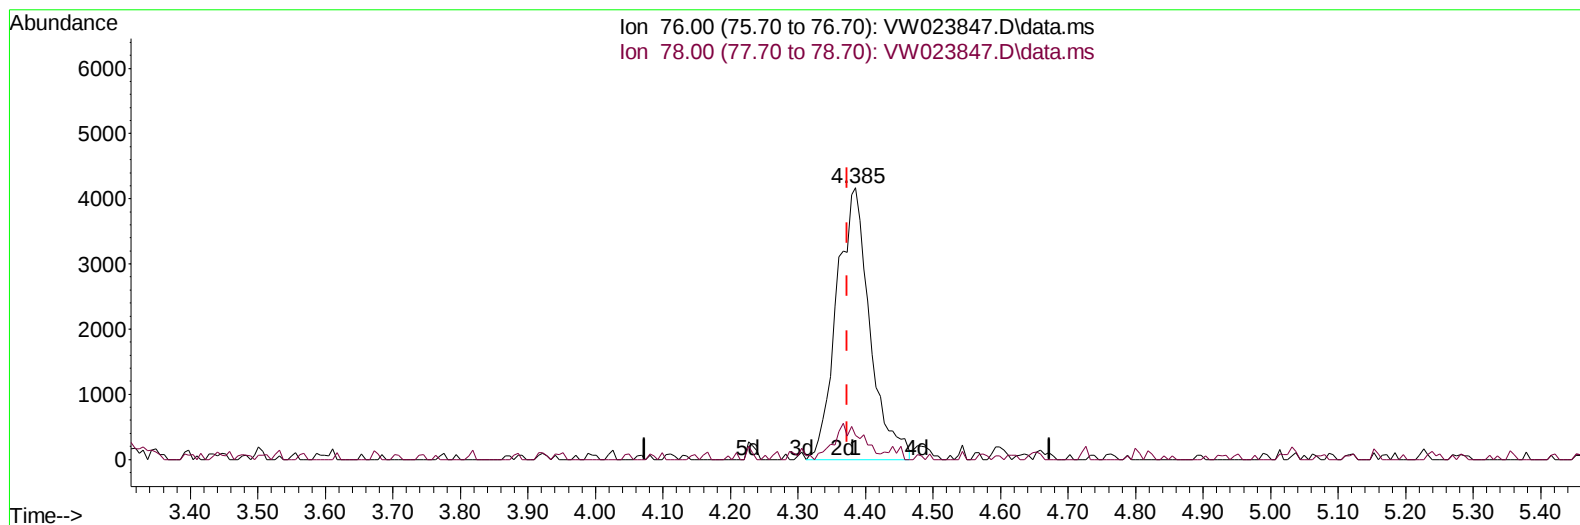

TIC: VW023847.D\data.ms

(14) Carbon disulfide (T)

4.385min (+ 0.012) 2.15 ug/L m

response 14120

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	9.00	8.81
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
 Data File : VW023847.D
 Acq On : 18 Jul 2022 17:20
 Operator : SY/VA
 Sample : N3721-16
 Misc : 6.11g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C58

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:09:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 19 01:05:58 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/19/2022
 Supervised By :Mahesh Dadoda 07/20/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	210717	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	196457	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	81390	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	100201	18.618	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.480%	
7) Chloroethane-d5	2.879	69	87692	24.424	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	97.680%	
11) 1,1-Dichloroethene-d2	4.007	63	49548	11.306	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	45.240%	
21) 2-Butanone-d5	7.080	46	37329	44.717	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.440%	
24) Chloroform-d	7.647	84	125766	20.500	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.000%	
26) 1,2-Dichloroethane-d4	8.305	65	70811	18.872	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	75.480%	
32) Benzene-d6	8.275	84	209194	20.484	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	81.920%	
36) 1,2-Dichloropropane-d6	9.275	67	71031	23.091	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	92.360%	
41) Toluene-d8	10.323	98	194358	18.763	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.040%	
43) trans-1,3-Dichloroprop...	10.579	79	25531	17.706	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	70.840%	
47) 2-Hexanone-d5	10.921	63	28842	44.588	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.180%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	68558	20.167	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	80.680%	
66) 1,2-Dichlorobenzene-d4	13.847	152	67813	23.340	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	93.360%	
Target Compounds						
13) Acetone	4.123	43	14894	25.235	ug/L	Qvalue 92
14) Carbon disulfide	4.385	76	14120m	2.149	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
Data File : VW023847.D
Acq On : 18 Jul 2022 17:20
Operator : SY/VA
Sample : N3721-16
Misc : 6.11g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C58

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/19/2022
Supervised By :Mahesh Dadoda 07/20/2022

Quant Time: Jul 19 01:09:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 19 01:05:58 2022
Response via : Initial Calibration

