




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
 Data File : VW023865.D
 Acq On : 19 Jul 2022 03:40
 Operator : SY/VA
 Sample : N3722-11
 Misc : 6.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C46

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/19/2022
 Supervised By :Mahesh Dadoda 07/20/2022

Quant Time: Jul 19 05:40:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 19 02:51:35 2022
 Response via : Initial Calibration

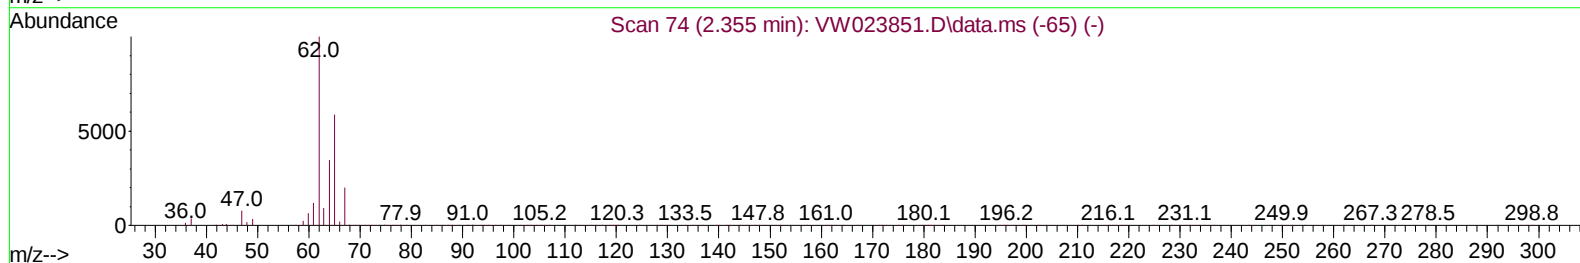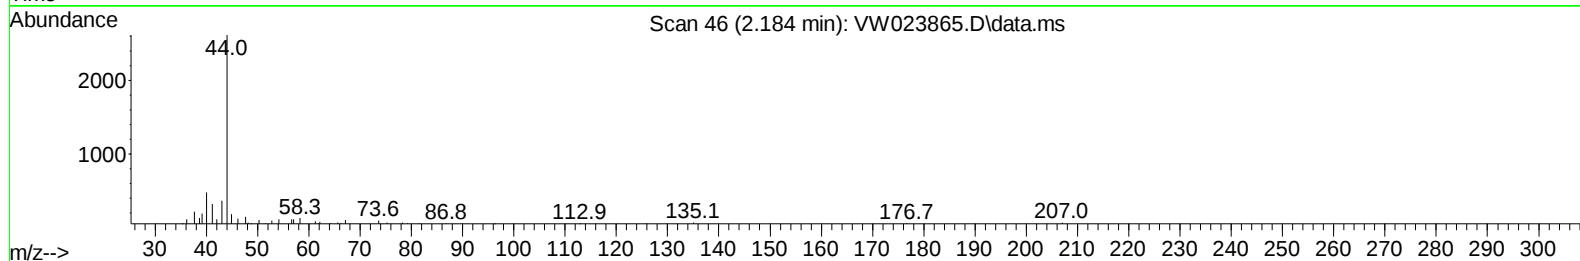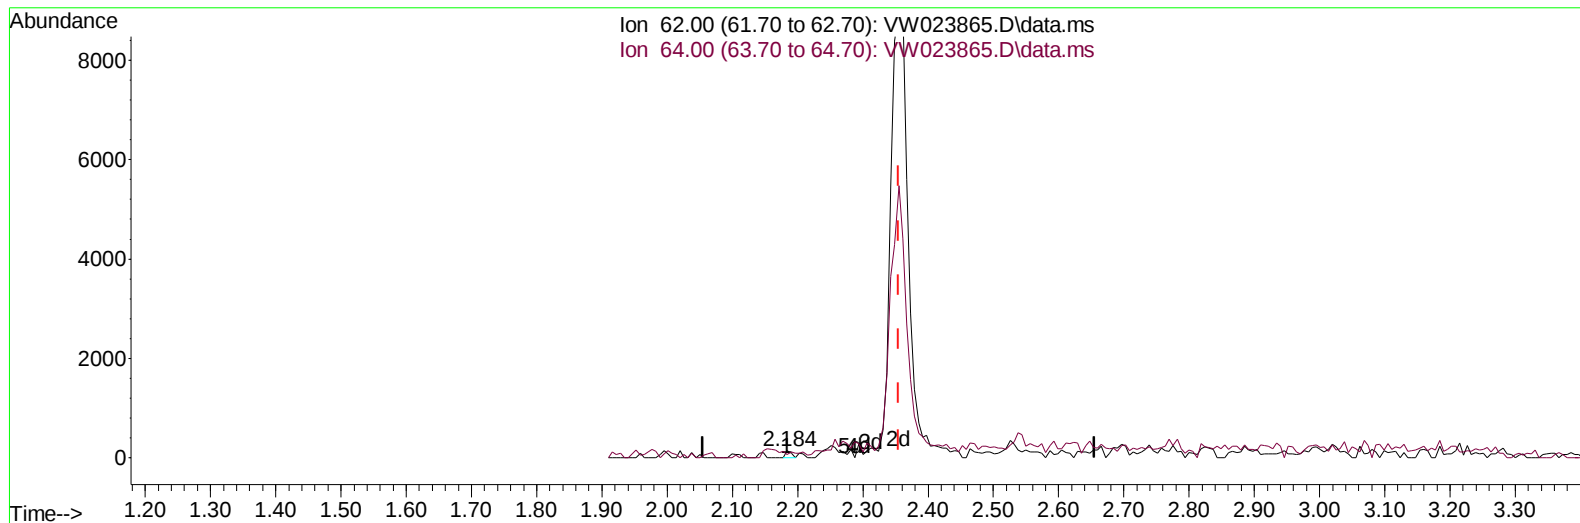

TIC: VW023865.D\data.ms

(5) Vinyl chloride (T)

2.184min (-0.171) 0.01 ug/L

response 81

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	34.30	44.53
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
 Data File : VW023865.D
 Acq On : 19 Jul 2022 03:40
 Operator : SY/VA
 Sample : N3722-11
 Misc : 6.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C46

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/19/2022
 Supervised By :Mahesh Dadoda 07/20/2022

Quant Time: Jul 19 05:40:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 19 02:51:35 2022
 Response via : Initial Calibration

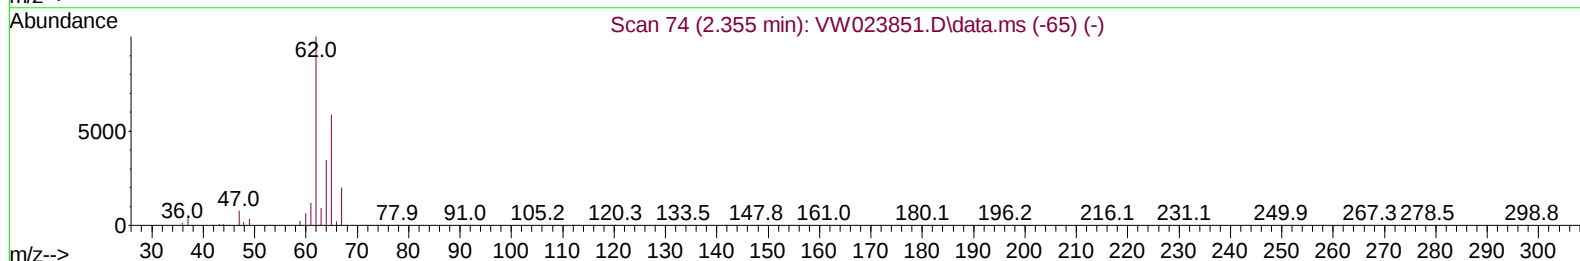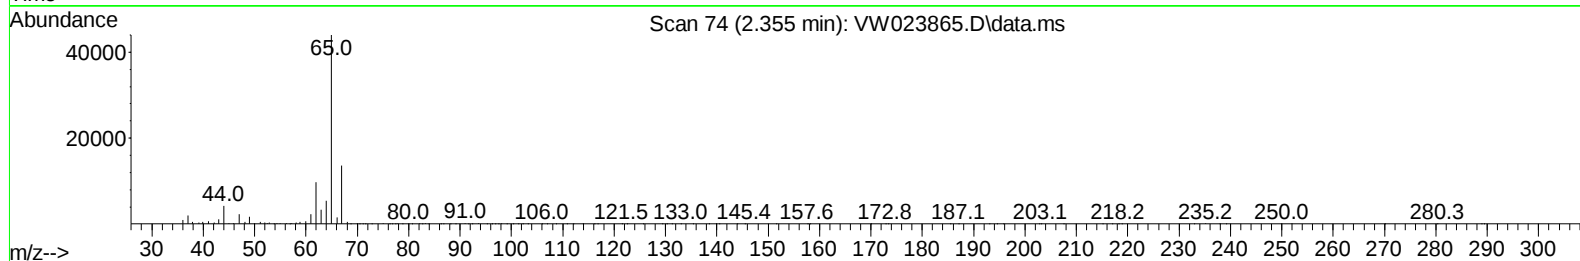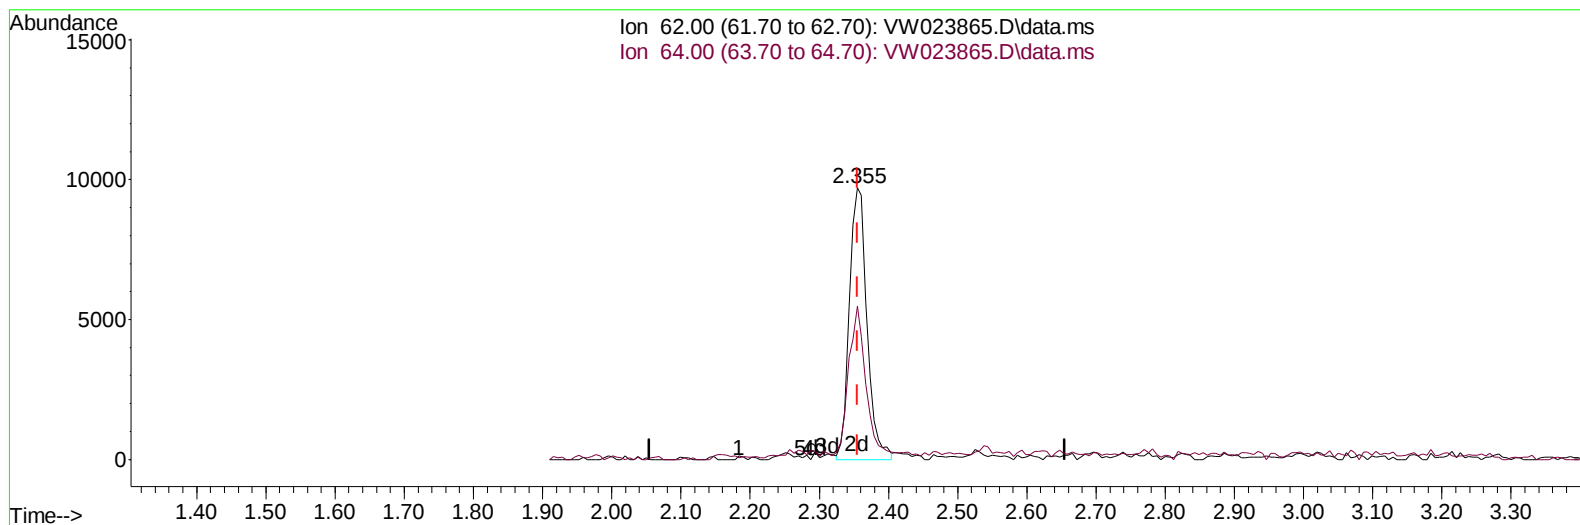

TIC: VW023865.D\data.ms

(5) Vinyl chloride (T)

2.355min (-0.000) 1.55 ug/L m

response 17169

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	34.30	56.38#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
 Data File : VW023865.D
 Acq On : 19 Jul 2022 03:40
 Operator : SY/VA
 Sample : N3722-11
 Misc : 6.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C46

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/19/2022
 Supervised By :Mahesh Dadoda 07/20/2022

Quant Time: Jul 19 05:40:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 19 02:51:35 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		387173	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		354480	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		136742	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		95105	9.618	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	38.480%		
7) Chloroethane-d5	2.879	69		68256	10.347	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	41.400%		
11) 1,1-Dichloroethene-d2	4.013	63		93195	11.574	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	46.280%		
21) 2-Butanone-d5	7.080	46		76074	49.597	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	99.200%		
24) Chloroform-d	7.647	84		219500	19.472	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	77.880%		
26) 1,2-Dichloroethane-d4	8.305	65		125078	18.142	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	72.560%		
32) Benzene-d6	8.275	84		373046	20.245	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	80.960%		
36) 1,2-Dichloropropane-d6	9.274	67		125594	22.627	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	90.520%		
41) Toluene-d8	10.323	98		325221	17.400	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	69.600%		
43) trans-1,3-Dichloroprop...	10.579	79		40248	15.470	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	61.880%		
47) 2-Hexanone-d5	10.920	63		57996	49.689	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	99.380%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		129396	21.095	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	84.360%		
66) 1,2-Dichlorobenzene-d4	13.853	152		109726	22.478	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	89.920%		
Target Compounds							
5) Vinyl chloride	2.355	62		17169m	1.552	ug/L	
13) Acetone	4.123	43		20659	19.050	ug/L	95
16) Methylene chloride	4.922	84		37395	6.177	ug/L	96
20) cis-1,2-Dichloroethene	7.165	96		97582	17.689	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
Data File : VW023865.D
Acq On : 19 Jul 2022 03:40
Operator : SY/VA
Sample : N3722-11
Misc : 6.36g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C46

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/19/2022
Supervised By :Mahesh Dadoda 07/20/2022

Quant Time: Jul 19 05:40:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 19 02:51:35 2022
Response via : Initial Calibration

