


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071822\
Data File : VW023829.D
Acq On : 18 Jul 2022 07:59
Operator : SY/VA
Sample : BFB588
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB588

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Title : SFAM01.0
Last Update : Wed Jul 20 06:30:31 2022

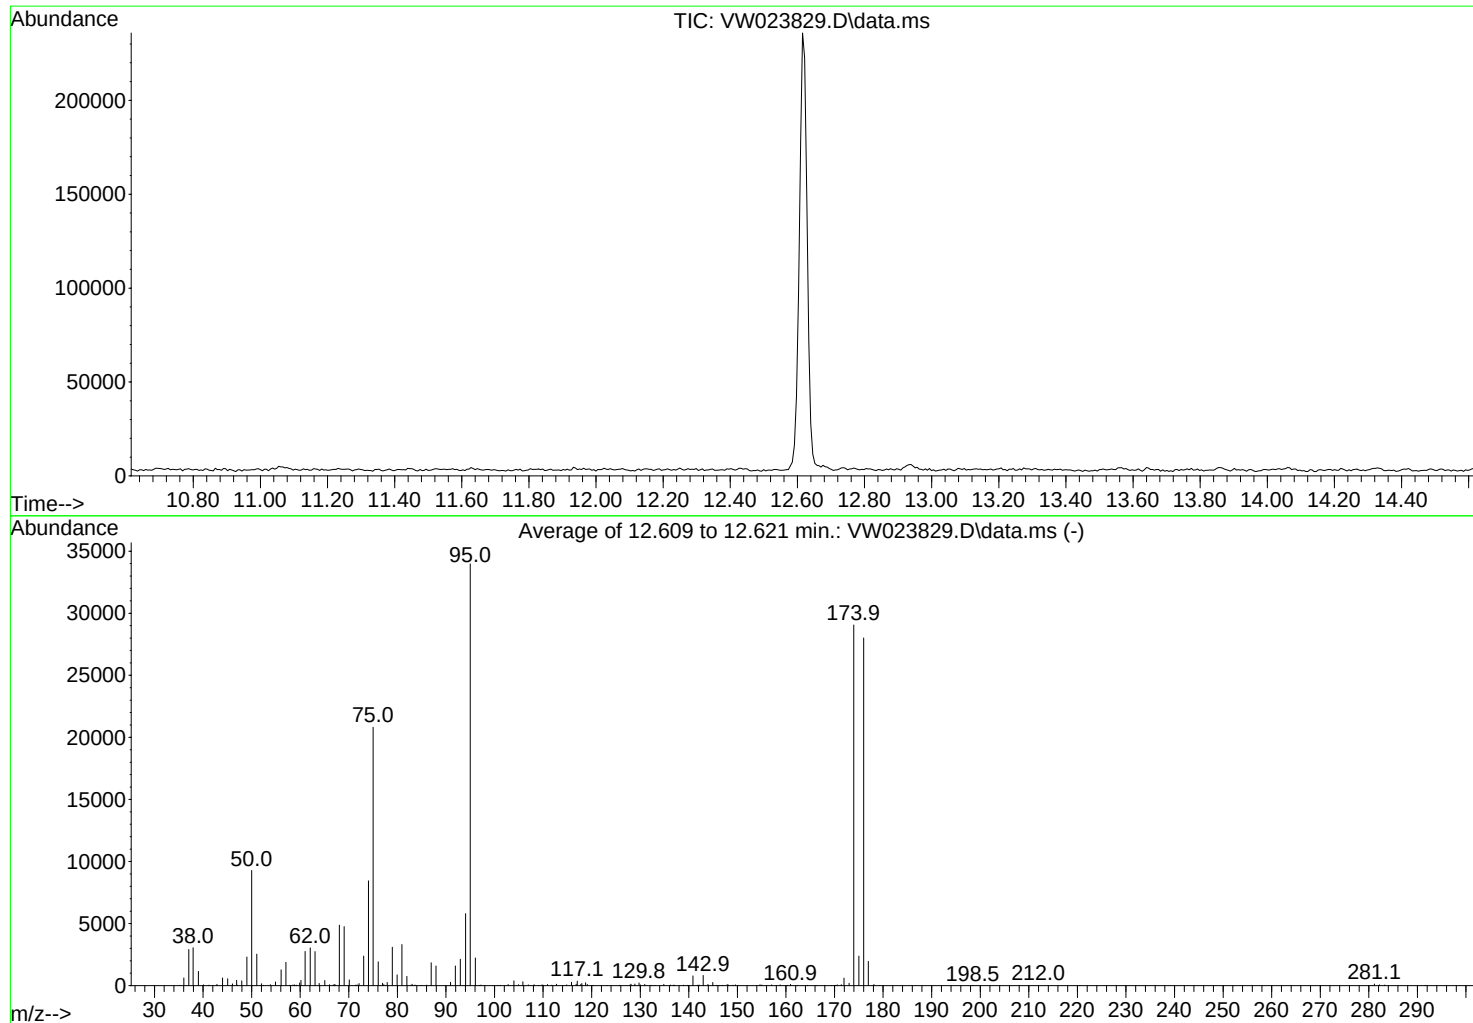

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	27.3	9277	PASS
75	95	30	80	61.3	20816	PASS
95	95	100	100	100.0	33979	PASS
96	95	5	9	6.6	2230	PASS
173	174	0.00	2	0.7	201	PASS
174	95	50	120	85.5	29053	PASS
175	174	5	9	8.2	2388	PASS
176	174	95	105	96.4	28005	PASS
177	176	5	10	7.0	1960	PASS

m/z	Abundance
35.80	72.0
36.50	132.0
37.10	104.0
37.80	98.0
38.80	107.0
39.10	82.0
39.70	150.0
40.50	67.0
41.30	97.0
42.40	97.0
43.10	78.0
44.00	121.0
45.20	67.0
47.10	72.0
48.00	80.0
49.00	109.0
50.50	109.0
53.20	95.0
54.30	75.0
56.30	124.0
58.10	76.0
63.20	80.0
63.80	115.0
64.40	50.0
66.50	62.0
70.60	60.0
72.20	87.0
76.50	50.0
77.80	60.0
84.50	57.0
88.20	57.0
96.80	72.0
111.30	64.0
113.80	77.0
114.60	62.0
120.00	81.0
127.30	153.0
148.60	75.0
157.60	62.0

Instrument :
MSVOA_W
ClientSampleId :
BFB588

m/z	Abundance
36.00	546.0
37.00	2866.0
38.00	2872.0
39.00	1072.0
39.90	165.0
41.20	156.0
42.30	109.0
42.90	94.0
44.00	577.0
45.10	499.0
46.10	176.0
46.90	513.0
48.00	468.0
49.00	2099.0
50.00	8130.0
51.10	2024.0
52.00	203.0
53.00	81.0
53.80	55.0
55.00	378.0
56.10	979.0
57.10	1714.0
58.50	159.0
59.90	655.0
61.00	2441.0
62.00	2706.0
63.00	2606.0
64.10	266.0
65.10	468.0
66.80	169.0
68.10	4110.0
69.00	4279.0
70.10	374.0
71.70	205.0
73.10	2350.0
74.00	6851.0
75.00	18216.0
76.00	1912.0
77.20	217.0
78.00	381.0
78.90	2783.0
80.00	781.0
80.90	2455.0
82.00	541.0
83.00	175.0
83.70	117.0
86.90	1535.0
88.00	1047.0
90.90	143.0
91.90	1285.0
93.00	2144.0
94.10	5065.0
95.00	28880.0
96.10	2036.0
96.90	96.0
97.20	99.0
100.70	99.0
102.90	93.0
104.00	178.0
104.90	66.0
105.80	254.0
106.90	60.0
108.10	75.0
109.10	57.0
109.80	84.0
110.90	101.0
112.80	140.0
115.80	242.0
116.80	364.0
117.70	243.0
118.70	334.0
125.70	73.0
127.90	196.0
128.90	111.0
129.90	86.0
130.90	69.0
134.80	57.0
138.90	70.0
139.70	61.0
140.80	581.0
142.10	155.0
143.00	654.0
144.90	183.0
146.40	65.0
147.90	113.0
149.10	59.0
149.70	107.0
154.60	63.0
155.10	73.0
157.20	69.0
158.80	96.0
160.30	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB588

160.90	106.0
162.30	80.0
169.40	53.0
170.60	79.0
171.90	506.0
173.00	604.0
174.00	22704.0
175.00	2101.0
176.00	20232.0
176.90	1544.0
178.20	96.0
179.20	58.0
198.50	68.0
220.50	52.0
281.20	264.0
282.20	75.0
283.30	86.0

Instrument :
MSVOA_W
ClientSampleId :
BFB588

m/z	Abundance
35.20	69.0
36.10	595.0
37.00	3457.0
38.00	3784.0
39.10	1407.0
40.10	211.0
41.10	153.0
42.00	71.0
42.90	78.0
44.10	845.0
45.10	670.0
46.00	176.0
46.90	776.0
48.00	500.0
49.00	2676.0
50.00	10611.0
51.00	2923.0
52.40	100.0
53.80	119.0
54.40	52.0
54.90	218.0
56.00	1464.0
57.10	2123.0
58.20	128.0
58.80	59.0
59.20	102.0
60.20	582.0
61.00	3205.0
62.10	3565.0
63.00	3256.0
63.90	287.0
65.00	483.0
66.10	151.0
67.00	267.0
68.00	5473.0
69.00	5198.0
70.10	572.0
72.10	358.0
73.10	2321.0
74.10	9351.0
75.00	22928.0
76.10	1990.0
76.90	321.0
78.00	310.0
78.90	3537.0
79.90	932.0
80.90	3849.0
82.00	922.0
83.10	167.0
87.00	1856.0
88.00	2099.0
91.00	391.0
92.00	1827.0
92.90	2174.0
94.00	6596.0
95.00	38136.0
96.00	2594.0
97.20	75.0
99.60	55.0
101.20	71.0
102.80	72.0
103.90	505.0
105.00	80.0
105.90	337.0
106.90	77.0
108.20	81.0
110.00	122.0
110.90	176.0
111.80	77.0
112.80	155.0
114.80	85.0
115.90	259.0
117.10	425.0
118.00	238.0
119.10	281.0
120.10	119.0
128.10	223.0
128.80	107.0
129.80	370.0
131.00	127.0
132.20	66.0
134.80	112.0
136.30	106.0
136.80	127.0
138.90	51.0
140.90	981.0
142.90	913.0
143.90	130.0
145.00	306.0
146.00	53.0
147.90	145.0
149.10	67.0

Instrument :
MSVOA_W
ClientSampleId :
BFB588

149.50	82.0
154.70	104.0
157.00	62.0
158.80	118.0
161.00	55.0
164.40	64.0
170.50	133.0
172.00	685.0
173.90	31976.0
175.00	2558.0
176.00	31600.0
177.00	1924.0
178.10	87.0
281.10	131.0
282.20	60.0

Instrument :
MSVOA_W
ClientSampleId :
BFB588

m/z	Abundance
36.00	726.0
37.10	2716.0
38.00	2802.0
39.00	1215.0
39.80	170.0
40.30	123.0
41.10	105.0
42.20	83.0
42.80	146.0
44.00	789.0
45.00	687.0
46.10	96.0
47.10	327.0
47.90	432.0
49.10	2485.0
50.00	9091.0
51.00	2659.0
52.00	255.0
53.10	124.0
53.90	63.0
54.80	287.0
56.00	1385.0
57.00	1796.0
57.80	97.0
58.80	124.0
60.10	711.0
61.00	2641.0
62.00	2846.0
63.10	2632.0
63.90	337.0
65.00	297.0
66.00	97.0
67.20	184.0
68.00	5038.0
69.10	4784.0
70.10	468.0
71.40	104.0
72.10	407.0
73.00	2491.0
74.10	9112.0
75.00	21304.0
76.00	1861.0
77.00	251.0
77.80	249.0
79.00	2968.0
79.90	895.0
81.00	3620.0
81.90	799.0
82.80	102.0
83.60	61.0
84.90	77.0
86.00	108.0
87.00	2149.0
87.90	1595.0
90.90	277.0
92.00	1668.0
92.90	2054.0
94.00	5757.0
95.00	34920.0
96.00	2059.0
97.00	145.0
102.70	99.0
104.10	485.0
105.00	89.0
105.90	359.0
107.00	51.0
108.10	87.0
109.80	107.0
111.10	191.0
111.80	54.0
112.60	70.0
114.90	109.0
115.90	323.0
117.00	657.0
117.90	257.0
118.80	378.0
120.30	94.0
123.20	56.0
128.10	128.0
129.00	173.0
129.70	193.0
130.00	190.0
130.90	105.0
132.40	69.0
133.00	59.0
134.90	136.0
136.10	56.0
137.00	128.0
140.90	817.0
141.80	116.0
142.90	892.0
144.00	170.0

Instrument :
MSVOA_W
ClientSampleId :
BFB588

145.00	279.0
145.70	79.0
146.90	60.0
148.20	163.0
150.10	69.0
154.60	51.0
155.00	66.0
156.90	59.0
160.90	146.0
166.30	53.0
168.00	64.0
170.20	94.0
171.40	215.0
172.00	642.0
174.00	32480.0
175.00	2505.0
176.00	32184.0
177.00	2411.0
178.00	88.0
212.00	84.0
280.70	53.0
282.20	56.0
283.30	52.0
291.60	69.0

Instrument :
MSVOA_W
ClientSampleId :
BFB588