




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071824\
Data File : VW029639.D
Acq On : 18 Jul 2024 17:52
Operator : SY/MD
Sample : P3264-16
Misc : 6.05g/10mL/MSVOA_W/SoIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CM3

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:17:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 19 01:07:26 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/19/2024
Supervised By :Mahesh Dadoda 07/24/2024

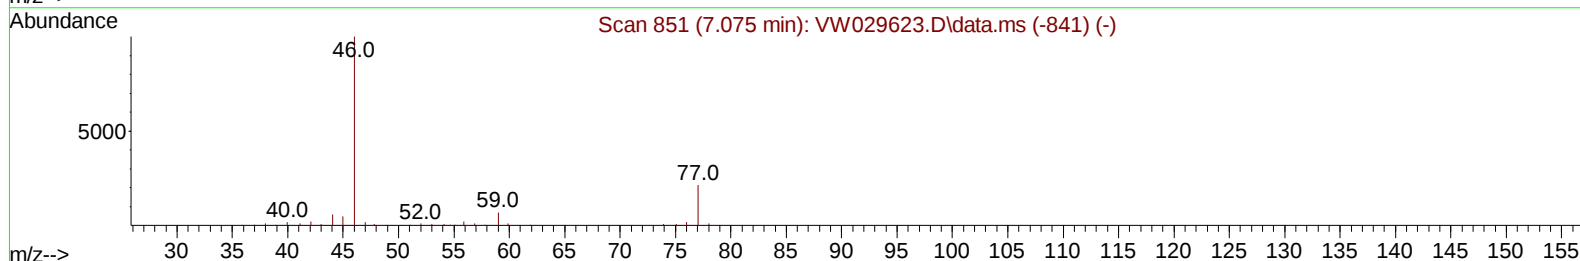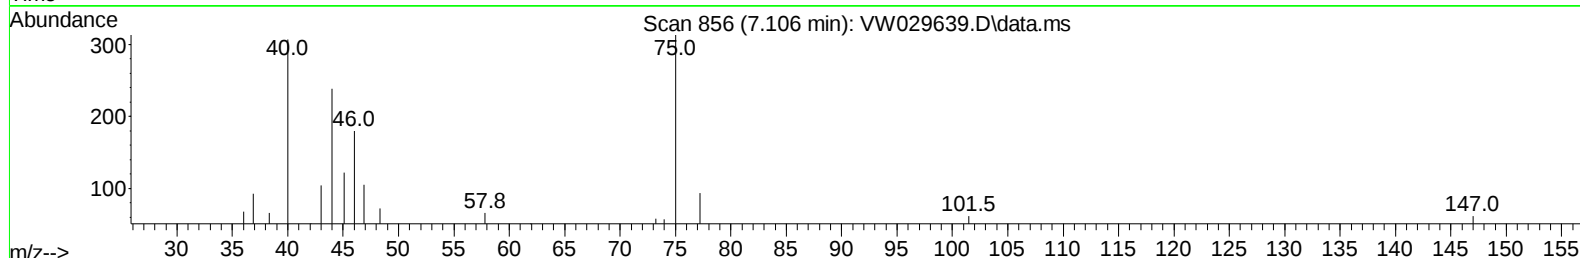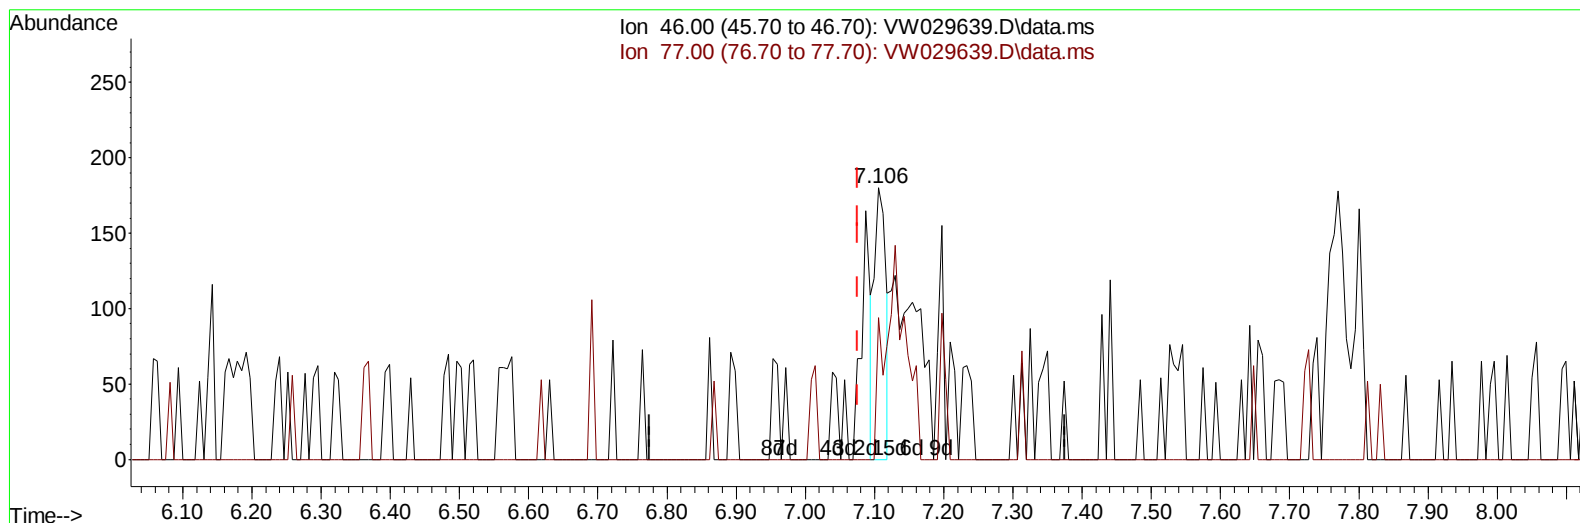

TIC: VW029639.D\data.ms

(21) 2-Butanone-d5 (S)

7.106min (+ 0.031) 0.13 ug/L

response 210

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	21.10	26.19
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071824\
Data File : VW029639.D
Acq On : 18 Jul 2024 17:52
Operator : SY/MD
Sample : P3264-16
Misc : 6.05g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CM3

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:17:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 19 01:07:26 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/19/2024
Supervised By :Mahesh Dadoda 07/24/2024

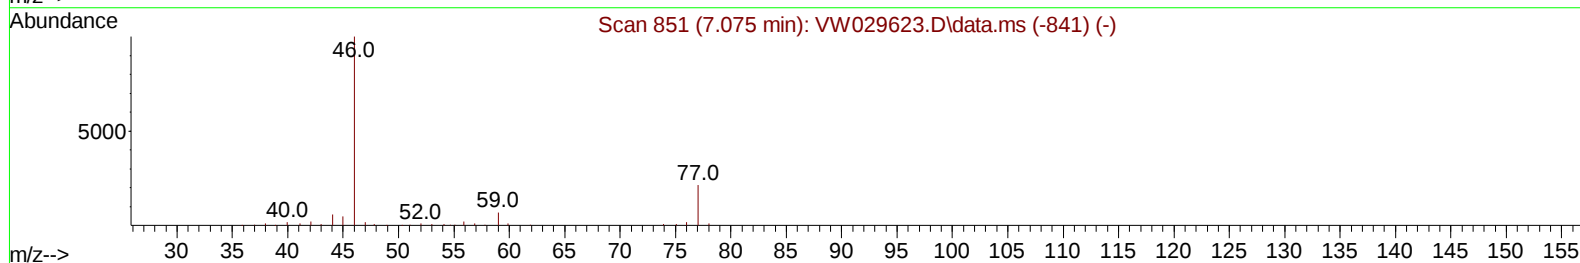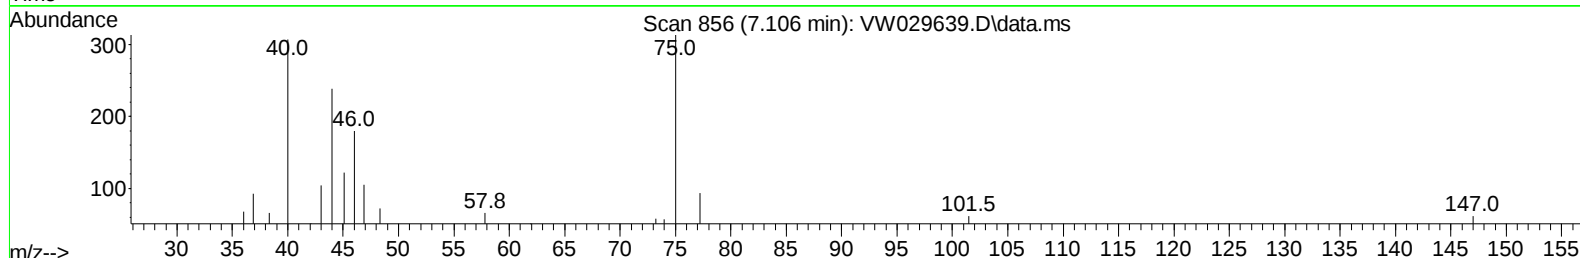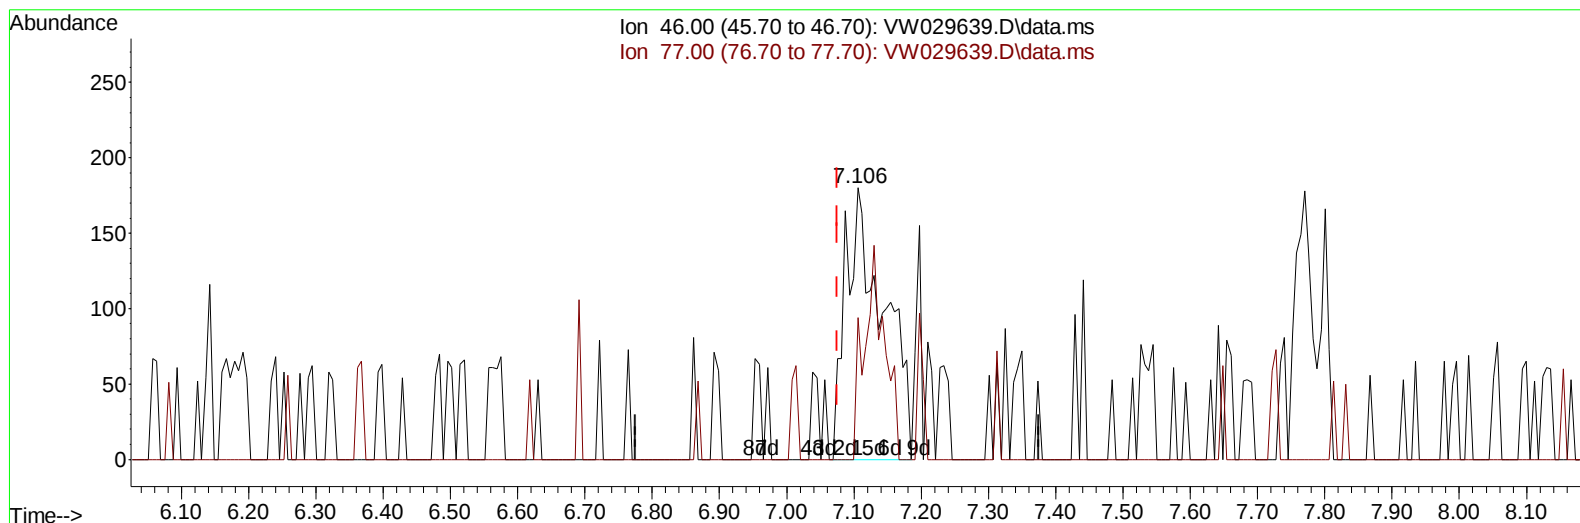

TIC: VW029639.D\data.ms

(21) 2-Butanone-d5 (S)

7.106min (+ 0.031) 0.45 ug/L m

response 705

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	21.10	7.80#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071824\
 Data File : VW029639.D
 Acq On : 18 Jul 2024 17:52
 Operator : SY/MD
 Sample : P3264-16
 Misc : 6.05g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CM3

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:17:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 19 01:07:26 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/19/2024
 Supervised By :Mahesh Dadoda 07/24/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		322643	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		211914	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		47632	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		19442	3.730	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150		Recovery =	14.920%	#	
7) Chloroethane-d5	2.893	69		18231	4.858	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	19.440%	#	
11) 1,1-Dichloroethene-d2	4.015	65		6380	2.726	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	10.920%	#	
21) 2-Butanone-d5	7.106	46		705m	0.451	ug/L	0.03
Spiked Amount 50.000	Range 20	- 135		Recovery =	0.900%	#	
24) Chloroform-d	7.648	84		29874	3.203	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	12.800%	#	
26) 1,2-Dichloroethane-d4	8.307	65		19066	3.485	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	13.920%	#	
32) Benzene-d6	8.276	84		45498	3.584	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	14.320%	#	
36) 1,2-Dichloropropane-d6	9.270	67		17207	4.239	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	16.960%	#	
41) Toluene-d8	10.325	98		21882	1.960	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	7.840%	#	
43) trans-1,3-Dichloroprop...	10.587	79		2454	1.428	ug/L	0.01
Spiked Amount 25.000	Range 30	- 135		Recovery =	5.720%	#	
47) 2-Hexanone-d5	10.934	63		295	0.400	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135		Recovery =	0.800%	#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		6032	1.830	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	7.320%	#	
66) 1,2-Dichlorobenzene-d4	13.848	152		2435	1.468	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	5.880%	#	
Target Compounds							Qvalue
16) Methylene chloride	4.917	84		21874	3.787	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071824\
Data File : VW029639.D
Acq On : 18 Jul 2024 17:52
Operator : SY/MD
Sample : P3264-16
Misc : 6.05g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CM3

Manual IntegrationsAPPROVED

Quant Time: Jul 19 01:17:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 19 01:07:26 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/19/2024
Supervised By :Mahesh Dadoda 07/24/2024

