

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW071918\
 Data File : VW004051.D
 Acq On : 19 Jul 2018 23:08
 Operator : VA/AP
 Sample : J4023-02
 Misc : 6.48G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DB1K3

Quant Time: Jul 20 07:22:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071818S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 20 07:22:04 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	288910	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	282316	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	119112	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	62228	21.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.08%
7) Chloroethane-d5	2.89	69	46154	22.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.64%
10) 1,1-Dichloroethene-d2	4.01	63	108820	15.87	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.48%
20) 2-Butanone-d5	7.08	46	54064	32.26	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.52%
24) Chloroform-d	7.65	84	170351	24.84	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.36%
26) 1,2-Dichloroethane-d4	8.31	65	97328	23.57	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.28%
29) Benzene-d6	8.27	84	297853	22.75	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.00%
33) 1,2-Dichloropropane-d6	9.27	67	106511	24.39	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.56%
37) Toluene-d8	10.33	98	257019	21.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.36%
38) trans-1,3-Dichloropropene-	10.58	79	39417	20.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.16%
39) 2-Hexanone-d5	10.93	63	35887	30.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	61.04%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	95391	19.93	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.72%
61) 1,2-Dichlorobenzene-d4	13.86	152	101208	26.42	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.68%

Target Compounds


					Qvalue
13) Acetone	4.12	43	52744	28.950	ug/L 100
16) Methylene chloride	4.91	84	13816	2.493	ug/L 87
21) 2-Butanone	7.18	43	8720	3.857	ug/L 86
40) 1,2-Dichloropropane	9.27	63	12116	2.583	ug/L # 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW071918\
Data File : VW004051.D
Acq On : 19 Jul 2018 23:08
Operator : VA/AP
Sample : J4023-02
Misc : 6.48G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB1K3

Quant Time: Jul 20 07:22:26 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071818S.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 20 07:22:04 2018
Response via : Initial Calibration




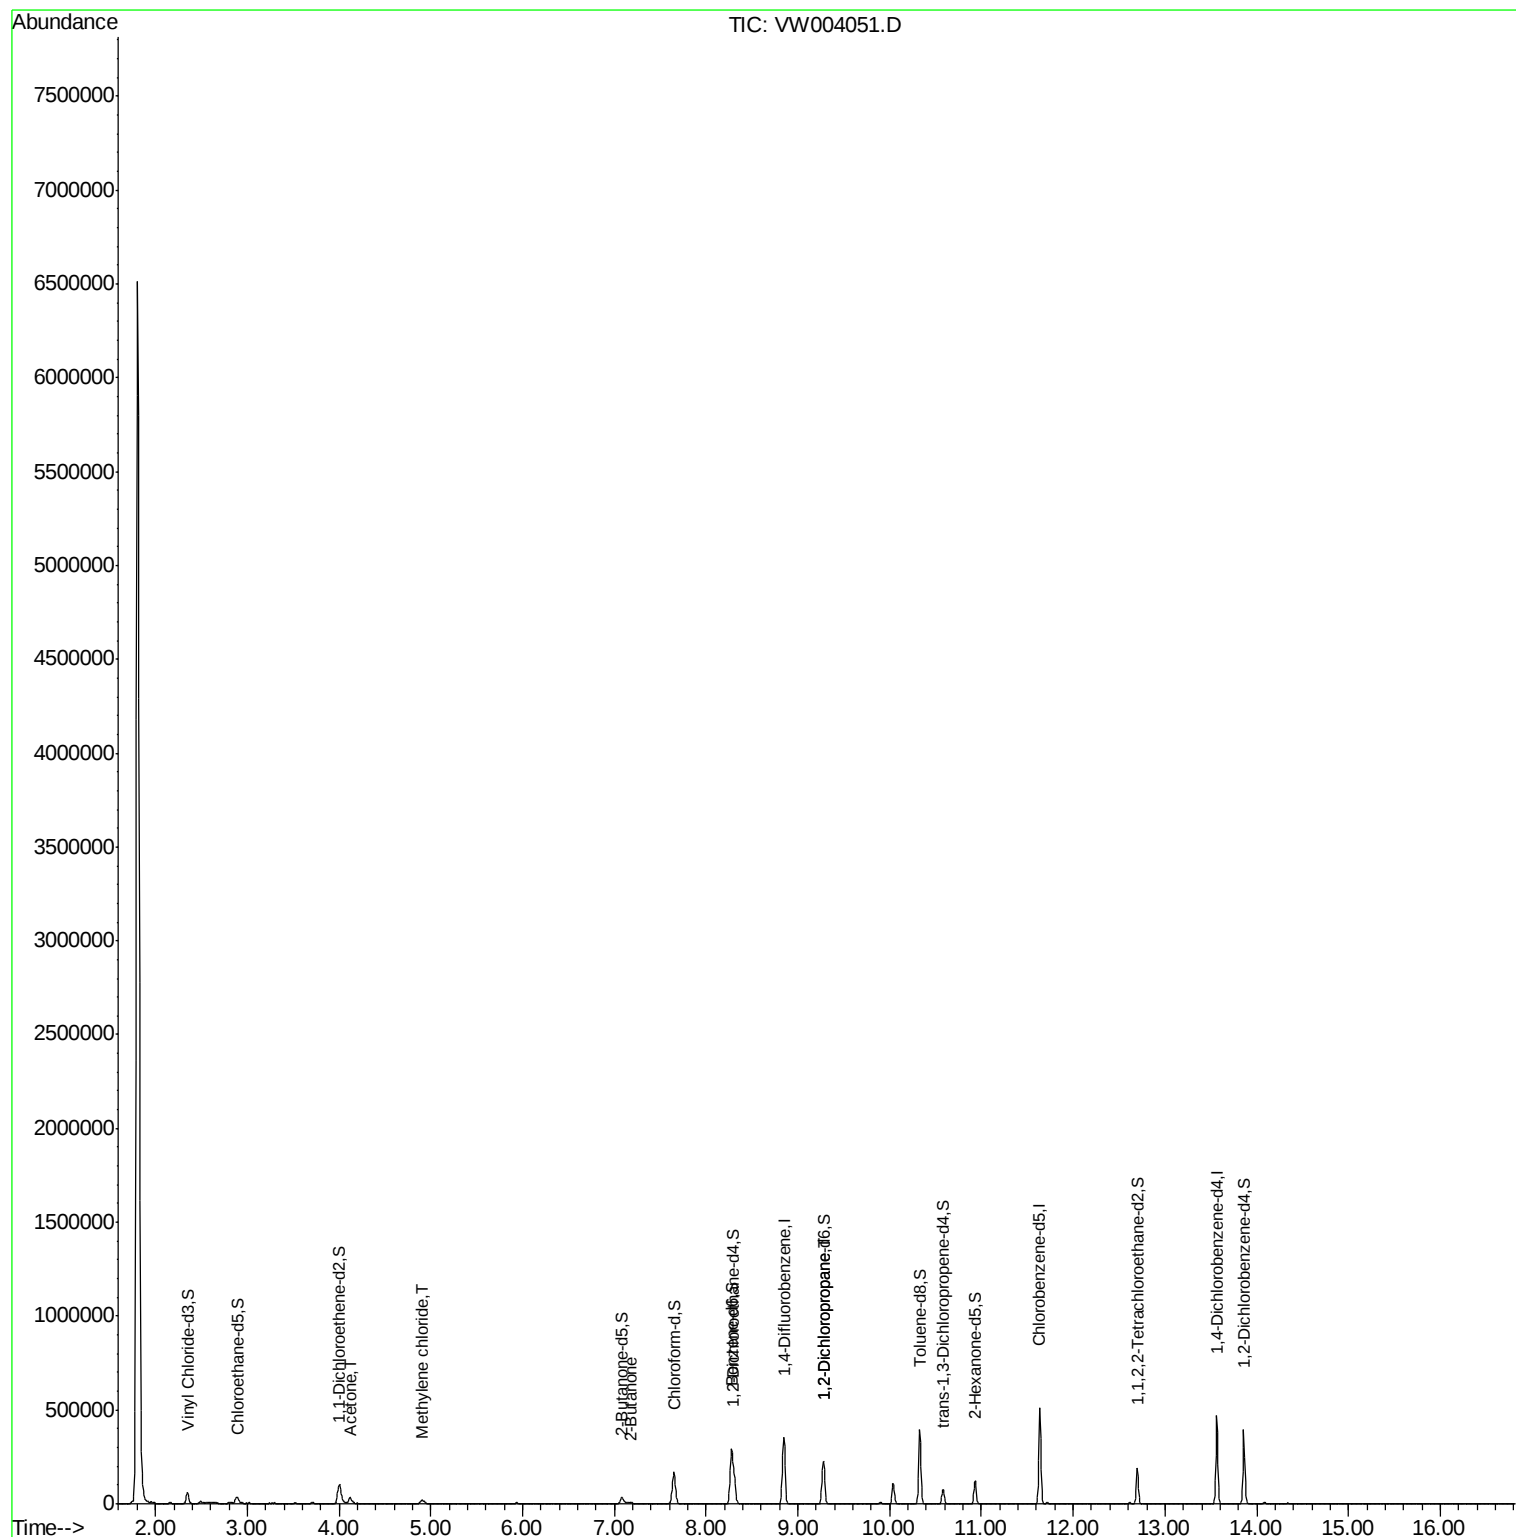


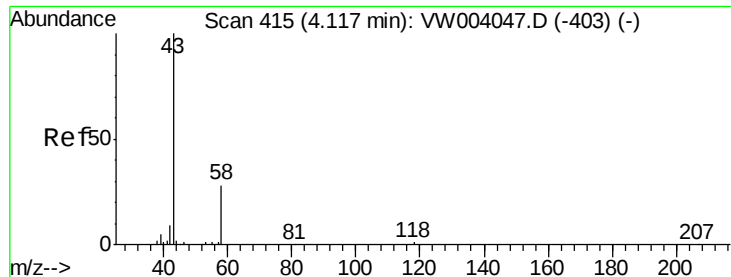

#13
Acetone
Concen: 28.950 ug/L
RT: 4.12 min Scan# 416
Delta R.T. 0.01 min
Lab File: VW004051.D
Acq: 19 Jul 2018 23:08




Instrument :
MSVOA_W
ClientSampleId :
DB1K3


Tgt Ion: 43 Resp: 52744
Ion Ratio Lower Upper
43 100
58 29.9 0.0 59.4

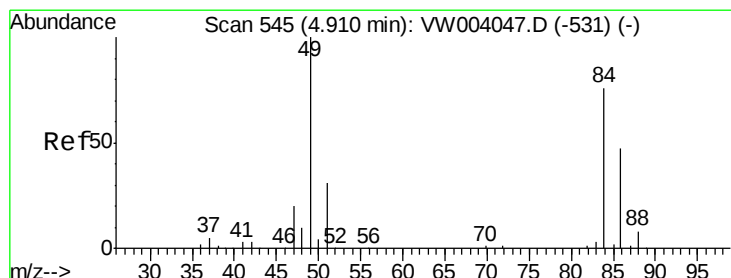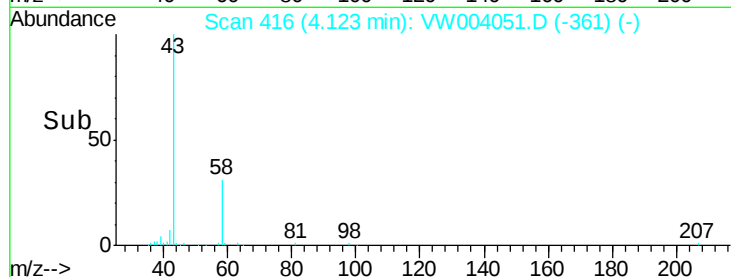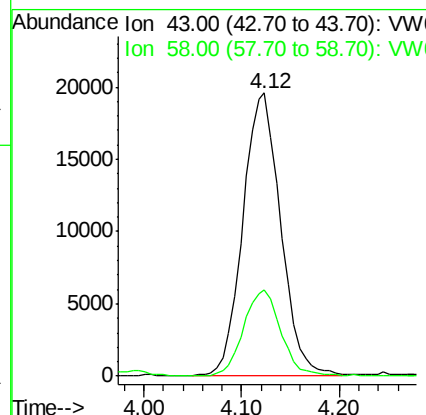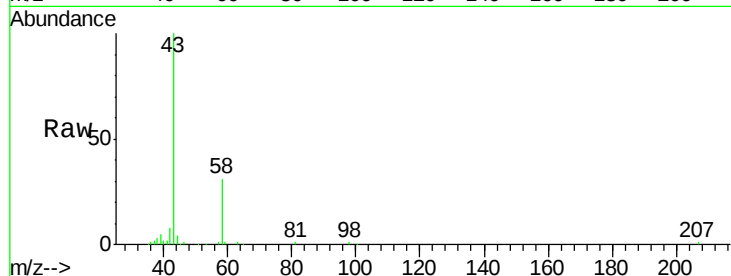

#16
Methylene chloride
Concen: 2.493 ug/L
RT: 4.91 min Scan# 545
Delta R.T. -0.00 min
Lab File: VW004051.D
Acq: 19 Jul 2018 23:08

Tgt Ion: 84 Resp: 13816
Ion Ratio Lower Upper
84 100
49 117.4 94.2 175.0
86 56.4 45.1 83.9

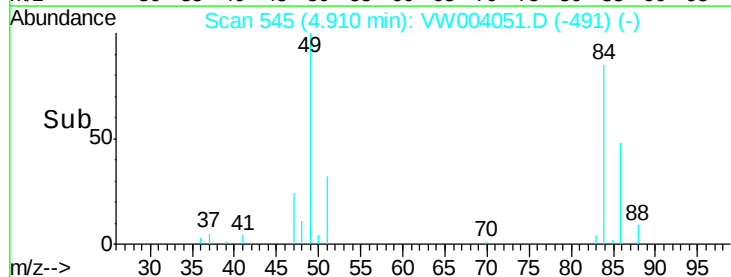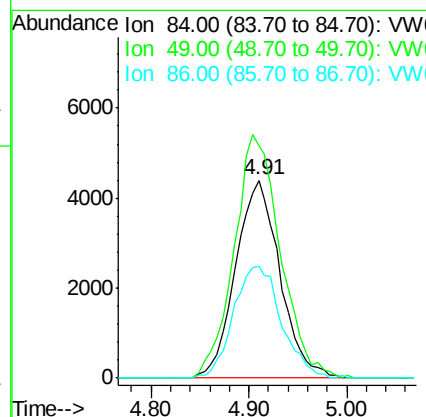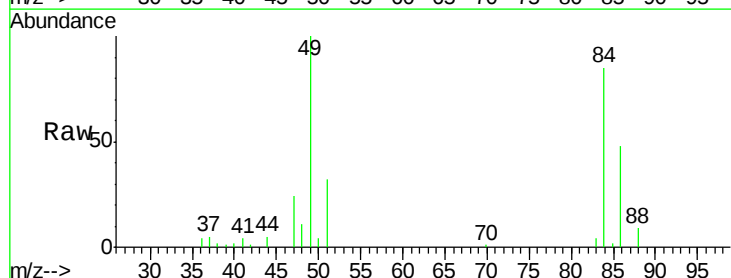

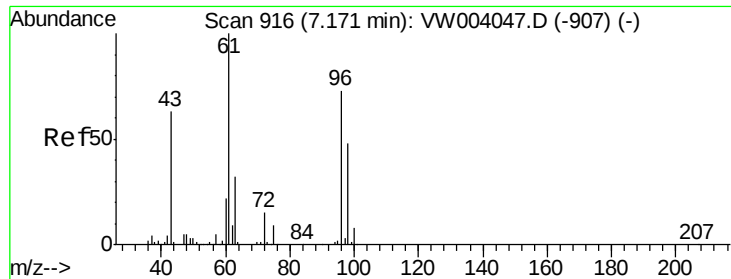

#21

2-Butanone

Concen: 3.857 ug/L

RT: 7.18 min Scan# 918

Delta R.T. 0.01 min

Lab File: VW004051.D

Acq: 19 Jul 2018 23:08

Instrument :

MSVOA_W

ClientSampleId :





DB1K3

Tgt Ion: 43 Resp: 8720

Ion Ratio Lower Upper

43 100

72 17.5 12.1 36.3

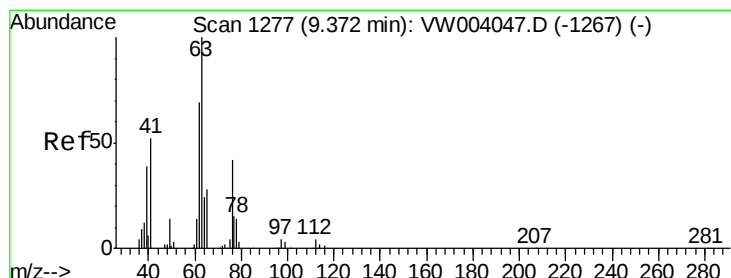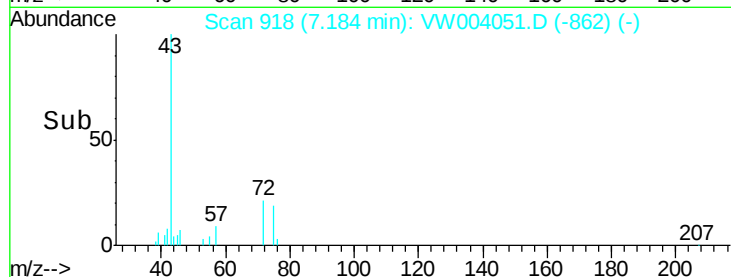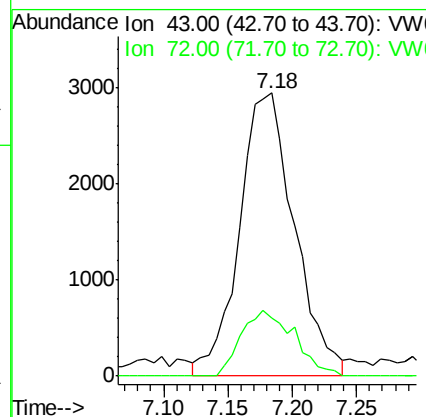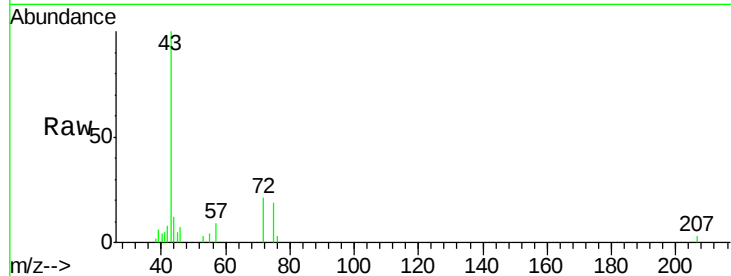

#40

1,2-Dichloropropane

Concen: 2.583 ug/L

RT: 9.27 min Scan# 1261

Delta R.T. -0.10 min

Lab File: VW004051.D

Acq: 19 Jul 2018 23:08

Tgt Ion: 63 Resp: 12116

Ion Ratio Lower Upper

63 100

112 0.4 3.0 4.4#

