


Tert butyl alcohol

Response Ratio

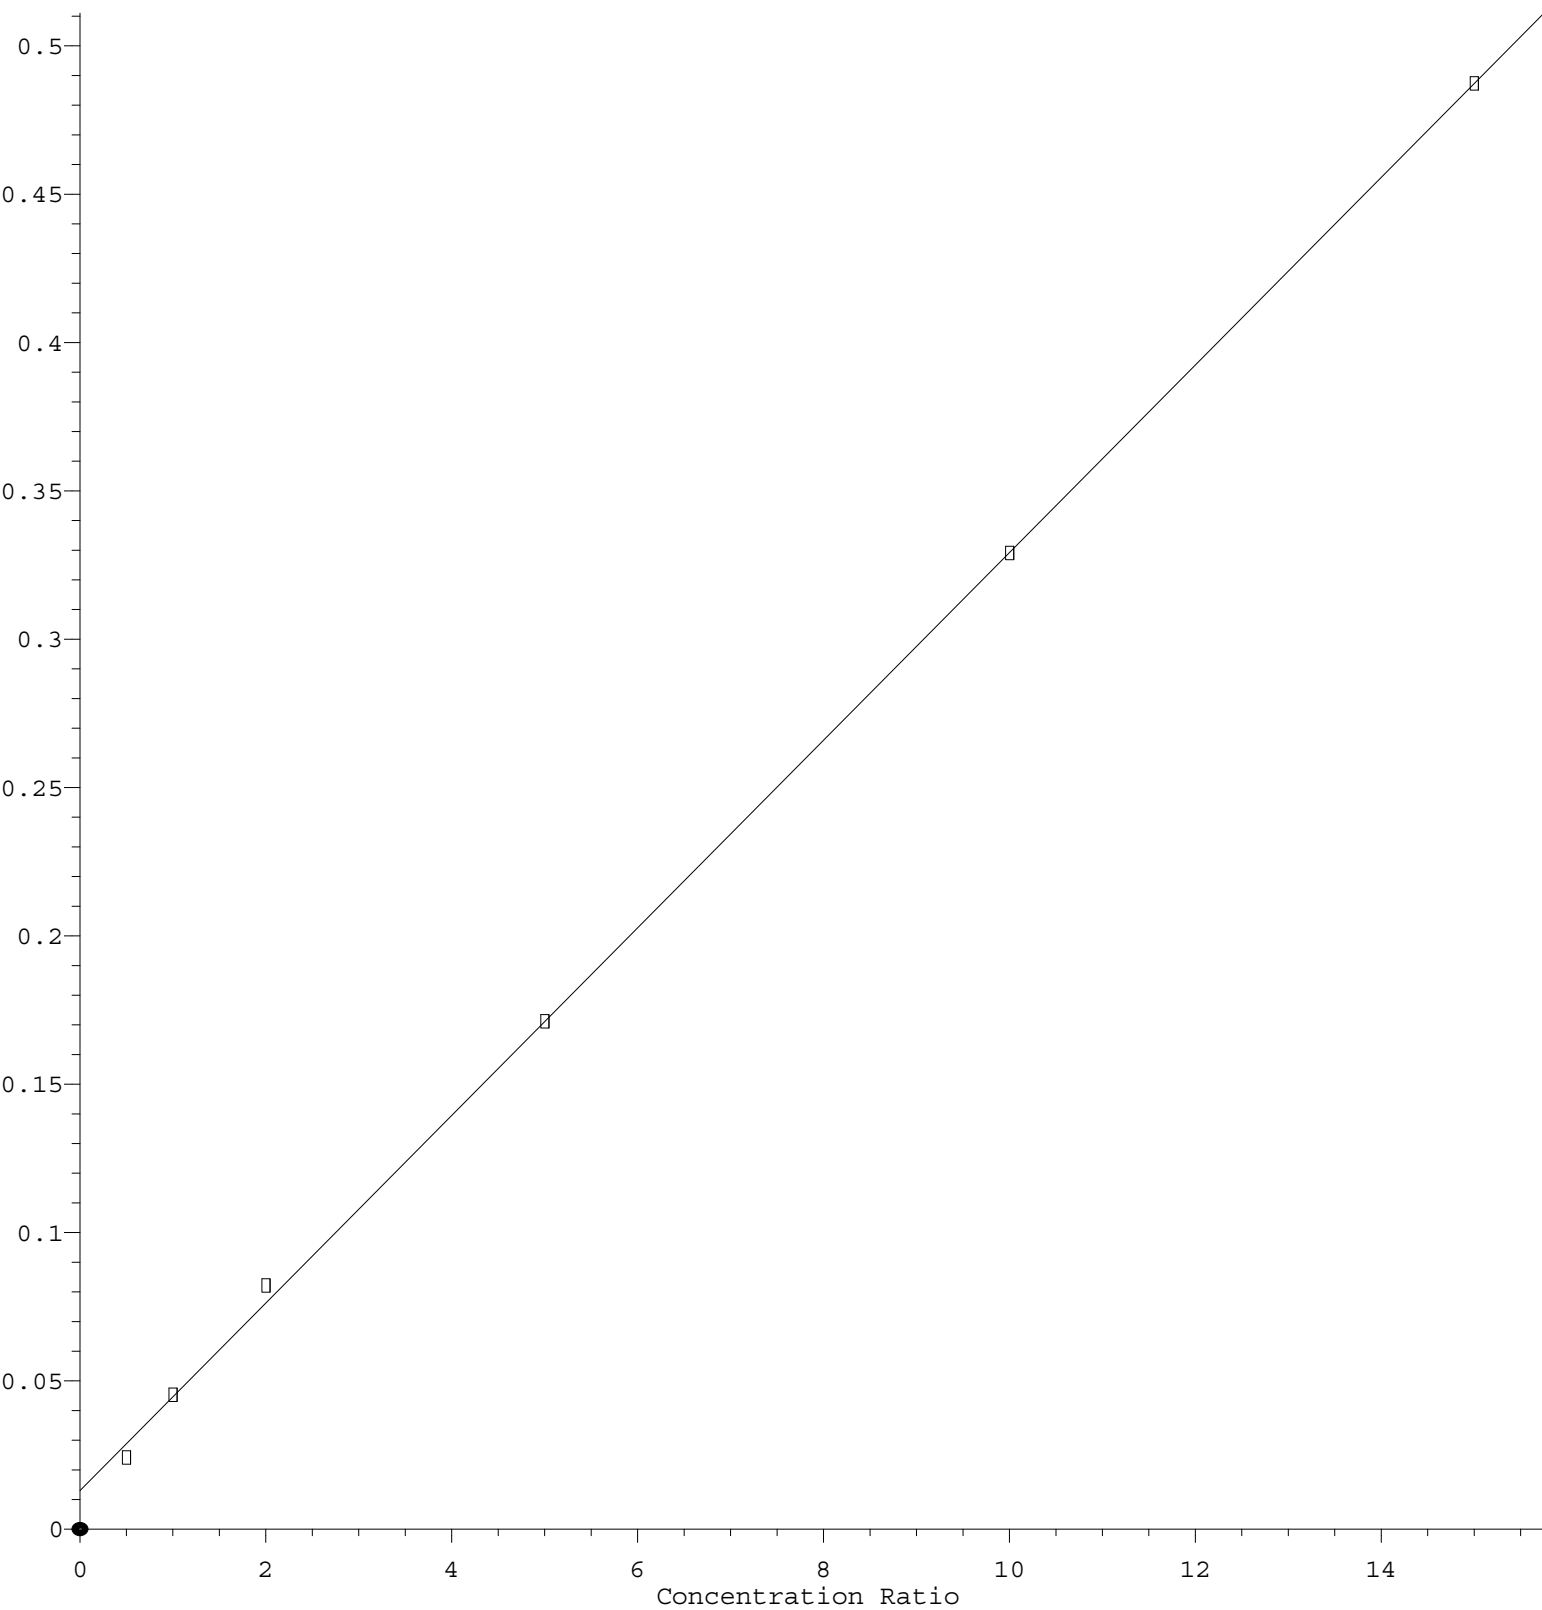

$$\text{Response} = 3.161\text{e-}002 * \text{Amt} + 1.335\text{e-}002$$


Coef of Det (r^2) = 0.999665 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W071921S.M

Calibration Table Last Updated: Tue Jul 20 04:37:55 2021

1,2-Dichloroethane-d4

Response Ratio

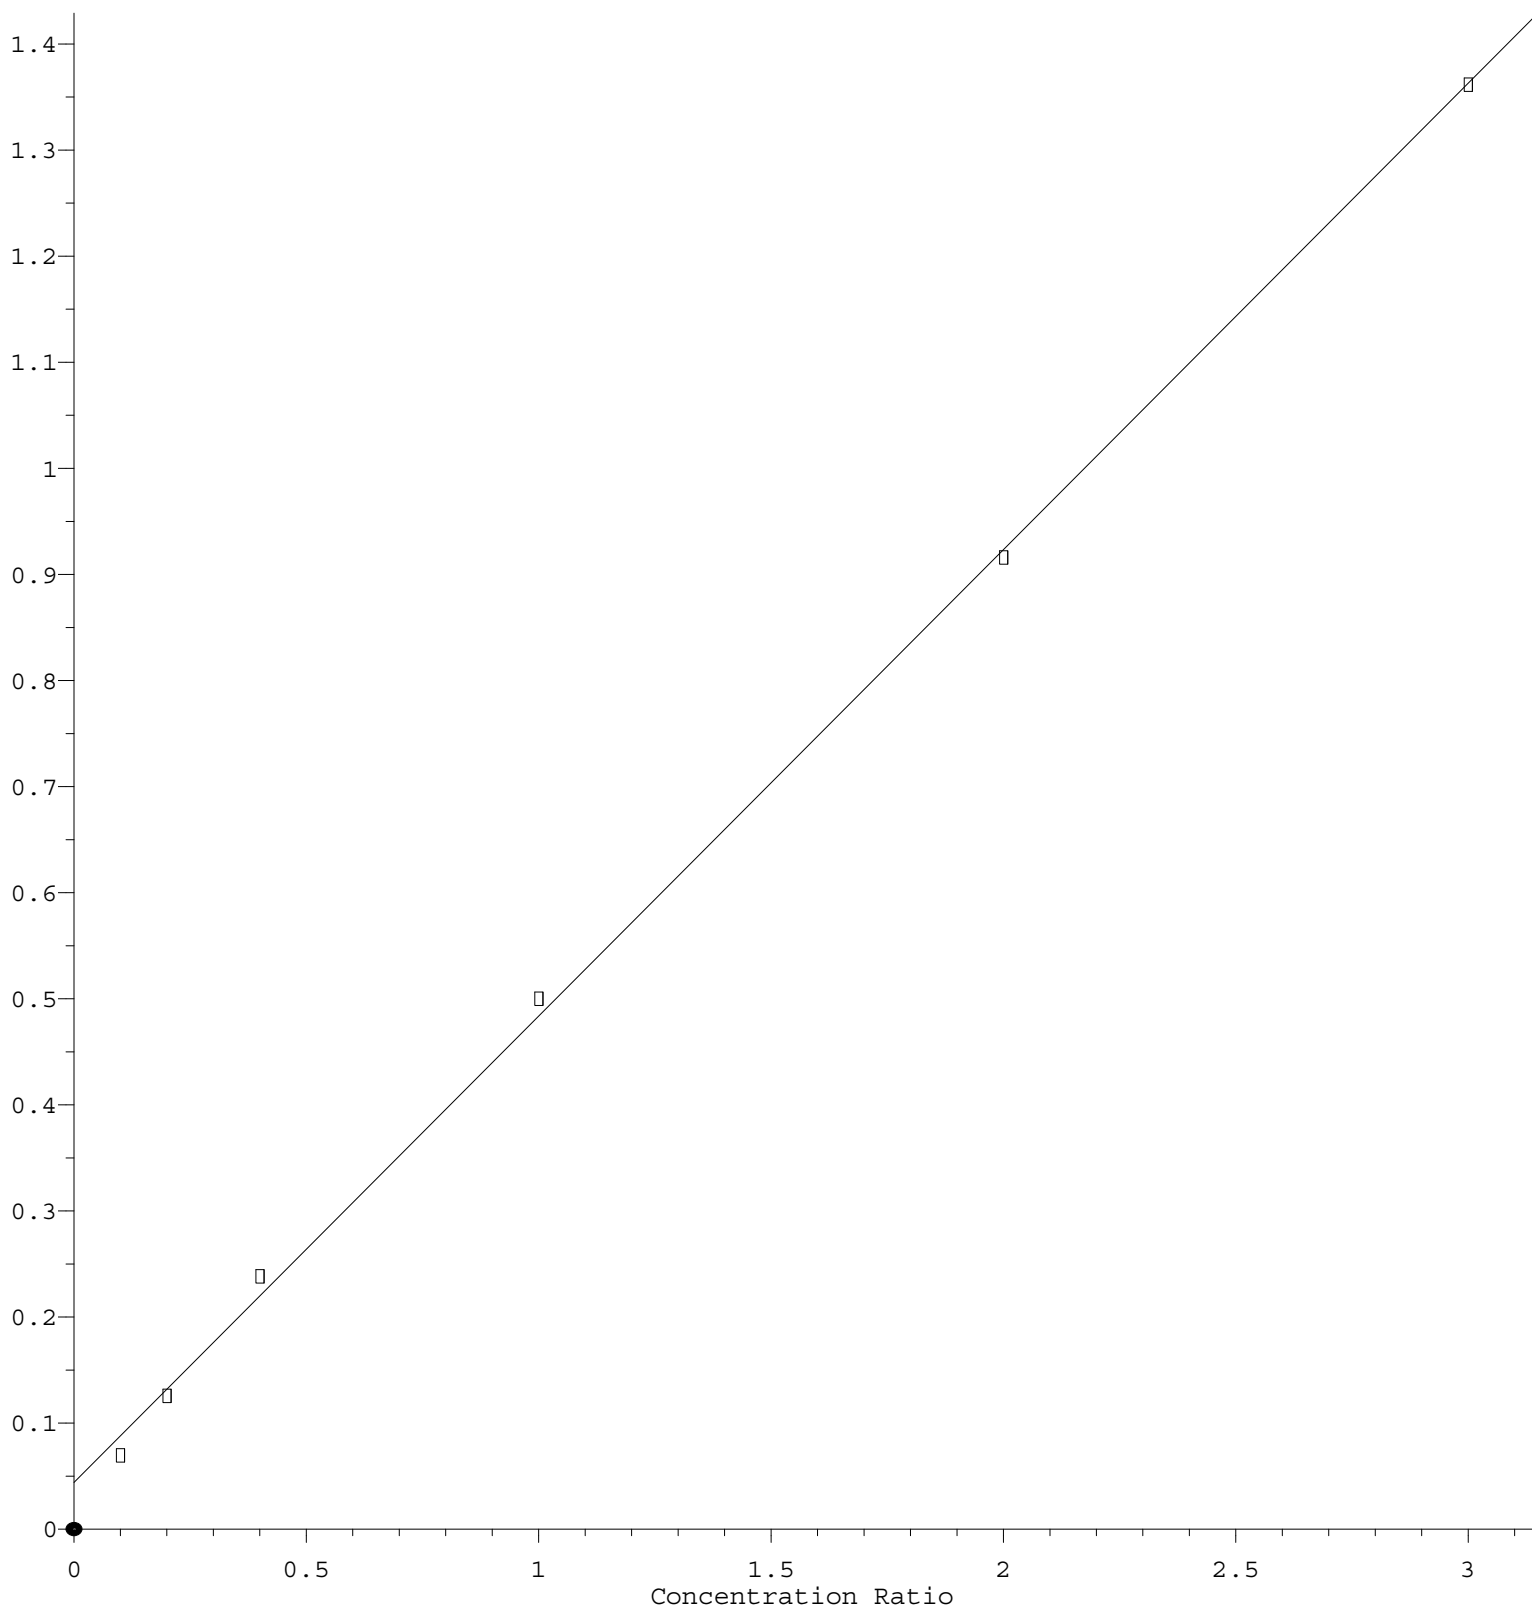

$$\text{Response} = 4.397\text{e-}001 * \text{Amt} + 4.413\text{e-}002$$


Coef of Det (r^2) = 0.999202 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W071921S.M

Calibration Table Last Updated: Tue Jul 20 04:37:55 2021

Methylene Chloride

Response Ratio

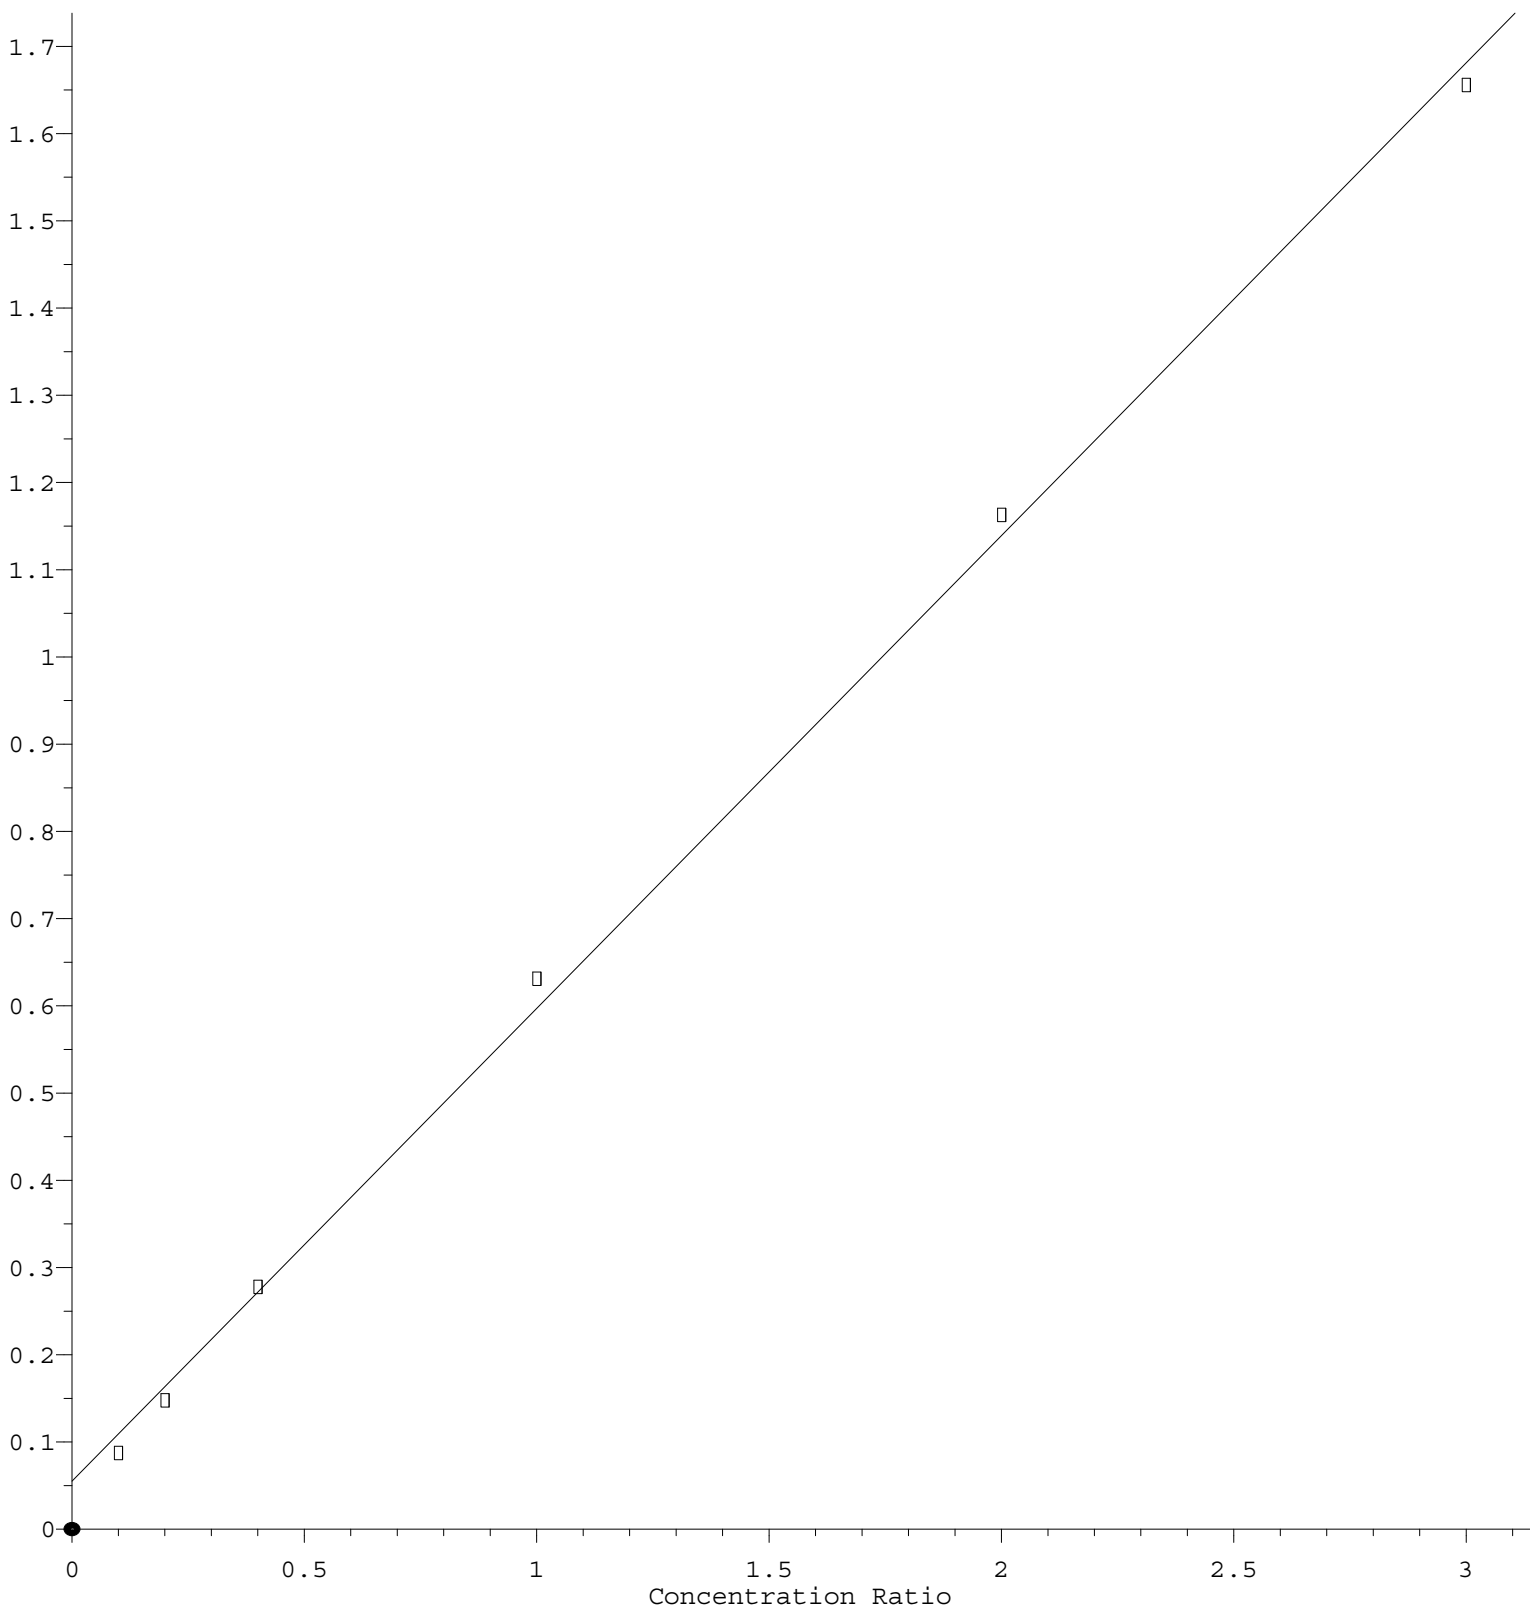

$$\text{Response} = 5.423\text{e-}001 * \text{Amt} + 5.480\text{e-}002$$

Coef of Det (r^2) = 0.998428 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W071921S.M

Calibration Table Last Updated: Tue Jul 20 04:37:55 2021