




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
Data File : VW029651.D
Acq On : 19 Jul 2024 13:11
Operator : SY/MD
Sample : VIBLK498
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK498

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:27:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 19 23:16:32 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/22/2024
Supervised By :Mahesh Dadoda 07/24/2024

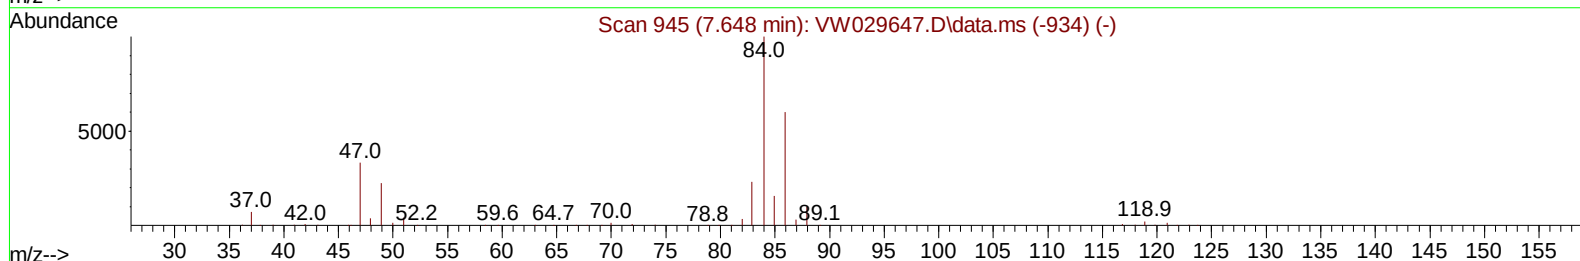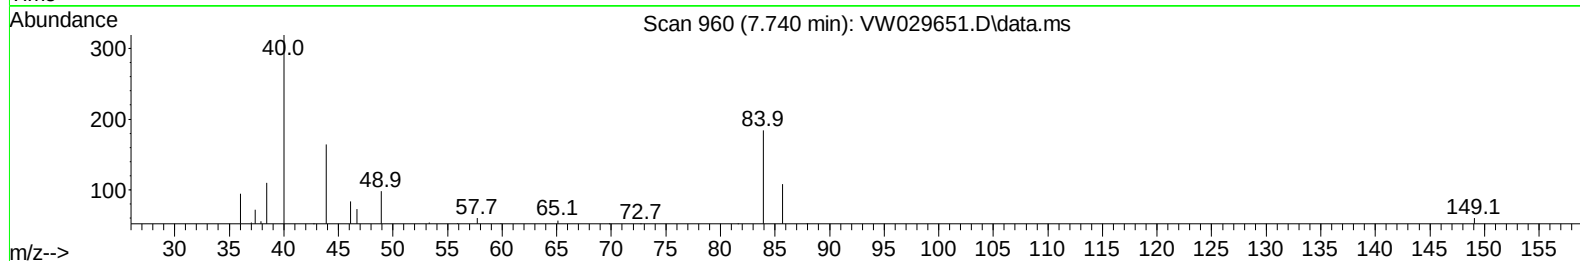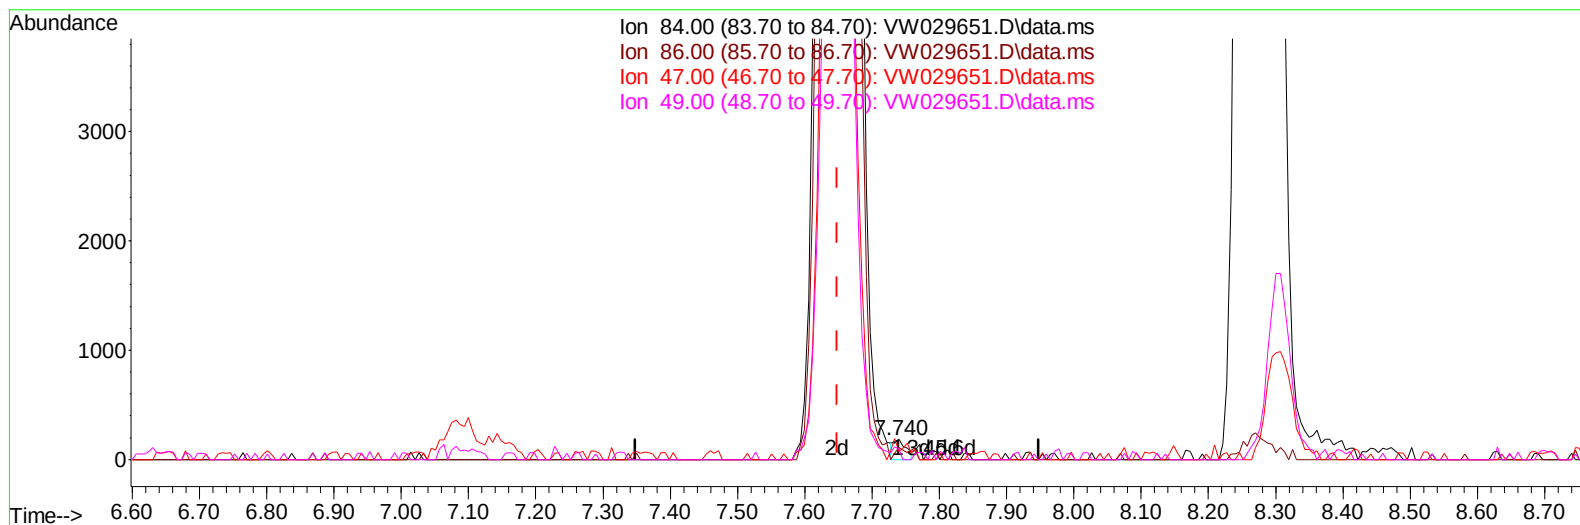

TIC: VW029651.D\data.ms

(24) Chloroform-d (S)

7.740min (+ 0.092) 0.03 ug/L

response	234	
Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	48.29
47.00	48.40	53.85
49.00	27.80	33.76




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
 Data File : VW029651.D
 Acq On : 19 Jul 2024 13:11
 Operator : SY/MD
 Sample : VIBLK498
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK498

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:27:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 19 23:16:32 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/22/2024
 Supervised By :Mahesh Dadoda 07/24/2024

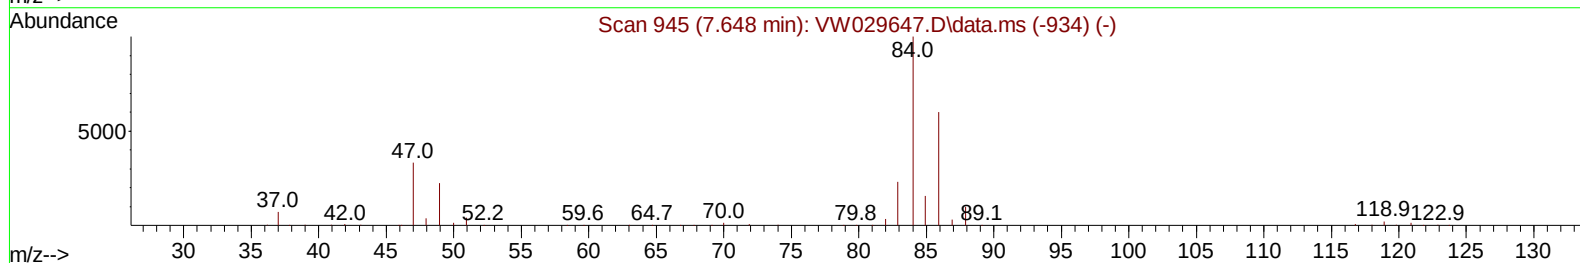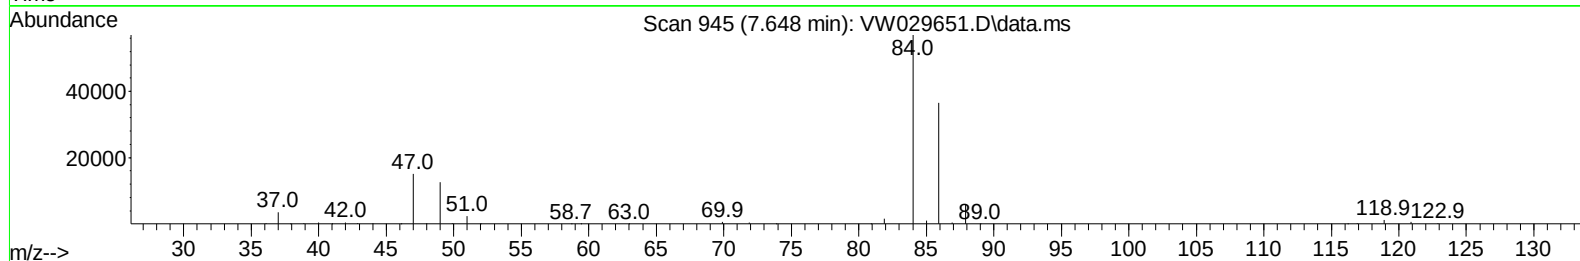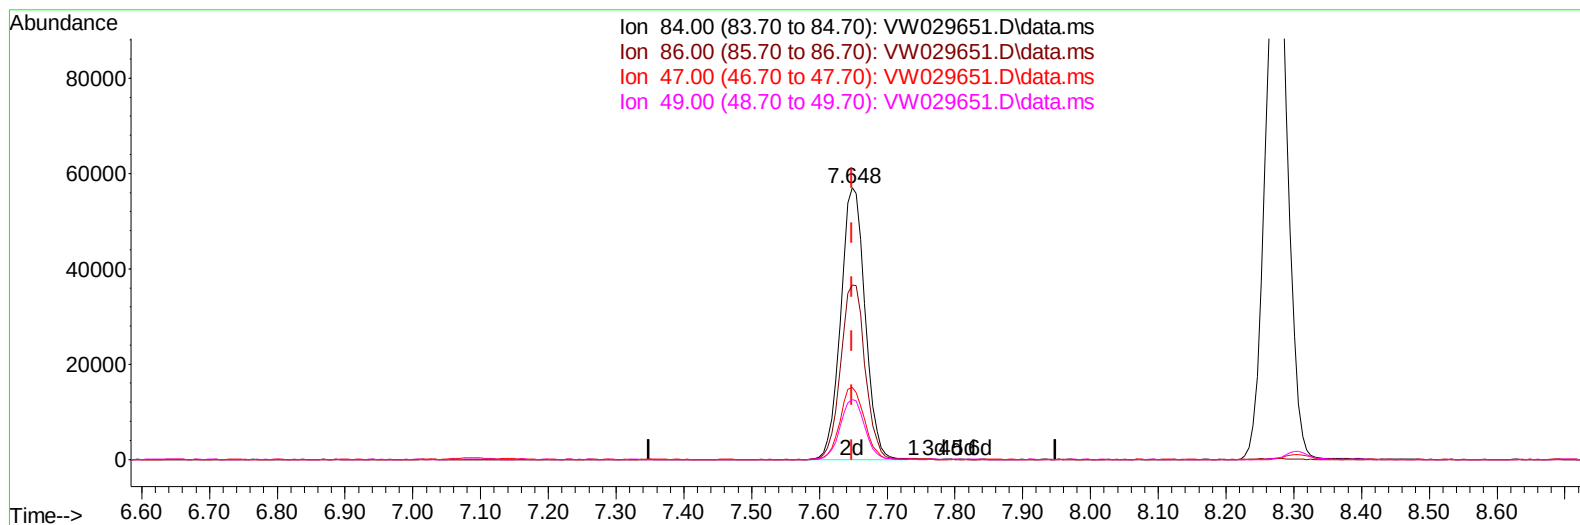

TIC: VW029651.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.000) 20.29 ug/L m

response 142011

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	0.08#
47.00	48.40	0.09#
49.00	27.80	0.06#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
 Data File : VW029651.D
 Acq On : 19 Jul 2024 13:11
 Operator : SY/MD
 Sample : VIBLK498
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK498

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:27:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 19 23:16:32 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/22/2024
 Supervised By :Mahesh Dadoda 07/24/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		242112	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		227070	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		105291	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		63326	16.191	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	64.760%		
7) Chloroethane-d5	2.899	69		51893	18.426	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	73.720%		
11) 1,1-Dichloroethene-d2	4.021	65		32215	18.342	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	73.360%		
21) 2-Butanone-d5	7.081	46		35967	30.634	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	61.260%		
24) Chloroform-d	7.648	84		142011m	20.289	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	81.160%		
26) 1,2-Dichloroethane-d4	8.307	65		83130	20.249	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	81.000%		
32) Benzene-d6	8.276	84		267052	19.632	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	78.520%		
36) 1,2-Dichloropropane-d6	9.270	67		90658	20.844	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	83.360%		
41) Toluene-d8	10.325	98		236021	19.729	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	78.920%		
43) trans-1,3-Dichloroprop...	10.581	79		31184	16.932	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	67.720%		
47) 2-Hexanone-d5	10.922	63		23128	29.264	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	58.520%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		61899	17.529	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	70.120%		
66) 1,2-Dichlorobenzene-d4	13.849	152		73622	20.078	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	80.320%		
Target Compounds							
16) Methylene chloride	4.911	84		15019	3.465	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
Data File : VW029651.D
Acq On : 19 Jul 2024 13:11
Operator : SY/MD
Sample : VIBLK498
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK498

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:27:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 19 23:16:32 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/22/2024
Supervised By :Mahesh Dadoda 07/24/2024

