




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
 Data File : VW029657.D
 Acq On : 19 Jul 2024 15:34
 Operator : SY/MD
 Sample : P3265-10
 Misc : 5.00g/10mL/MSVOA_W/SoIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4DA8

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:21:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 19 23:16:32 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/22/2024
 Supervised By :Mahesh Dadoda 07/24/2024

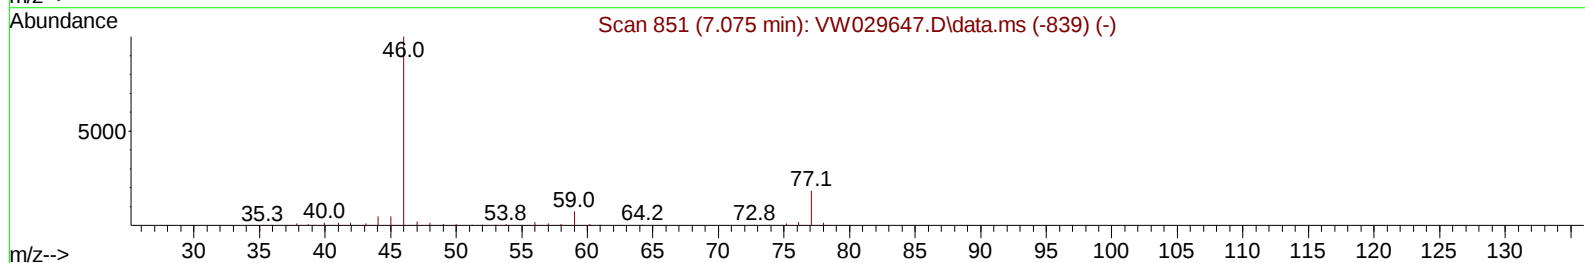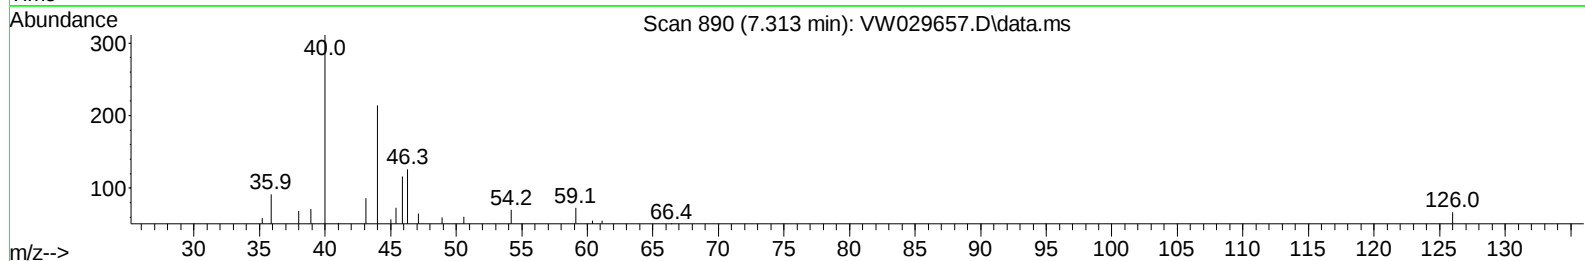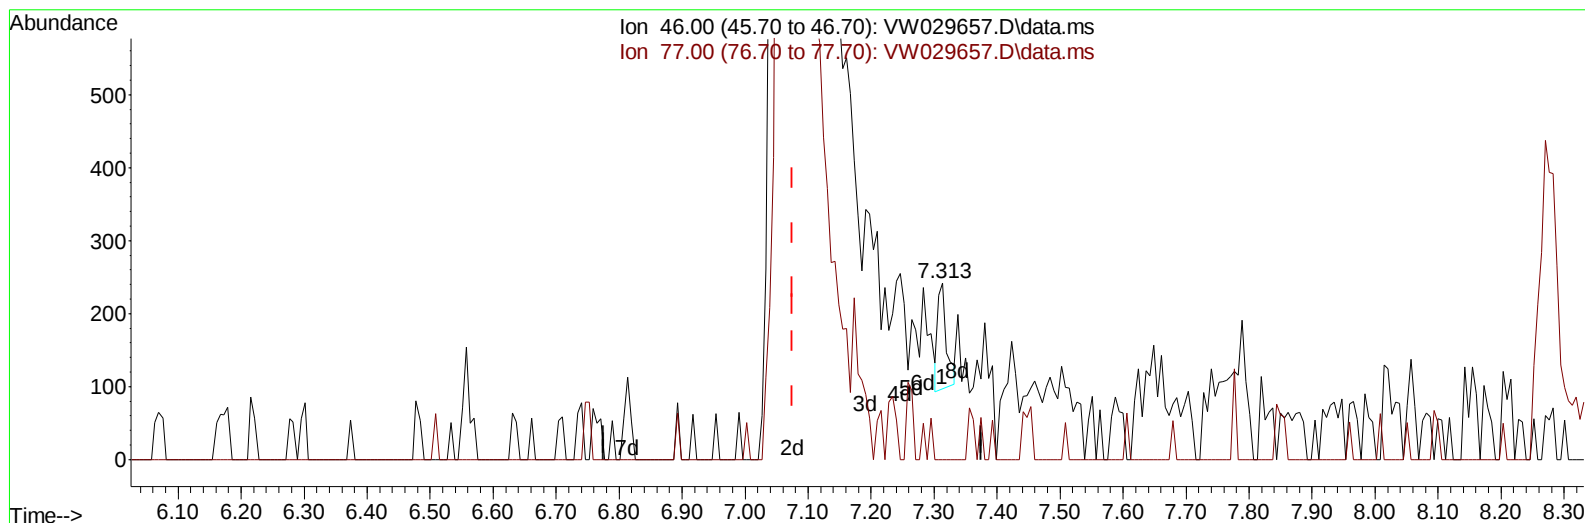

TIC: VW029657.D\data.ms

(21) 2-Butanone-d5 (S)

7.313min (+ 0.238) 0.06 ug/L

response 141

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	21.10	14.89
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
 Data File : VW029657.D
 Acq On : 19 Jul 2024 15:34
 Operator : SY/MD
 Sample : P3265-10
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4DA8

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:21:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 19 23:16:32 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/22/2024
 Supervised By :Mahesh Dadoda 07/24/2024

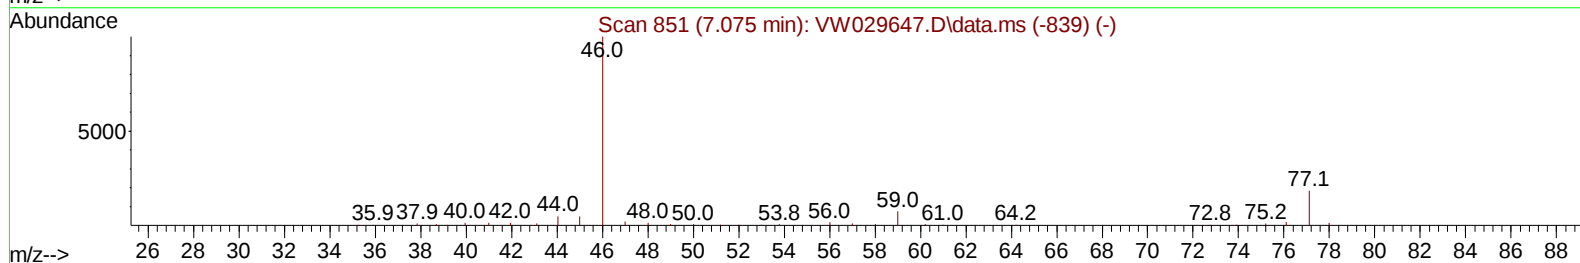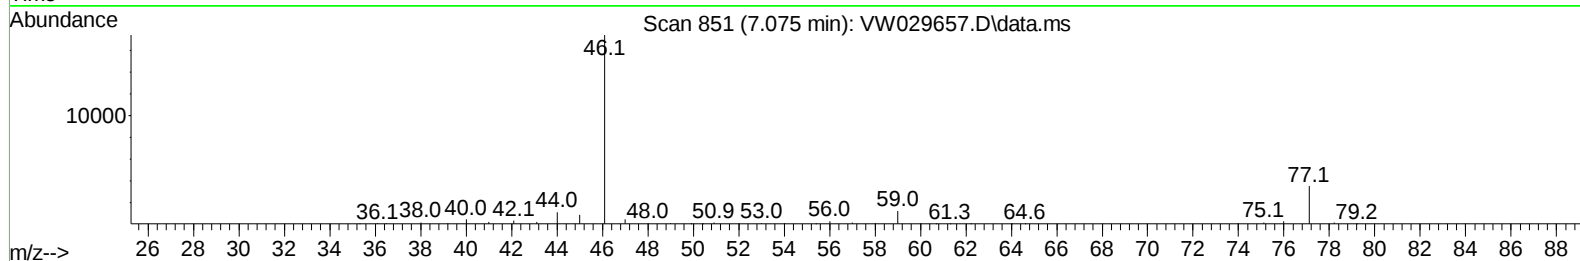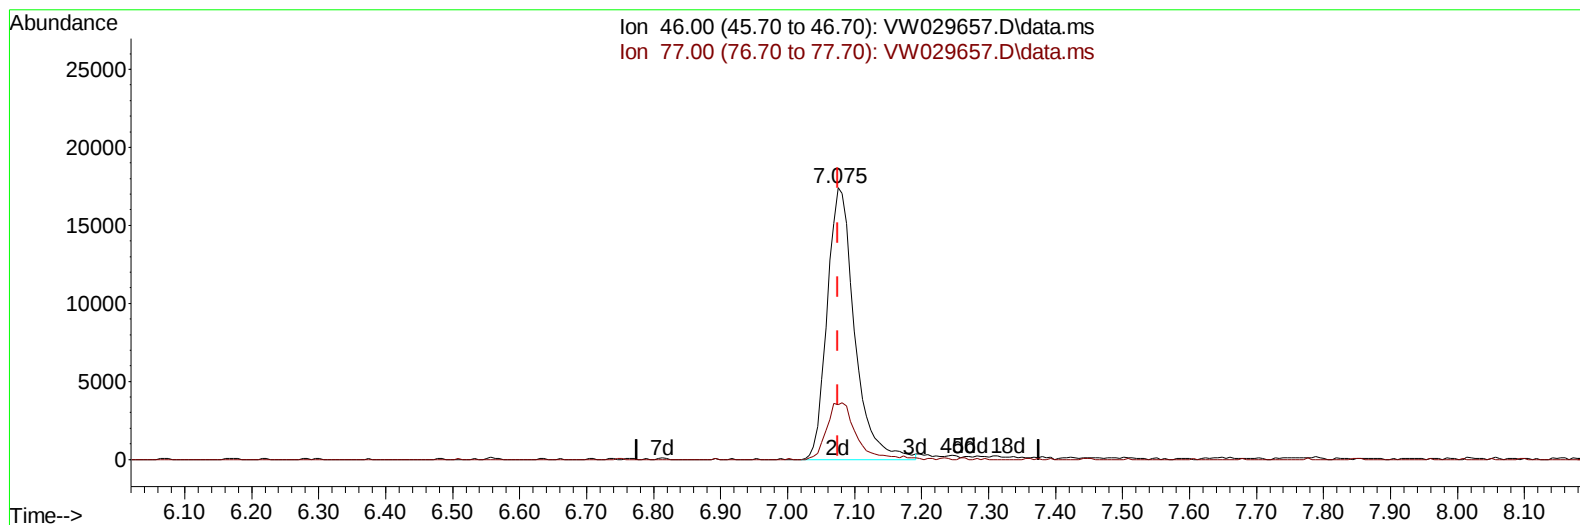

TIC: VW029657.D\data.ms

(21) 2-Butanone-d5 (S)

7.075min (+ 0.000) 22.36 ug/L m

response 49346

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	21.10	0.04#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
 Data File : VW029657.D
 Acq On : 19 Jul 2024 15:34
 Operator : SY/MD
 Sample : P3265-10
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4DA8

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:21:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 19 23:16:32 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/22/2024
 Supervised By :Mahesh Dadoda 07/24/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	455011	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	417510	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	197336	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	88176	11.996	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	48.000%	
7) Chloroethane-d5	2.899	69	71835	13.573	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	54.280%	
11) 1,1-Dichloroethene-d2	4.021	65	43850	13.285	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	53.160%	
21) 2-Butanone-d5	7.075	46	49346m	22.364	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	44.720%	
24) Chloroform-d	7.648	84	194885	14.816	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	59.280%	
26) 1,2-Dichloroethane-d4	8.307	65	111243	14.418	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	57.680%#	
32) Benzene-d6	8.270	84	372911	14.910	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	59.640%	
36) 1,2-Dichloropropane-d6	9.276	67	123903	15.494	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	61.960%#	
41) Toluene-d8	10.325	98	329213	14.967	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	59.880%	
43) trans-1,3-Dichloroprop...	10.581	79	42876	12.661	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	50.640%	
47) 2-Hexanone-d5	10.922	63	34618	23.823	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	47.640%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	86930	13.389	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	53.560%	
66) 1,2-Dichlorobenzene-d4	13.848	152	107481	15.640	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	62.560%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
Data File : VW029657.D
Acq On : 19 Jul 2024 15:34
Operator : SY/MD
Sample : P3265-10
Misc : 5.00g/10mL/MSVOA_W/SoIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4DA8

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:21:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 19 23:16:32 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/22/2024
Supervised By :Mahesh Dadoda 07/24/2024

