




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
Data File : VW029661.D
Acq On : 19 Jul 2024 17:09
Operator : SY/MD
Sample : P3263-18 RE
Misc : 5.34g/10mL/MSVOA_W/SOIL/B
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CK8RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 07/22/2024
Supervised By :Mahesh Dadoda 07/24/2024

Quant Time: Jul 19 23:22:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 19 23:16:32 2024
Response via : Initial Calibration

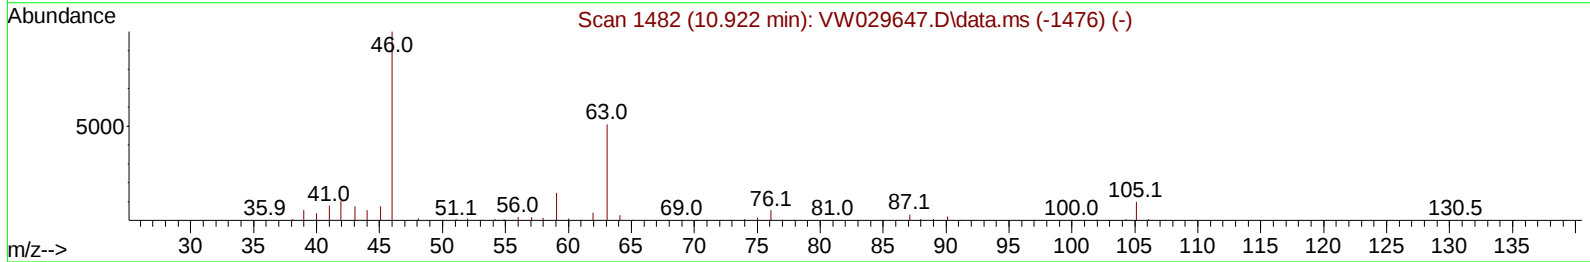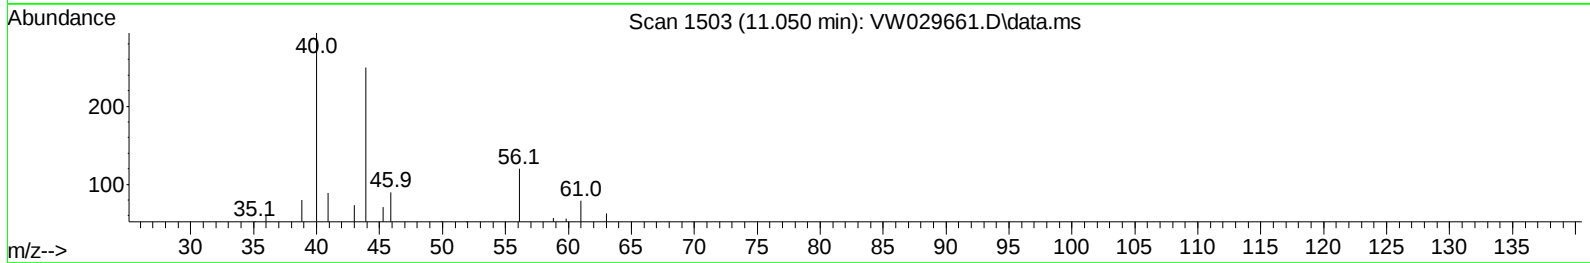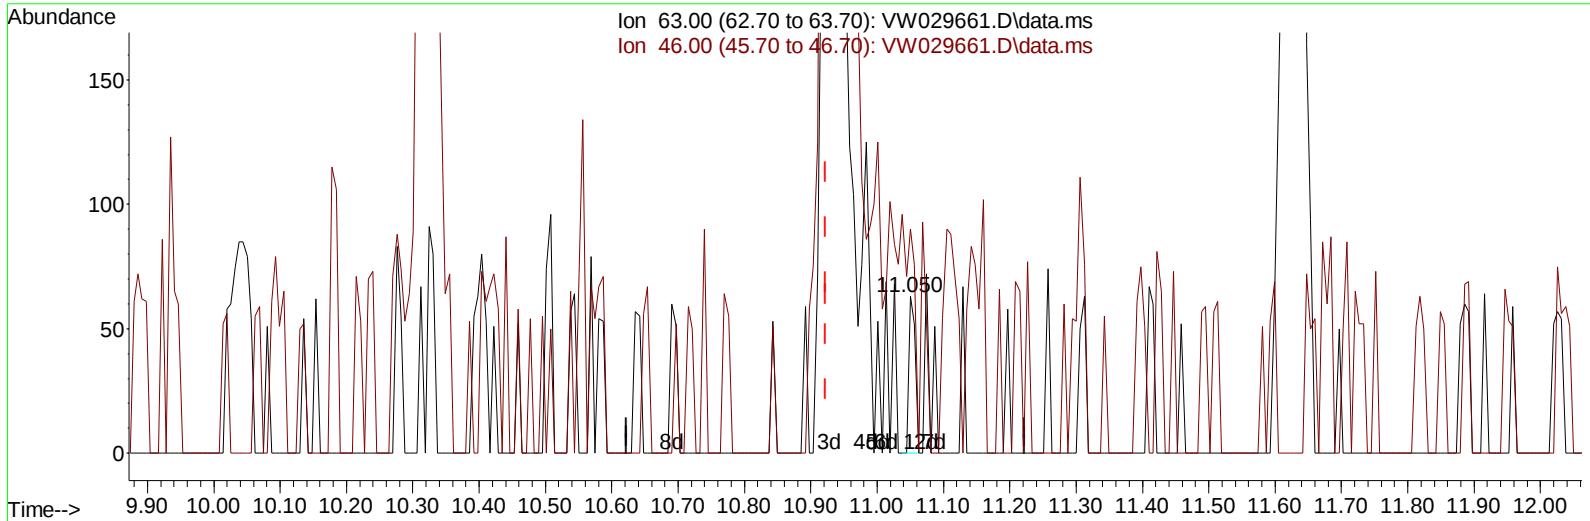

TIC: VW029661.D\data.ms

(47) 2-Hexanone-d5 (S)

11.050min (+ 0.128) 0.12 ug/L

response 42

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	190.20	145.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
 Data File : VW029661.D
 Acq On : 19 Jul 2024 17:09
 Operator : SY/MD
 Sample : P3263-18 RE
 Misc : 5.34g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CK8RE

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:22:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 19 23:16:32 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/22/2024
 Supervised By :Mahesh Dadoda 07/24/2024

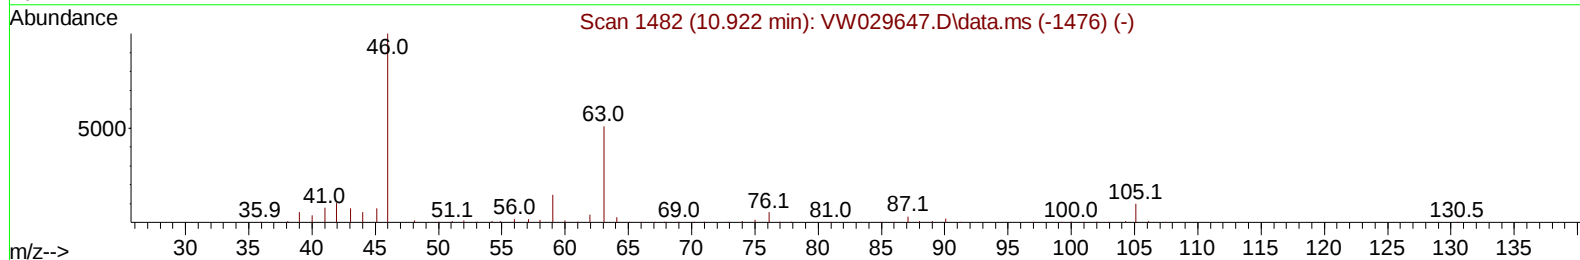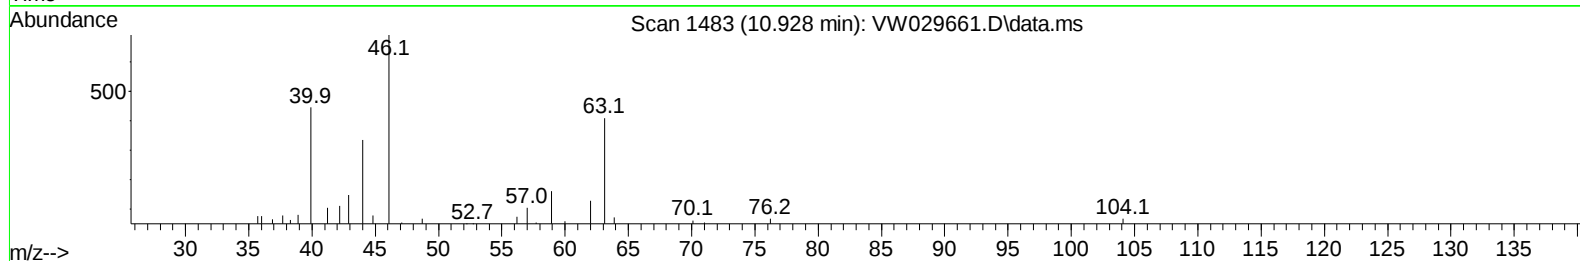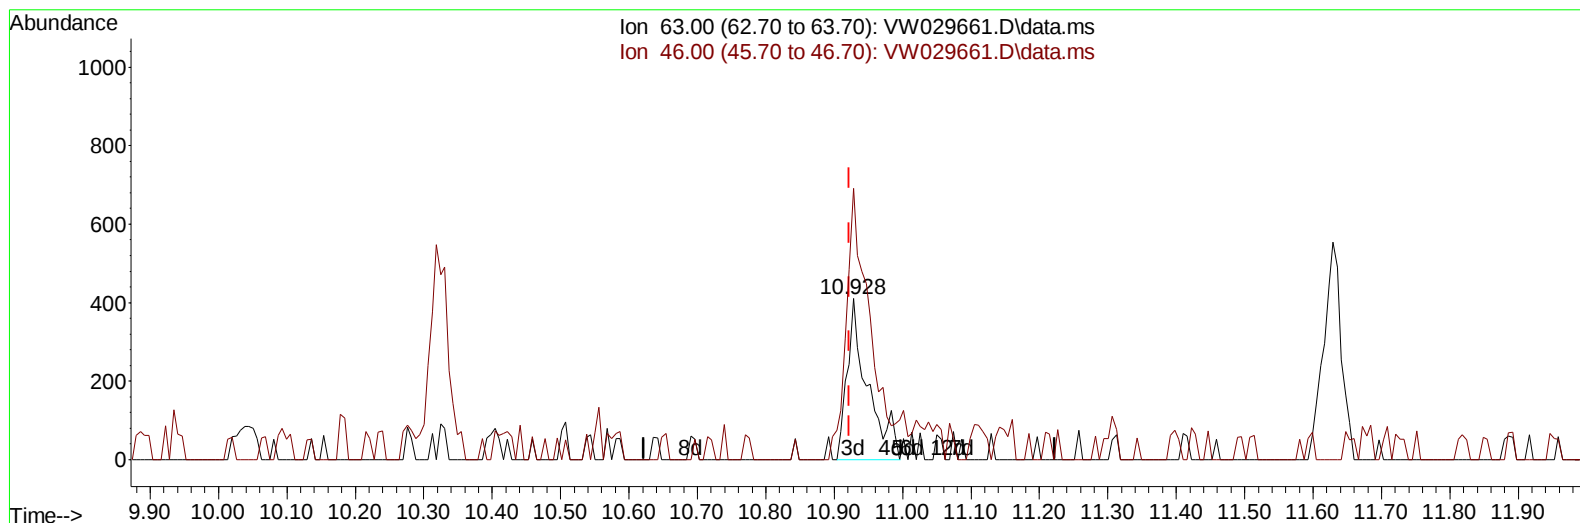

TIC: VW029661.D\data.ms

(47) 2-Hexanone-d5 (S)

10.928min (+ 0.006) 2.44 ug/L m

response 856

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	190.20	7.13#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
 Data File : VW029661.D
 Acq On : 19 Jul 2024 17:09
 Operator : SY/MD
 Sample : P3263-18 RE
 Misc : 5.34g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CK8RE

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:22:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 19 23:16:32 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/22/2024
 Supervised By :Mahesh Dadoda 07/24/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		224495	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		100714	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		18769	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		58728	16.194	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	64.760%		
7) Chloroethane-d5	2.905	69		53011	20.301	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	81.200%		
11) 1,1-Dichloroethene-d2	4.021	65		23385	14.360	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	57.440%		
21) 2-Butanone-d5	7.081	46		18544	17.034	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	34.060%		
24) Chloroform-d	7.648	84		120664	18.592	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	74.360%		
26) 1,2-Dichloroethane-d4	8.307	65		69016	18.130	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	72.520%		
32) Benzene-d6	8.276	84		130566	21.641	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	86.560%		
36) 1,2-Dichloropropane-d6	9.270	67		74543	38.642	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	154.560%#		
41) Toluene-d8	10.319	98		66223	12.481	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	49.920%		
43) trans-1,3-Dichloroprop...	10.581	79		2744	3.359	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	13.440%#		
47) 2-Hexanone-d5	10.928	63		856m	2.442	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	4.880%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		35594	22.726	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	90.920%		
66) 1,2-Dichlorobenzene-d4	13.848	152		10353	15.839	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	63.360%#		
Target Compounds							
						Qvalue	
13) Acetone	4.119	43		11856	10.790	ug/L	96
16) Methylene chloride	4.923	84		19015	4.731	ug/L	99
46) Tetrachloroethene	10.861	164		853	0.722	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071924\
Data File : VW029661.D
Acq On : 19 Jul 2024 17:09
Operator : SY/MD
Sample : P3263-18 RE
Misc : 5.34g/10mL/MSVOA_W/SOIL/B
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CK8RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 07/22/2024
Supervised By :Mahesh Dadoda 07/24/2024

Quant Time: Jul 19 23:22:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 19 23:16:32 2024
Response via : Initial Calibration

