

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW072019\
 Data File : VW011397.D
 Acq On : 20 Jul 2019 02:11
 Operator : SY/VA
 Sample : K3835-46
 Misc : 5.41G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SB-8(4-6)

Quant Time: Jul 20 06:47:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070819S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 11 08:14:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	271168	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	466318	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	387198	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	159243	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	182874	53.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.34%	
35) Dibromofluoromethane	7.88	113	143335	51.57	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.14%	
50) Toluene-d8	10.32	98	575971	51.27	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.54%	
62) 4-Bromofluorobenzene	12.62	95	195476	47.47	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.94%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW072019\
Data File : VW011397.D
Acq On : 20 Jul 2019 02:11
Operator : SY/VA
Sample : K3835-46
Misc : 5.41G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SB-8(4-6)

Quant Time: Jul 20 06:47:31 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070819S.M
Quant Title : SW846 8260
QLast Update : Thu Jul 11 08:14:17 2019
Response via : Initial Calibration

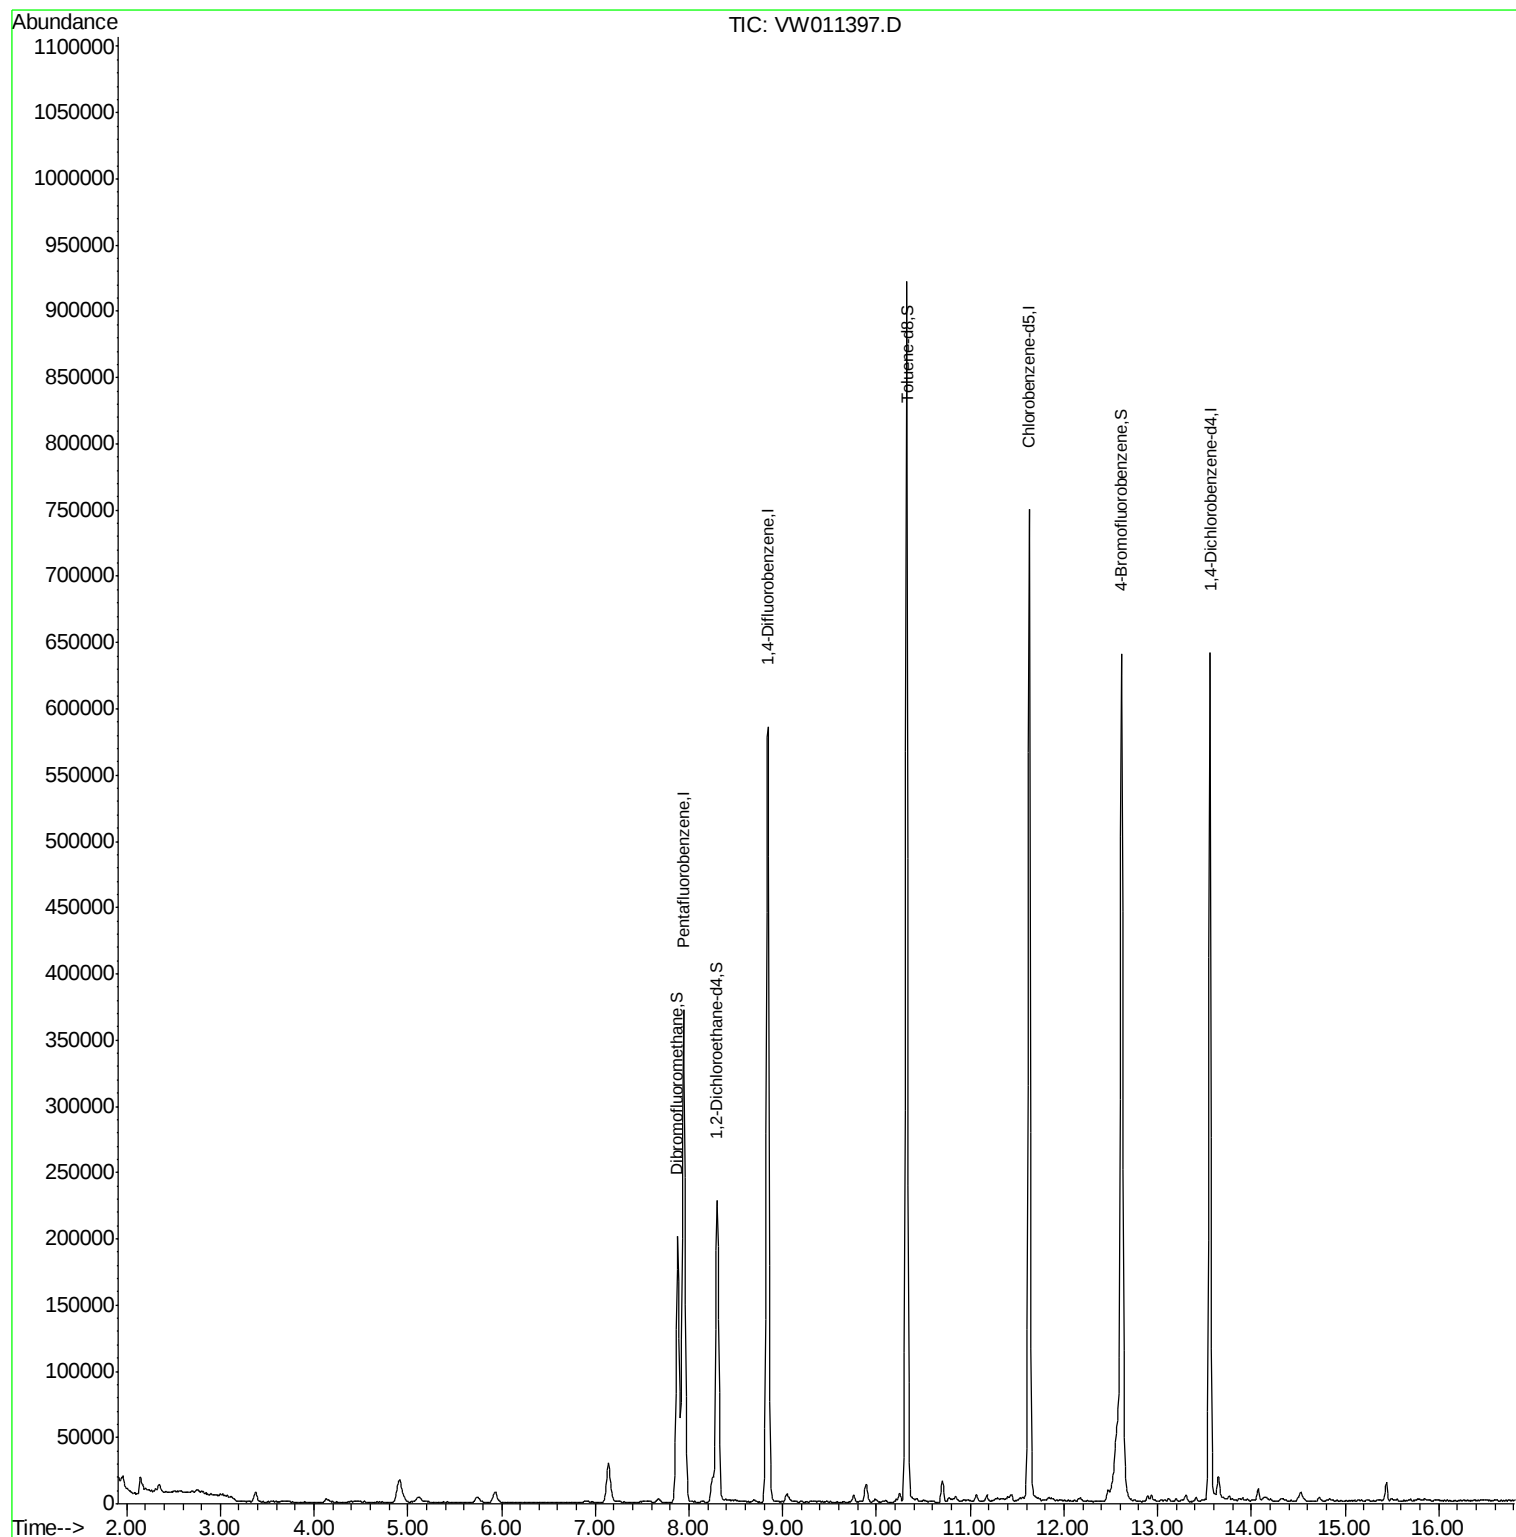

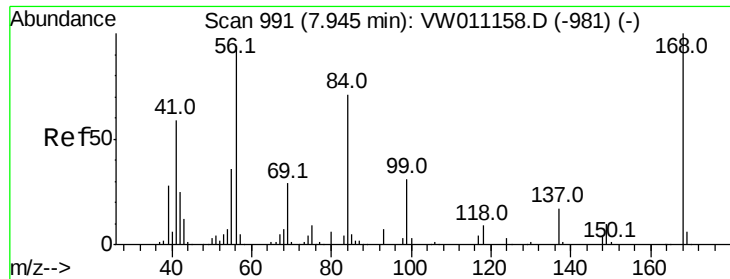

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW011397.D

Acq: 20 Jul 2019 02:11

Instrument :

MSVOA_W

ClientSampled :


SB-8(4-6)

Tot Ion:168 Resp: 271168

Ion Ratio Lower Upper

168 100

99 59.4 50.1 75.1

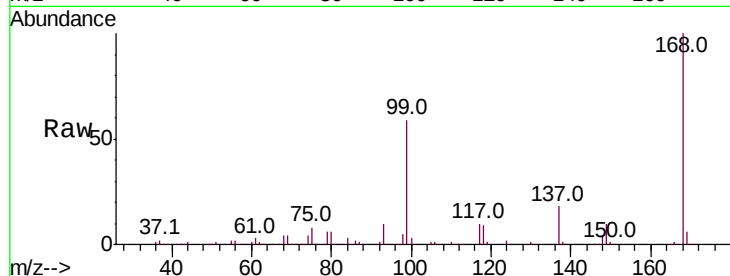

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95



100000

50000

0

Time-->

7.80 7.90 8.00 8.10

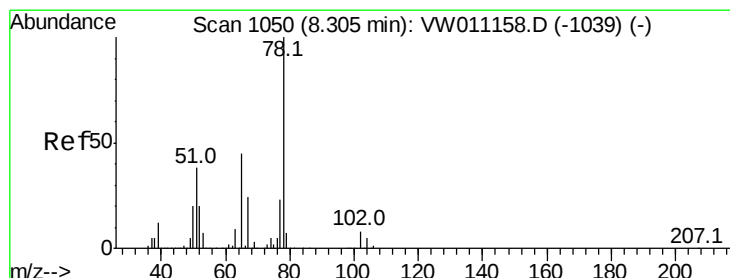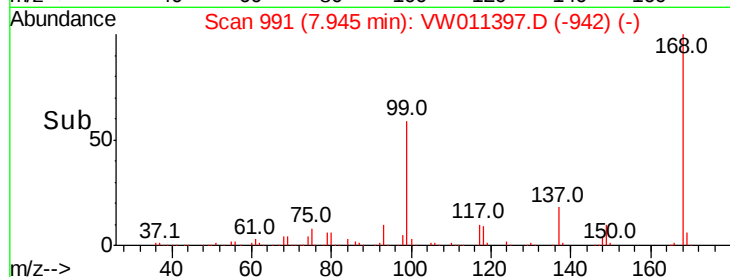

#33

1,2-Dichloroethane-d4

Concen: 53.671 ug/l

RT: 8.30 min Scan# 1049

Delta R.T. -0.01 min

Lab File: VW011397.D


Acq: 20 Jul 2019 02:11

Tgt Ion: 65 Resp: 182874

Ion Ratio Lower Upper

65 100

67 51.8 0.0 104.4

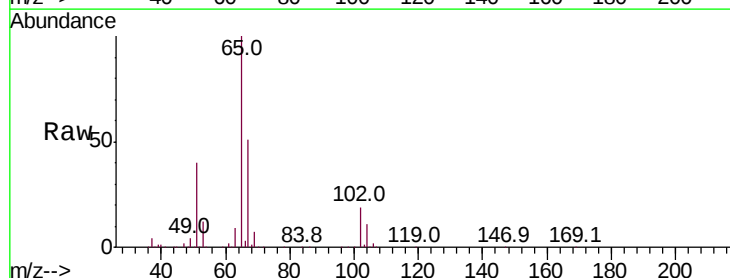

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.30

100000

80000

60000


40000


20000

0

Time-->

8.20 8.30 8.40

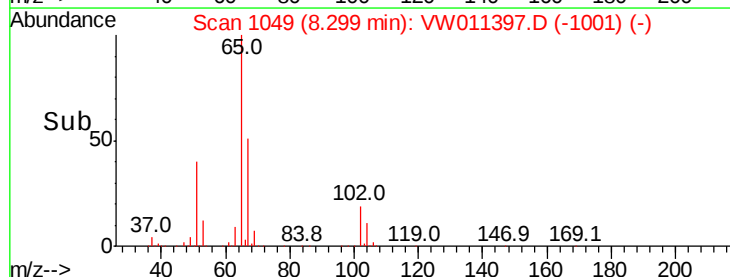


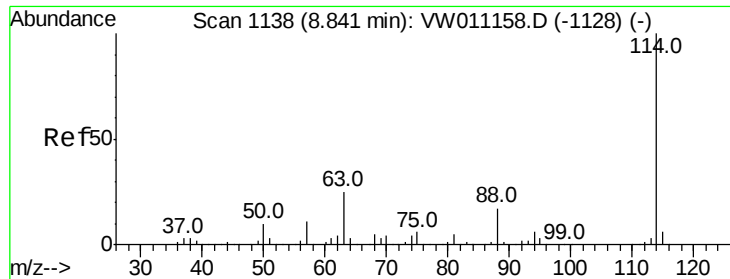




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW011397.D
 Acq: 20 Jul 2019 02:11

Instrument :
 MSVOA_W
 ClientSampleId :
 SB-8(4-6)

Tot Ion	Ratio	Lower	Upper
114	100		
63	24.4	0.0	50.8
88	16.4	0.0	34.2

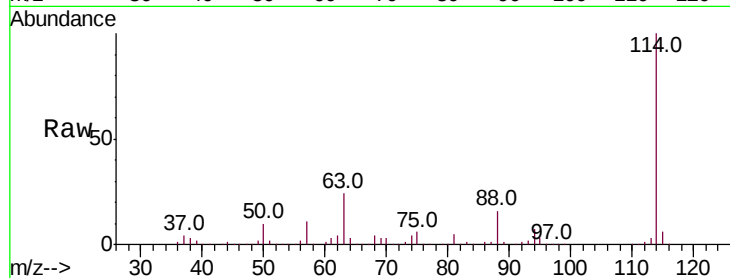


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

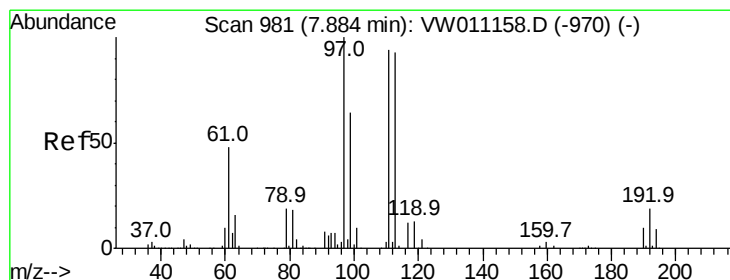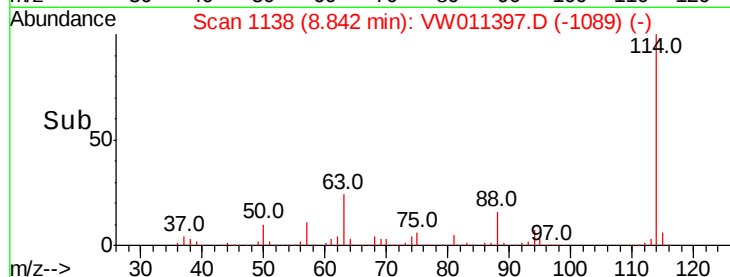
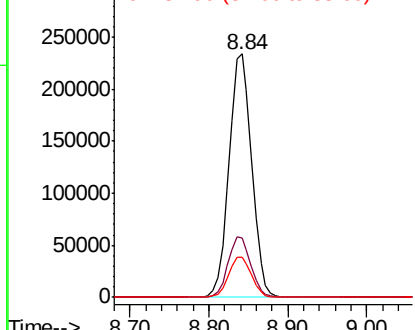



#35
 Dibromofluoromethane
 Concen: 51.569 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. 0.00 min
 Lab File: VW011397.D
 Acq: 20 Jul 2019 02:11

Tgt Ion	Ratio	Lower	Upper
113	100		
111	104.5	82.4	123.6
192	20.3	15.8	23.8

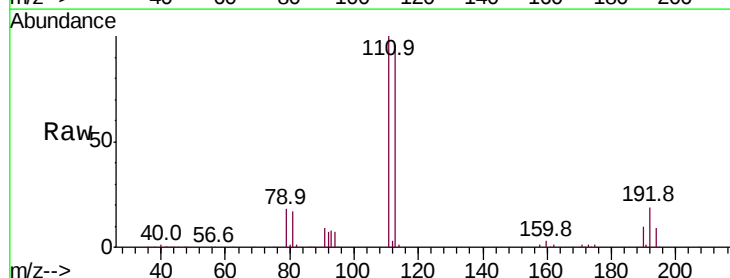

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

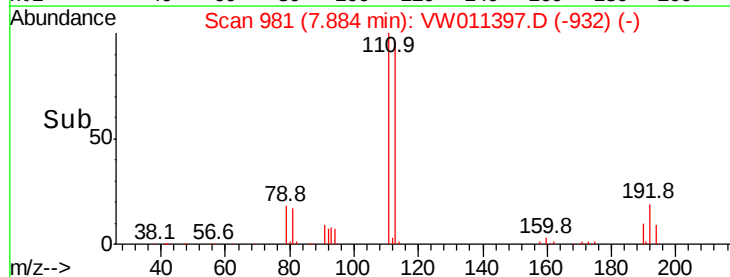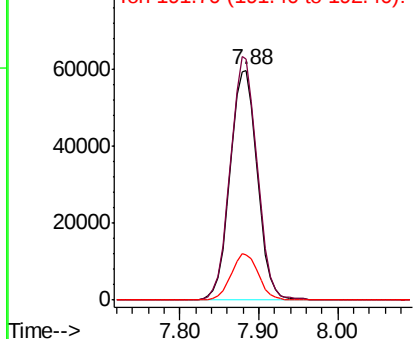

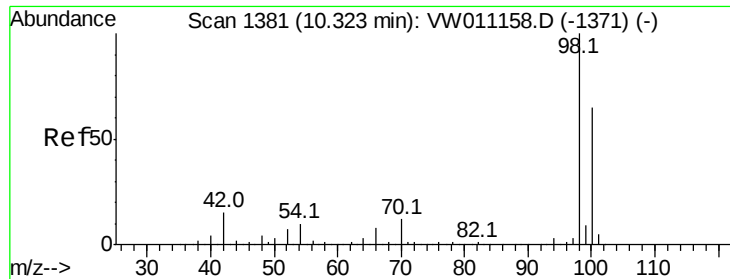

#50

Toluene-d8

Concen: 51.266 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW011397.D

Acq: 20 Jul 2019 02:11

Instrument :

MSVOA_W

ClientSampleId :


SB-8(4-6)

Tot Ion: 98 Resp: 575971

Ion Ratio Lower Upper




98 100

100 65.3 52.4 78.6

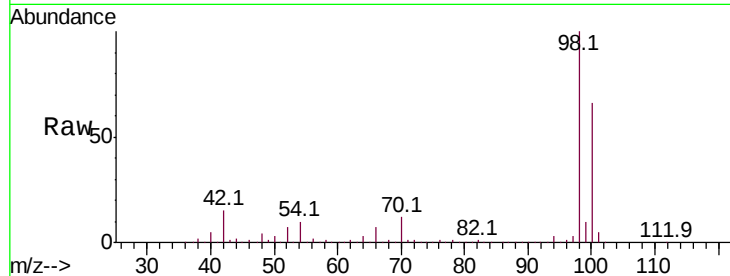

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

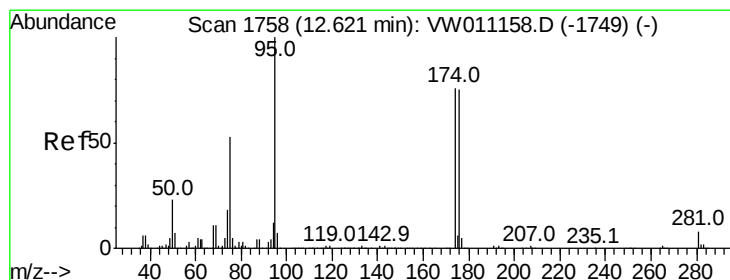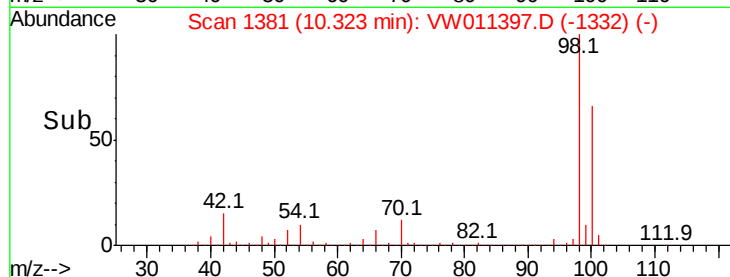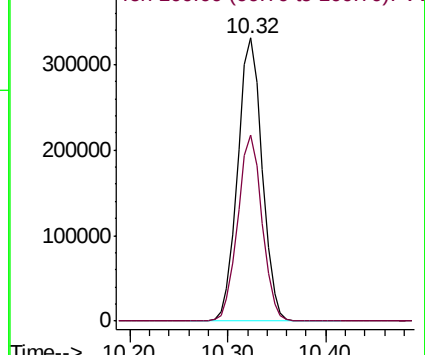

#62

4-Bromofluorobenzene

Concen: 47.468 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. -0.01 min

Lab File: VW011397.D

Acq: 20 Jul 2019 02:11


Tgt Ion: 95 Resp: 195476

Ion Ratio Lower Upper

95 100

174 72.5 0.0 147.6



176 70.6 0.0 144.6

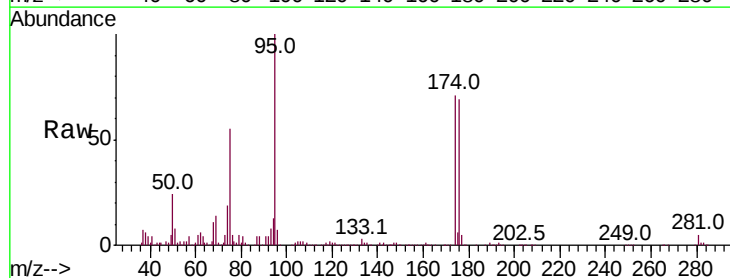


Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



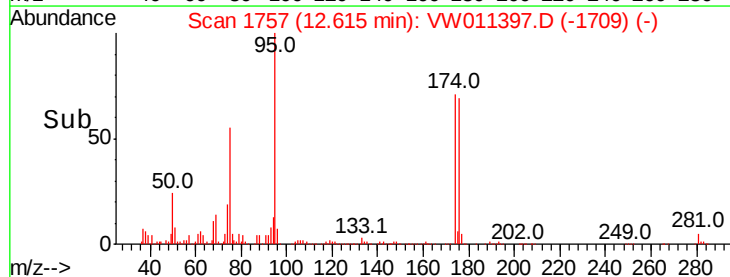
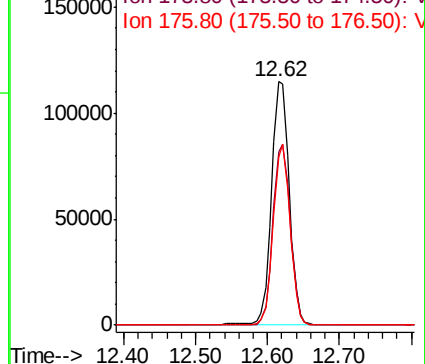


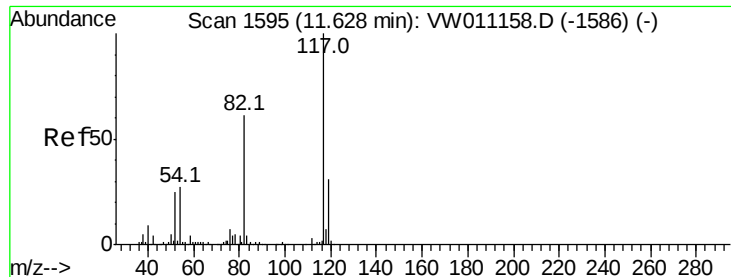

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.01 min
Lab File: VW011397.D
Acq: 20 Jul 2019 02:11

Instrument :
MSVOA_W
ClientSampleId :
SB-8(4-6)

Tot Ion:117 Resp: 387198
Ion Ratio Lower Upper
117 100
82 59.8 48.9 73.3
119 32.8 25.0 37.6

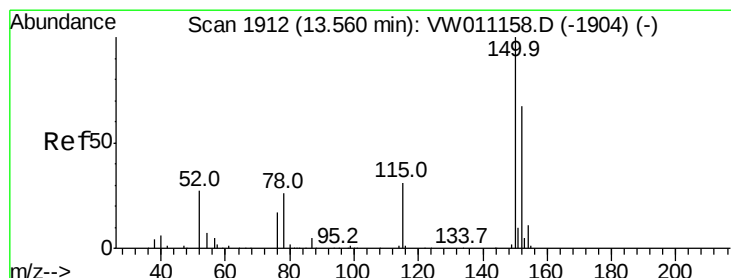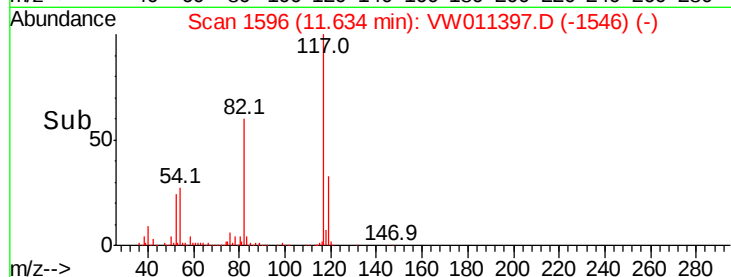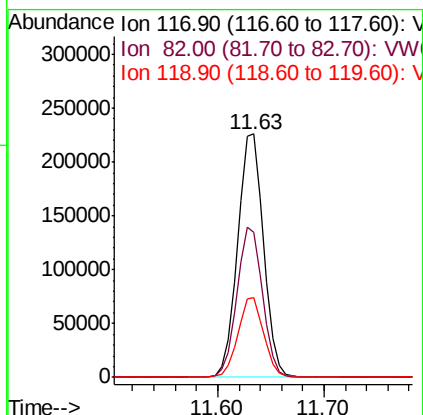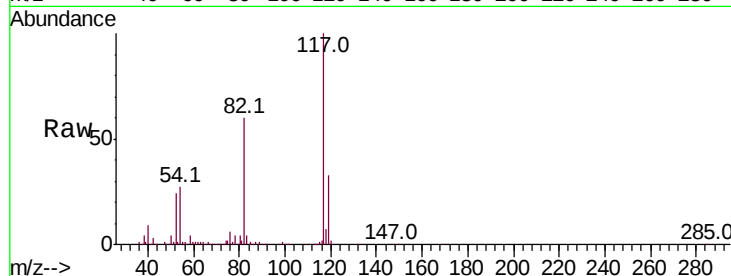

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. 0.00 min
Lab File: VW011397.D
Acq: 20 Jul 2019 02:11

Tgt Ion:152 Resp: 159243
Ion Ratio Lower Upper
152 100
115 59.7 30.1 90.3
150 156.3 0.0 346.0

