

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW072118\
 Data File : VW004123.D
 Acq On : 21 Jul 2018 19:16
 Operator : SY/AP
 Sample : J4065-05
 Misc : 4.39G/10ML/MSVOA_W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JHT34

Quant Time: Jul 23 00:05:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071818S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 21 06:22:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	266238	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	262799	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	114247	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	47627	18.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.32%
7) Chloroethane-d5	2.89	69	36515	19.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.96%
10) 1,1-Dichloroethene-d2	4.01	63	87861	13.91	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.64%
20) 2-Butanone-d5	7.08	46	68598	44.42	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.84%
24) Chloroform-d	7.65	84	143635	22.73	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.92%
26) 1,2-Dichloroethane-d4	8.31	65	93575	24.59	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.36%
29) Benzene-d6	8.27	84	246511	20.22	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.88%
33) 1,2-Dichloropropane-d6	9.28	67	93791	23.07	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.28%
37) Toluene-d8	10.33	98	206914	18.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.56%
38) trans-1,3-Dichloropropene-	10.59	79	36938	20.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.68%
39) 2-Hexanone-d5	10.93	63	43199	39.47	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.94%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	106187	23.84	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.36%
61) 1,2-Dichlorobenzene-d4	13.87	152	88485	24.09	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.36%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
40) 1,2-Dichloropropane	9.27	63	10305	2.360	ug/L	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW072118\
Data File : VW004123.D
Acq On : 21 Jul 2018 19:16
Operator : SY/AP
Sample : J4065-05
Misc : 4.39G/10ML/MSVOA_W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JHT34

Quant Time: Jul 23 00:05:28 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071818S.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 21 06:22:08 2018
Response via : Initial Calibration

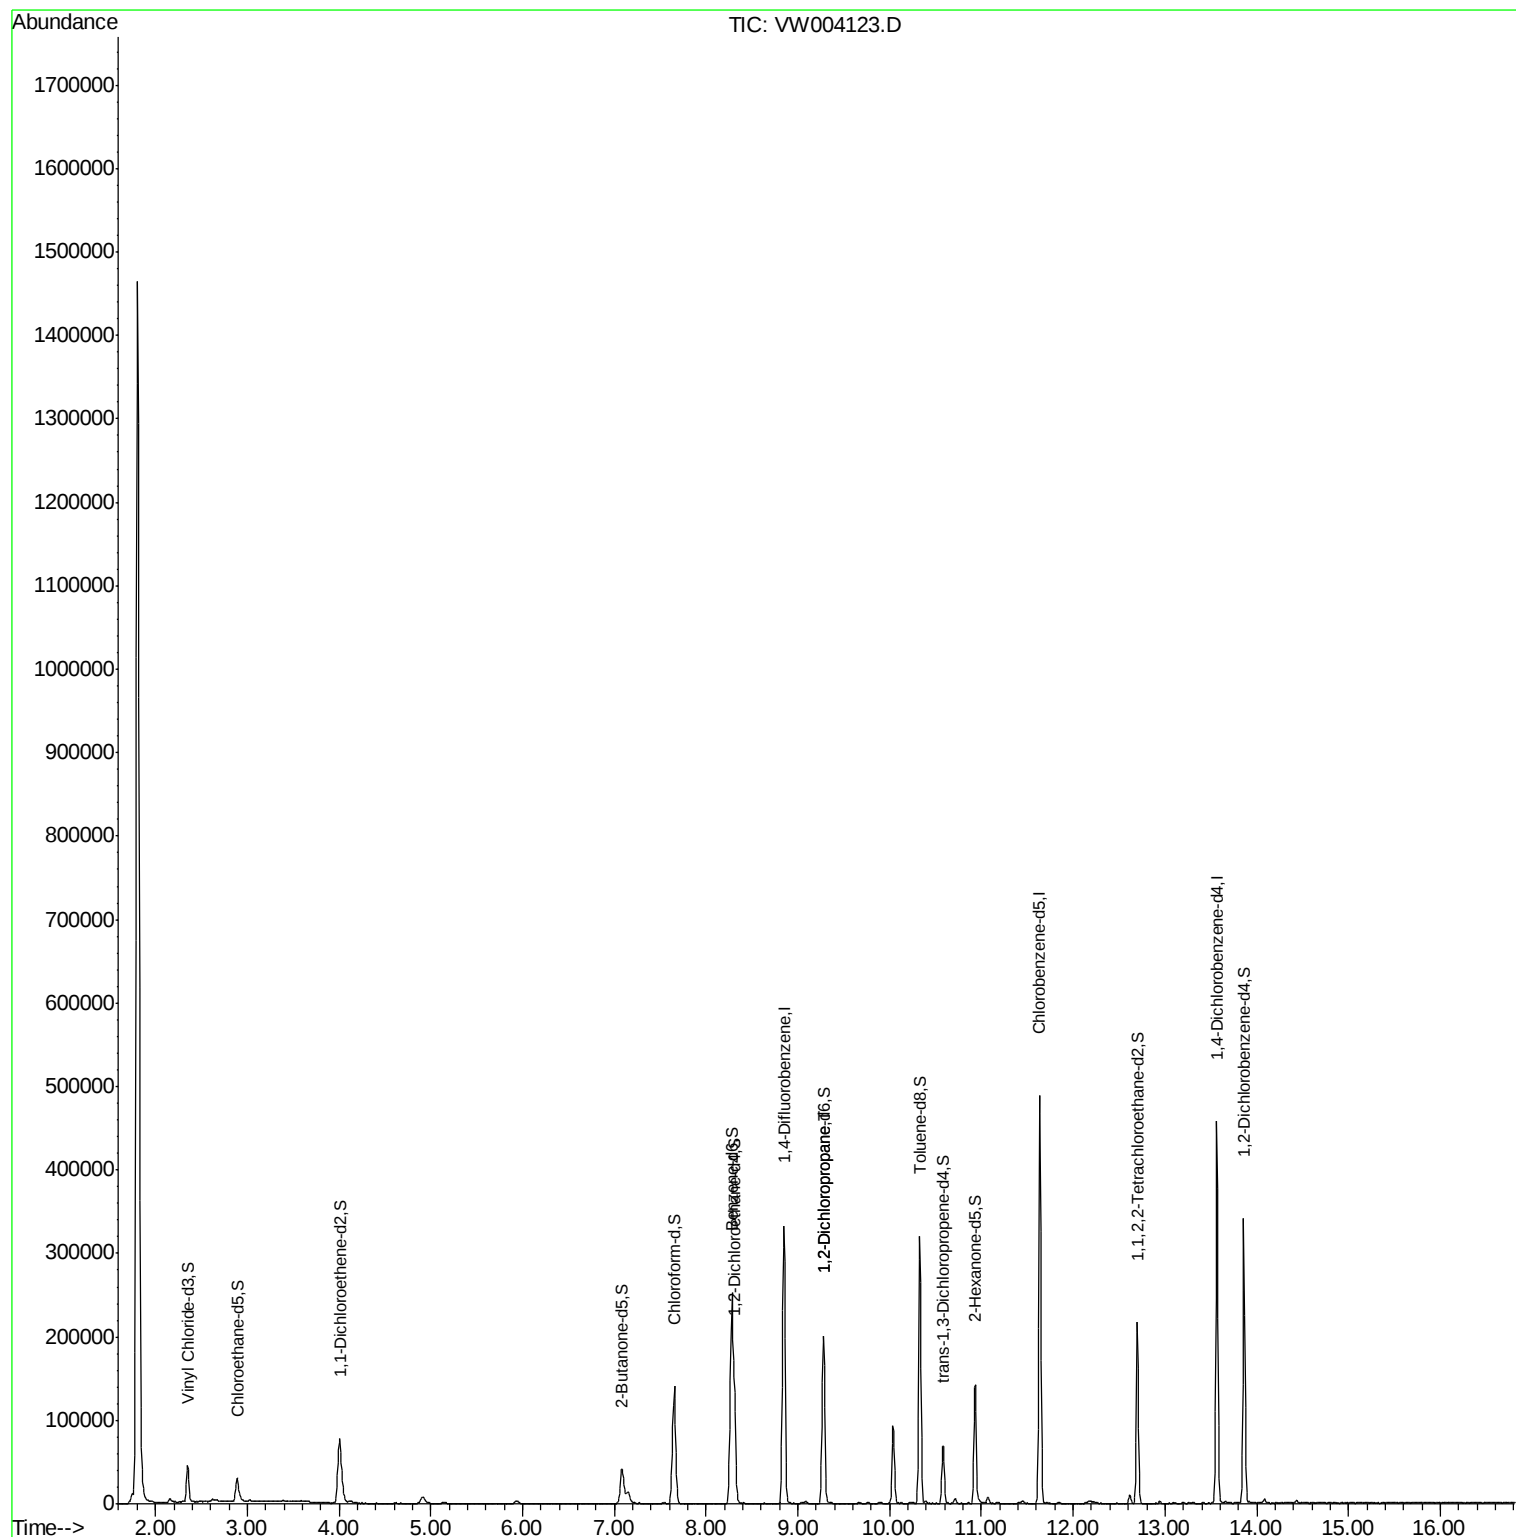

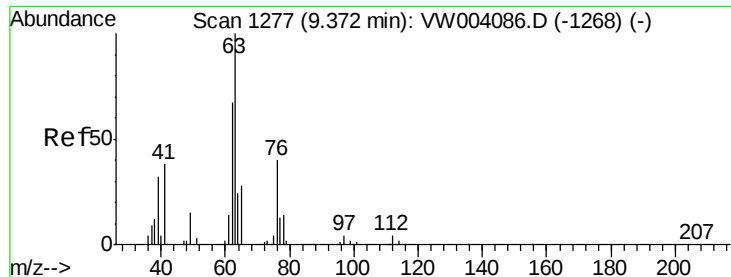

#40
 1,2-Dichloropropane
 Concen: 2.360 ug/L
 RT: 9.27 min Scan# 1261
 Delta R.T. -0.10 min
 Lab File: VW004123.D
 Acq: 21 Jul 2018 19:16

Instrument :
 MSVOA_W
 ClientSampleId :
 JHT34

Tgt Ion: 63 Resp: 10305
 Ion Ratio Lower Upper
 63 100
 112 0.5 3.0 4.4#

