

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW072118\
 Data File : VW004125.D
 Acq On : 21 Jul 2018 20:08
 Operator : SY/AP
 Sample : J4065-02
 Misc : 4.91G/10ML/MSVOA_W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JHT31

Quant Time: Jul 23 00:05:36 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071818S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 21 06:22:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	214331	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	195882	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	64116	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	39098	18.44	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.76%
7) Chloroethane-d5	2.89	69	29432	19.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.04%
10) 1,1-Dichloroethene-d2	4.00	63	68741	13.52	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.08%
20) 2-Butanone-d5	7.08	46	45405	36.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.04%
24) Chloroform-d	7.65	84	114437	22.50	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.00%
26) 1,2-Dichloroethane-d4	8.31	65	73427	23.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.84%
29) Benzene-d6	8.28	84	189605	20.87	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.48%
33) 1,2-Dichloropropane-d6	9.28	67	72850	24.04	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.16%
37) Toluene-d8	10.33	98	146925	17.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.96%
38) trans-1,3-Dichloropropene-	10.58	79	25911	19.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.84%
39) 2-Hexanone-d5	10.93	63	31463	38.57	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.14%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	81825	24.65	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.60%
61) 1,2-Dichlorobenzene-d4	13.87	152	47598	23.09	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.36%


Target Compounds					Qvalue
36) Methylcyclohexane	9.28	83	17327	3.263 ug/L #	17
40) 1,2-Dichloropropane	9.27	63	8262	2.538 ug/L #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW072118\
Data File : VW004125.D
Acq On : 21 Jul 2018 20:08
Operator : SY/AP
Sample : J4065-02
Misc : 4.91G/10ML/MSVOA_W/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JHT31

Quant Time: Jul 23 00:05:36 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM071818S.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 21 06:22:08 2018
Response via : Initial Calibration




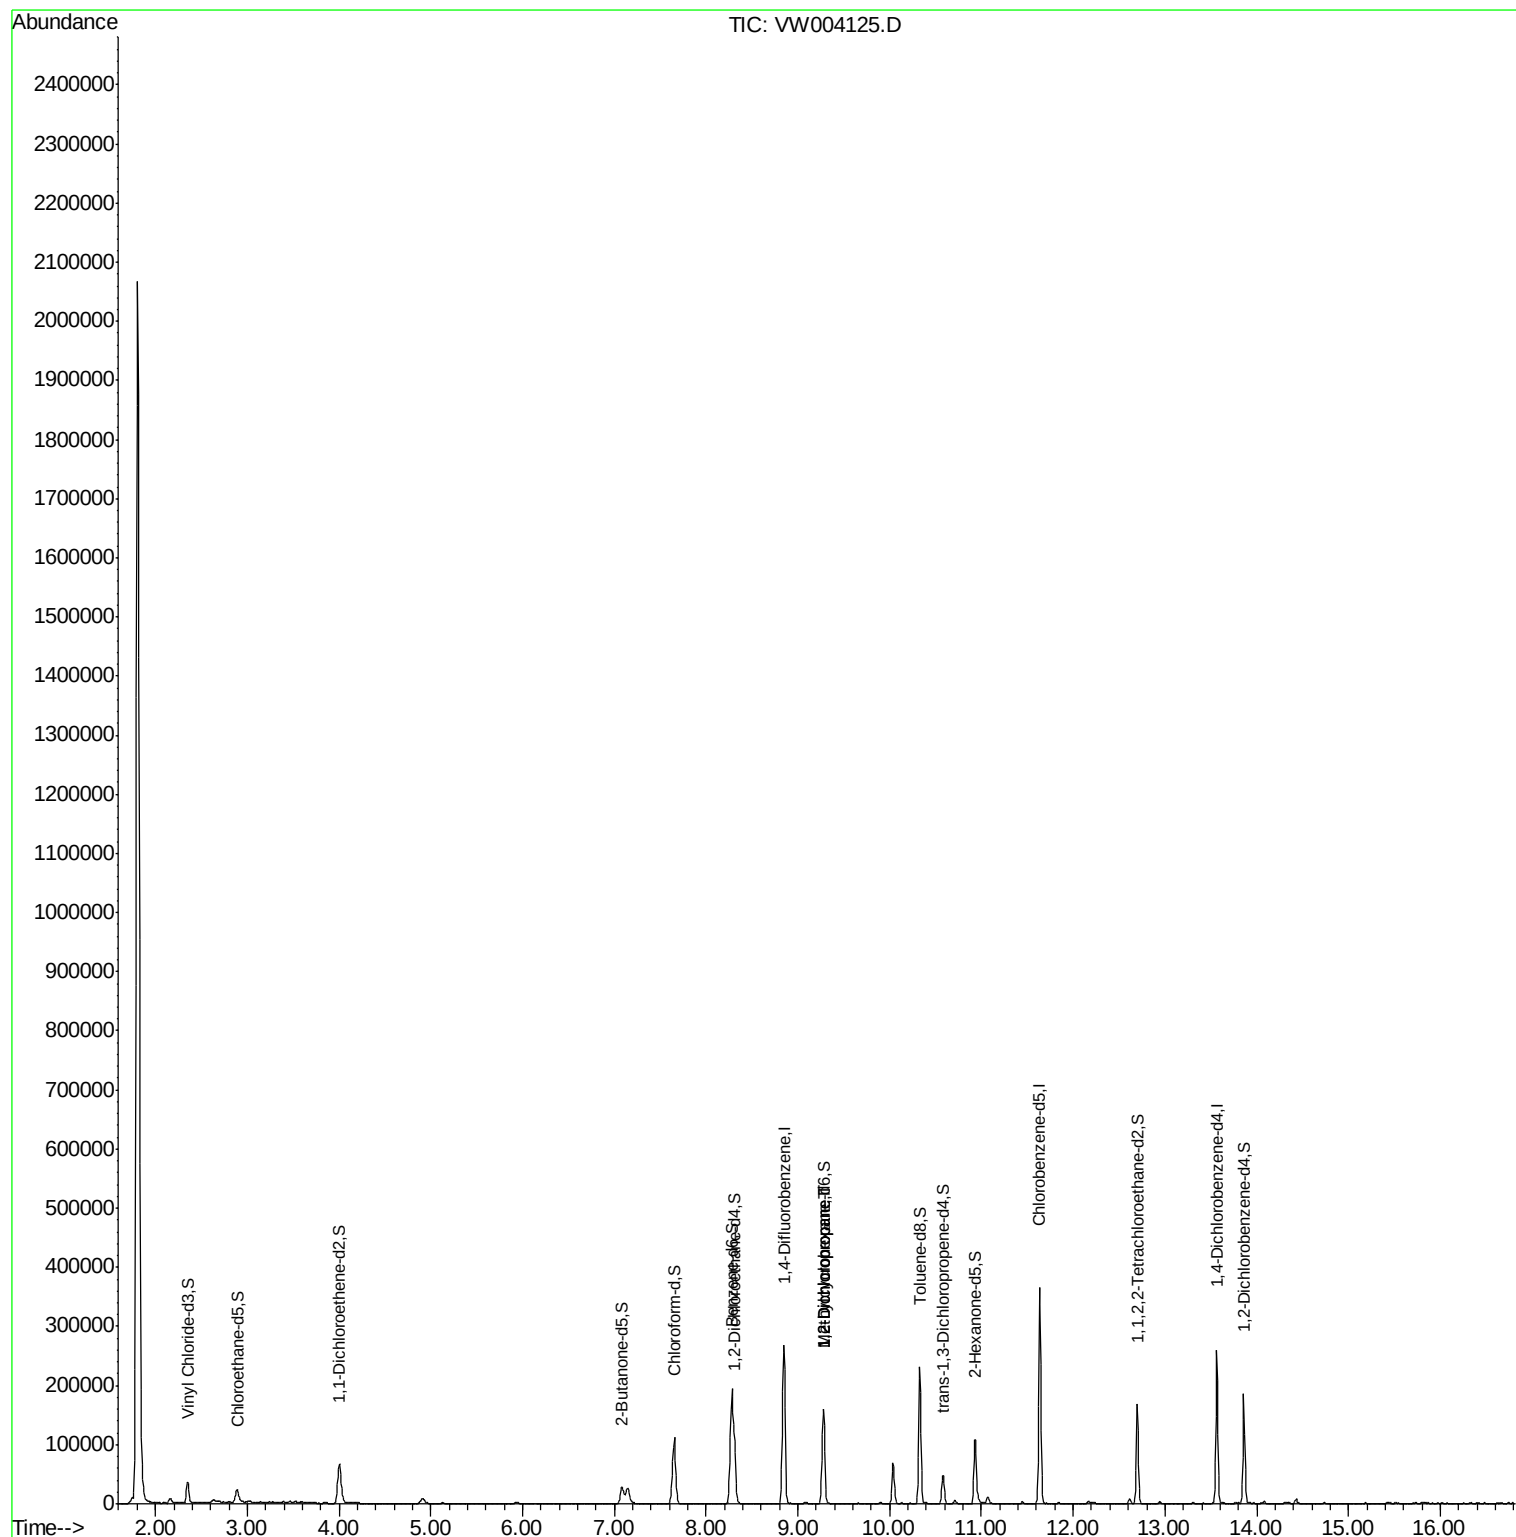


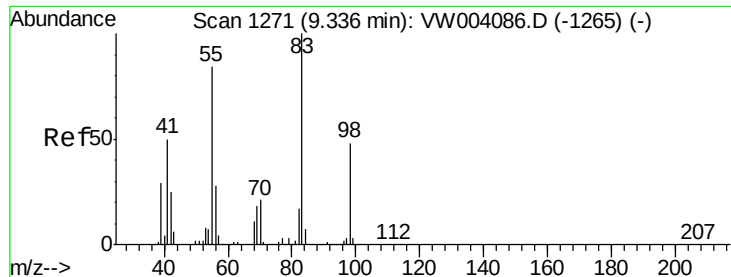

#36
Methylcyclohexane
Concen: 3.263 ug/L
RT: 9.28 min Scan# 1262
Delta R.T. -0.05 min
Lab File: VW004125.D
Acq: 21 Jul 2018 20:08

Instrument :
MSVOA_W
ClientSampleId :
JHT31

Tgt Ion: 83 Resp: 17327
Ion Ratio Lower Upper
83 100
55 0.1 65.8 98.6#
98 2.0 37.0 55.6#

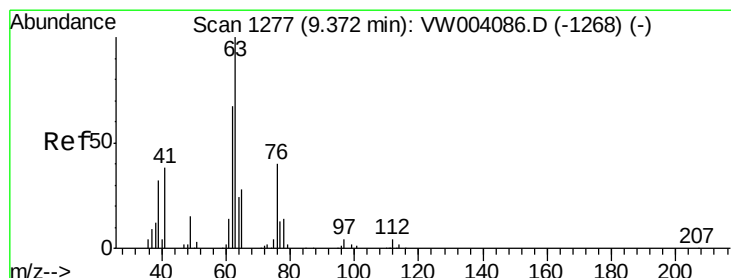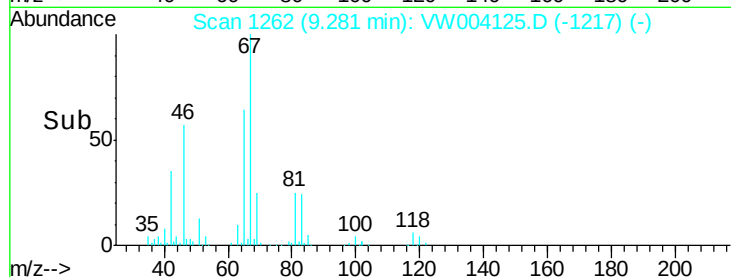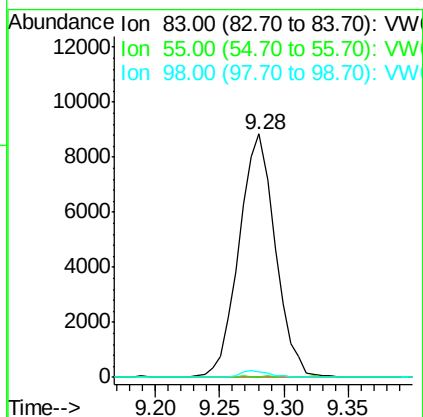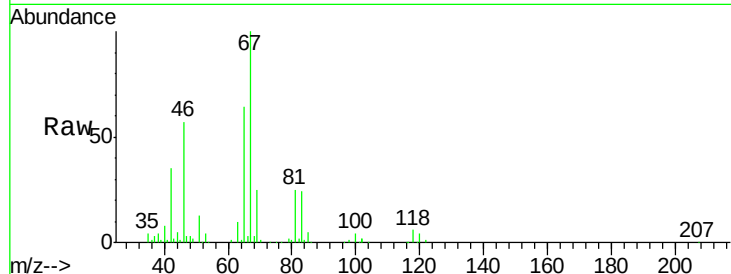

#40
1,2-Dichloropropane
Concen: 2.538 ug/L
RT: 9.27 min Scan# 1261
Delta R.T. -0.10 min
Lab File: VW004125.D
Acq: 21 Jul 2018 20:08

Tgt Ion: 63 Resp: 8262
Ion Ratio Lower Upper
63 100
112 0.6 3.0 4.4#

